

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022724\
 Data File : VW034449.D
 Acq On : 27 Feb 2024 15:11
 Operator : SY/MD
 Sample : P1566-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD0

Quant Time: Feb 28 03:57:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 28 03:52:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	135044	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	128071	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	65181	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	32731	4.175	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.600%
7) Chloroethane-d5	1.532	69	30377	4.388	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.060	65	16540	4.533	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	90.600%
20) 2-Butanone-d5	3.796	46	118982	58.052	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.100%
24) Chloroform-d	4.252	84	75104	4.772	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
26) 1,2-Dichloroethane-d4	4.947	65	43501	5.431	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.600%
32) Benzene-d6	4.963	84	136892	4.751	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	5.992	67	44090	5.125	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.600%
41) Toluene-d8	7.246	98	117185	4.536	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	7.561	79	14061	4.388	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.800%
46) 2-Hexanone-d5	8.024	63	97352	53.723	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	107.440%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	35518	5.216	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	51315	5.182	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.600%
Target Compounds						
					Qvalue	
13) Acetone	2.124	43	59039	28.321	ug/L	99
16) Methylene chloride	2.449	84	3937	0.408	ug/L #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034449.D
Acq On : 27 Feb 2024 15:11
Operator : SY/MD
Sample : P1566-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD0

Quant Time: Feb 28 03:57:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 28 03:52:36 2024
Response via : Initial Calibration

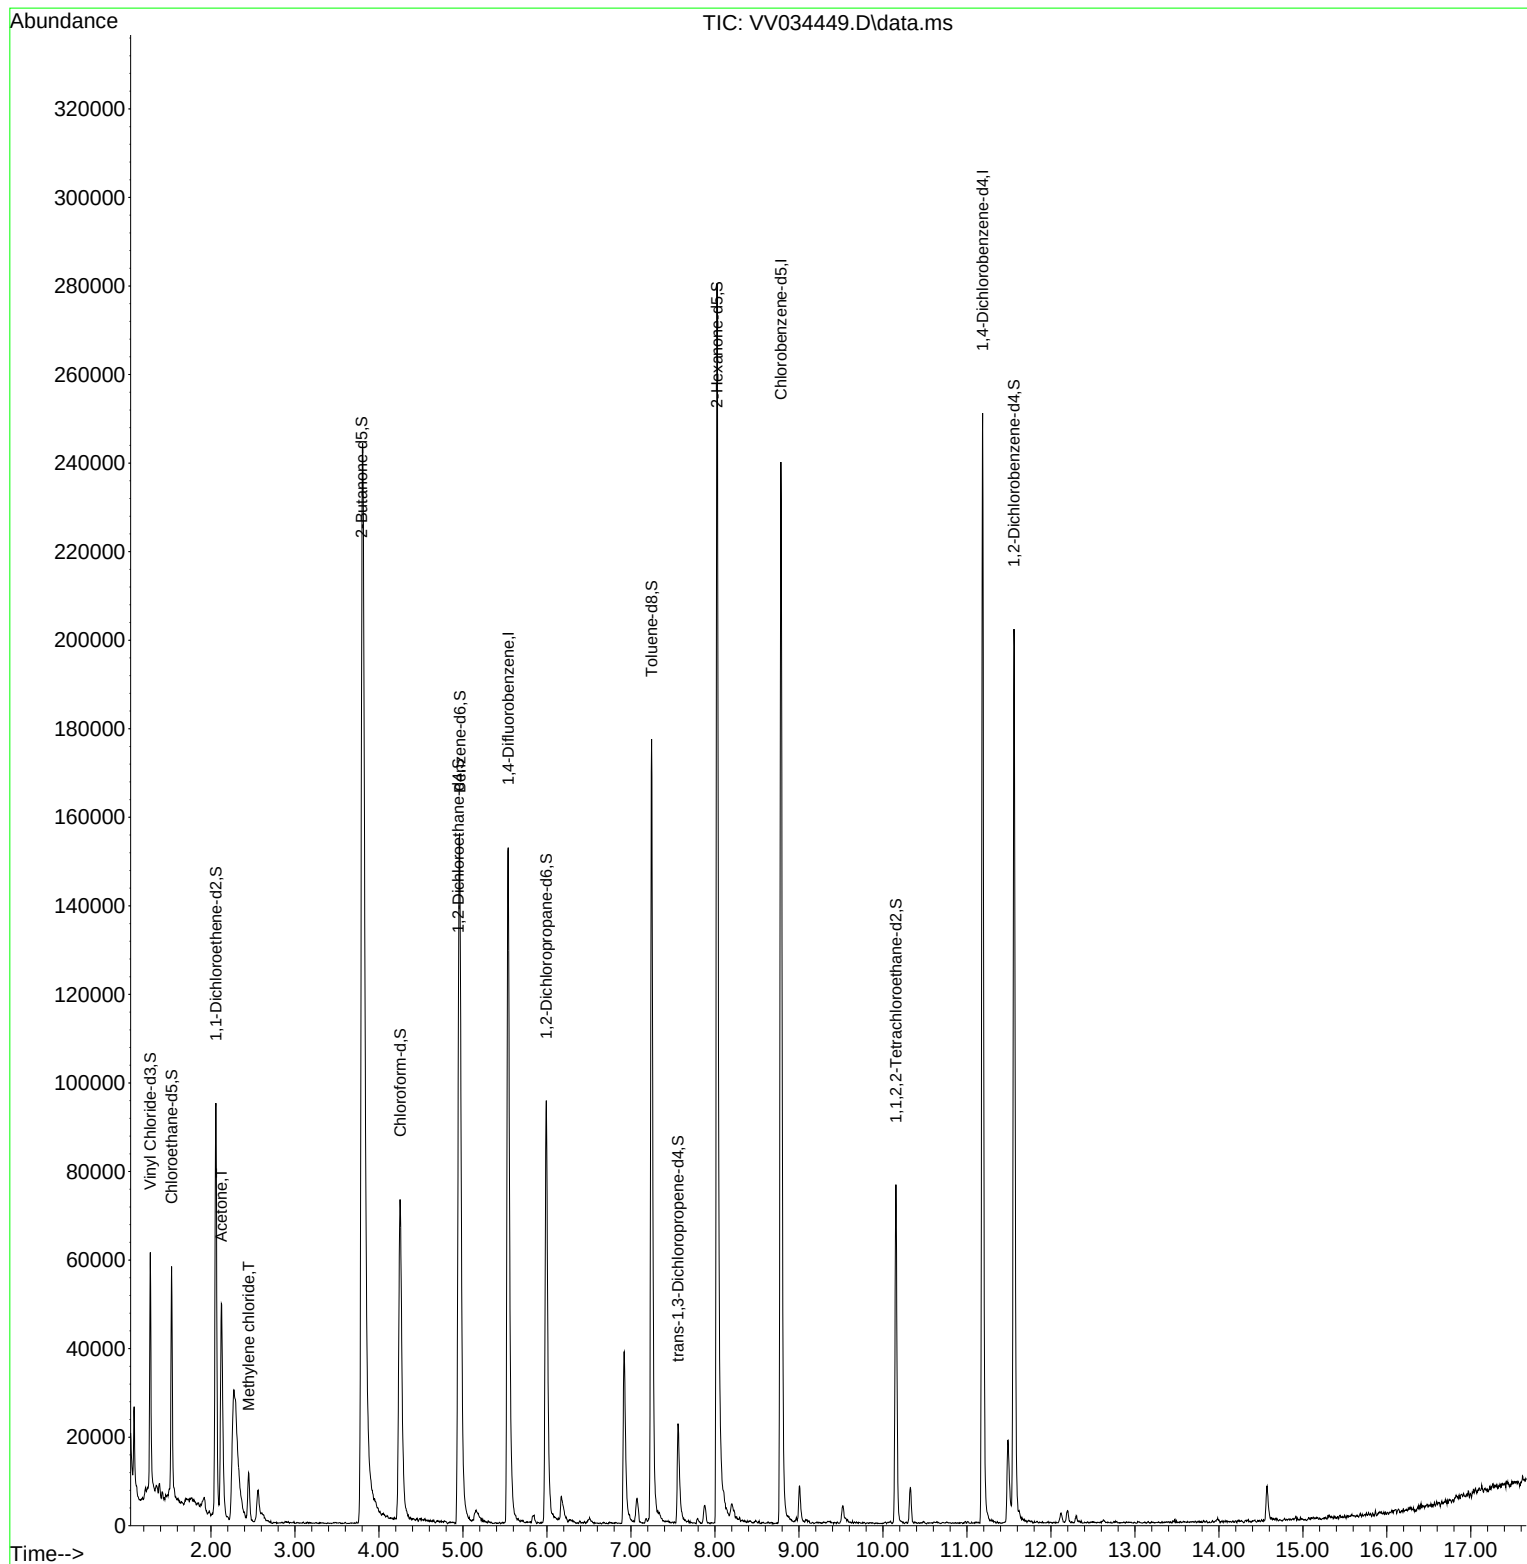

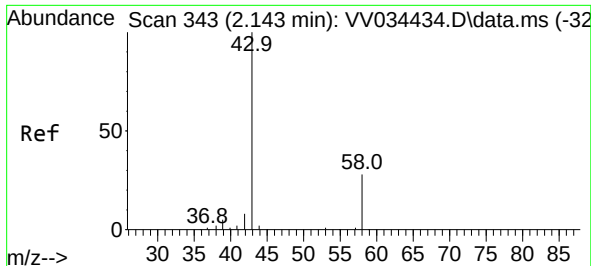

#13

Acetone

Concen: 28.321 ug/L

RT: 2.124 min Scan# 31

Delta R.T. -0.019 min

Lab File: VV034449.D

Acq: 27 Feb 2024 15:11

Instrument :

MSVOA_V

ClientSampleId :





JWAD0

Tgt Ion: 43 Resp: 59039

Ion Ratio Lower Upper

43 100

58 28.8 0.0 56.2

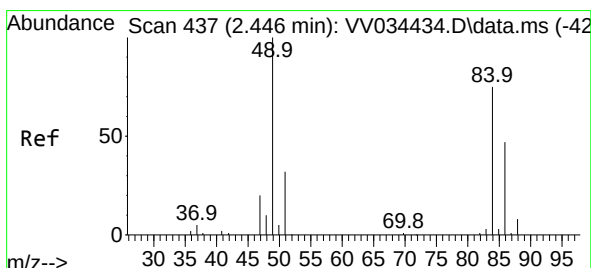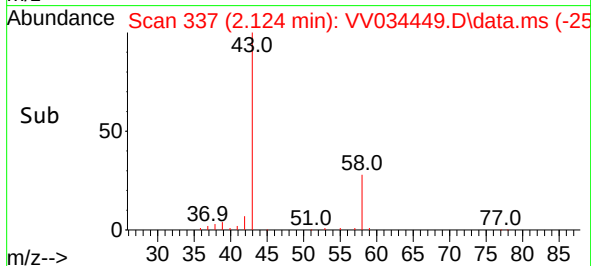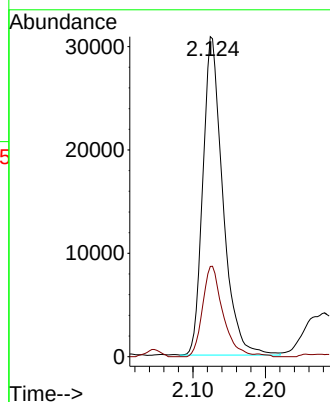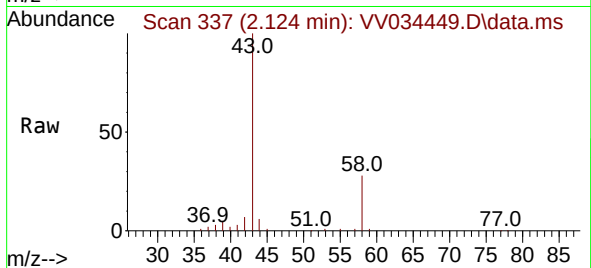

#16

Methylene chloride

Concen: 0.408 ug/L

RT: 2.449 min Scan# 438

Delta R.T. 0.003 min

Lab File: VV034449.D

Acq: 27 Feb 2024 15:11

Tgt Ion: 84 Resp: 3937

Ion Ratio Lower Upper

84 100

86 65.8 43.8 81.4

49 164.7 87.6 162.8#

