

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022724\
 Data File : VW034451.D
 Acq On : 27 Feb 2024 15:58
 Operator : SY/MD
 Sample : P1566-19DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD8DL

Quant Time: Feb 28 03:57:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 28 03:52:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	136823	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	131608	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	67574	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	34067	4.289	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.800%
7) Chloroethane-d5	1.532	69	31791	4.532	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.060	65	16255	4.397	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.000%
20) 2-Butanone-d5	3.802	46	118752	57.186	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.380%
24) Chloroform-d	4.252	84	78320	4.911	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	4.947	65	43215	5.325	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	4.963	84	140218	4.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	5.992	67	44490	5.033	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.600%
41) Toluene-d8	7.246	98	122389	4.610	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	7.561	79	15091	4.582	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.600%
46) 2-Hexanone-d5	8.027	63	102214	54.890	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.780%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	36496	5.216	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.400%
66) 1,2-Dichlorobenzene-d4	11.561	152	50925	4.960	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.200%
Target Compounds						Qvalue
13) Acetone	2.127	43	77407	36.650	ug/L	98
16) Methylene chloride	2.449	84	18592	1.900	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034451.D
Acq On : 27 Feb 2024 15:58
Operator : SY/MD
Sample : P1566-19DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD8DL

Quant Time: Feb 28 03:57:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 28 03:52:36 2024
Response via : Initial Calibration

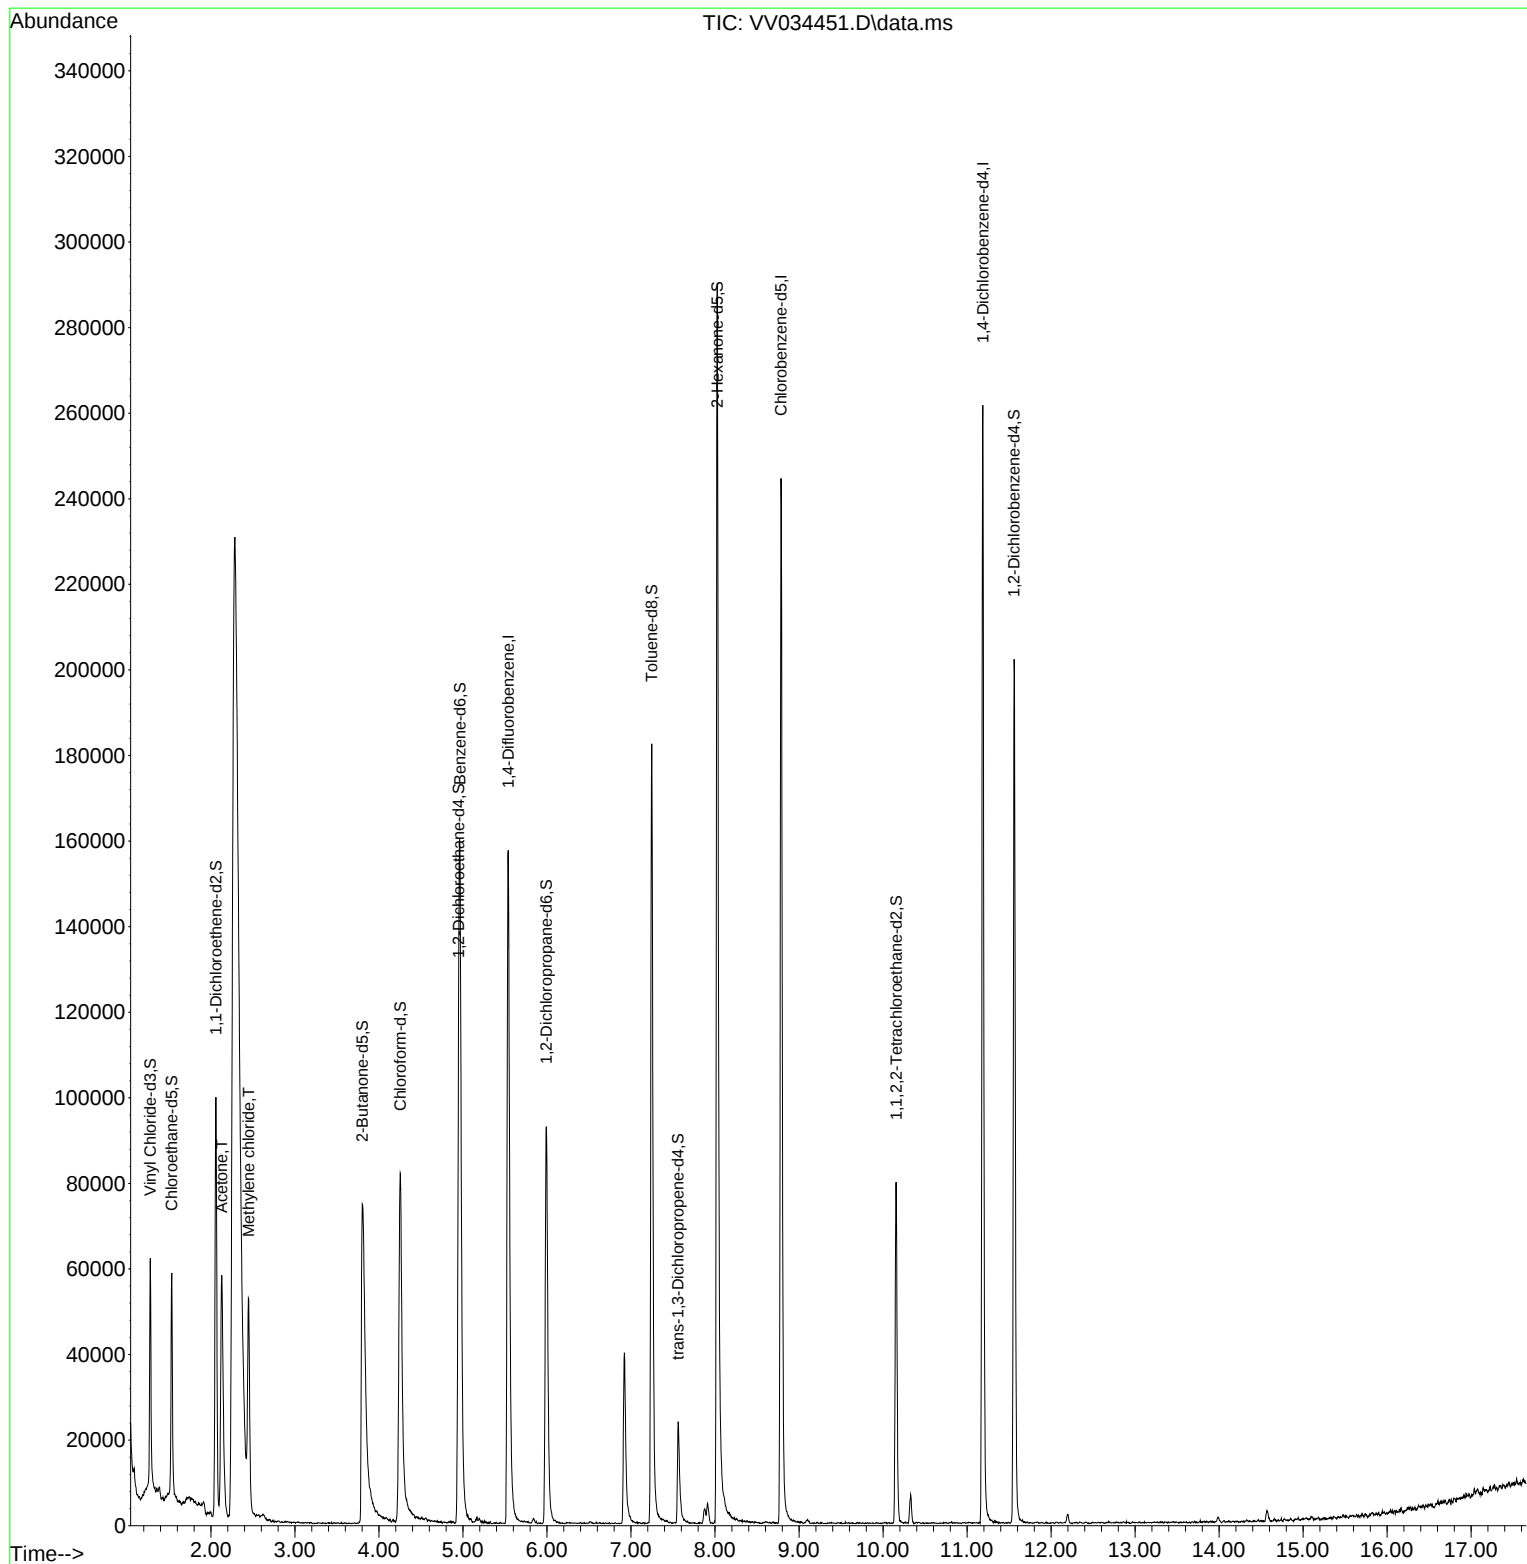

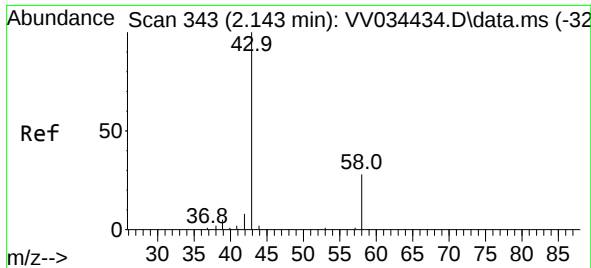

#13

Acetone

Concen: 36.650 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.016 min

Lab File: VV034451.D

Acq: 27 Feb 2024 15:58

Instrument :

MSVOA_V

ClientSampleId :





JWAD8DL

Tgt Ion: 43 Resp: 77407

Ion Ratio Lower Upper

43 100

58 29.0 0.0 56.2

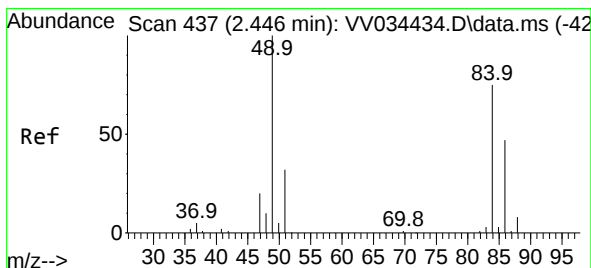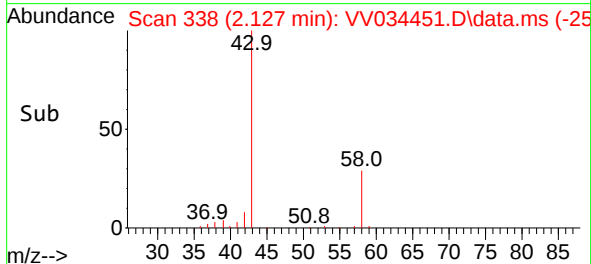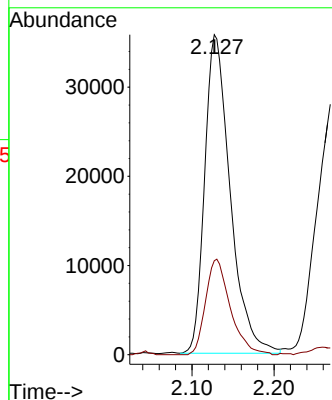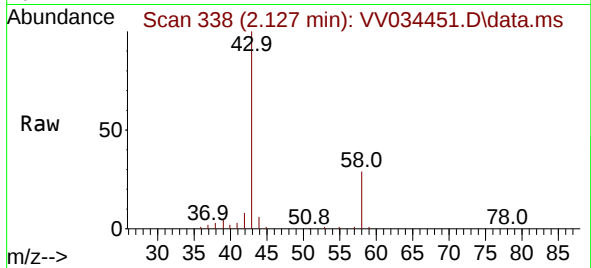

#16

Methylene chloride

Concen: 1.900 ug/L

RT: 2.449 min Scan# 438

Delta R.T. 0.003 min

Lab File: VV034451.D

Acq: 27 Feb 2024 15:58

Tgt Ion: 84 Resp: 18592

Ion Ratio Lower Upper

84 100

86 62.3 43.8 81.4

49 124.8 87.6 162.8

