

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW022724\
 Data File : VW034453.D
 Acq On : 27 Feb 2024 16:46
 Operator : SY/MD
 Sample : P1566-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 02/28/2024
 Supervised By :Mahesh Dadoda 02/28/2024

Quant Time: Feb 28 03:58:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 28 03:52:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	136612	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	130463	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	66652	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	32778	4.133	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.600%	
7) Chloroethane-d5	1.532	69	31248	4.462	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	89.200%	
11) 1,1-Dichloroethene-d2	2.060	65	14773	4.002	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.000%	
20) 2-Butanone-d5	3.809	46	119550	57.659	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	115.320%	
24) Chloroform-d	4.252	84	76130	4.781	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.600%	
26) 1,2-Dichloroethane-d4	4.947	65	43536	5.373	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.400%	
32) Benzene-d6	4.963	84	136068	4.636	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.800%	
36) 1,2-Dichloropropane-d6	5.992	67	43251	4.936	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.800%	
41) Toluene-d8	7.246	98	116385	4.422	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.400%	
43) trans-1,3-Dichloroprop...	7.561	79	14773	4.525	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.027	63	104969	56.864	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	113.720%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	35889	5.174	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.400%	
66) 1,2-Dichlorobenzene-d4	11.564	152	50331	4.970	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.400%	
Target Compounds						
13) Acetone	2.137	43	411863	195.304	ug/L	97
21) 2-Butanone	3.915	43	34790m	15.027	ug/L	
47) Tetrachloroethene	7.905	164	5385	0.728	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034453.D
Acq On : 27 Feb 2024 16:46
Operator : SY/MD
Sample : P1566-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
JWAD8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 02/28/2024
Supervised By :Mahesh Dadoda 02/28/2024

Quant Time: Feb 28 03:58:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 28 03:52:36 2024
Response via : Initial Calibration

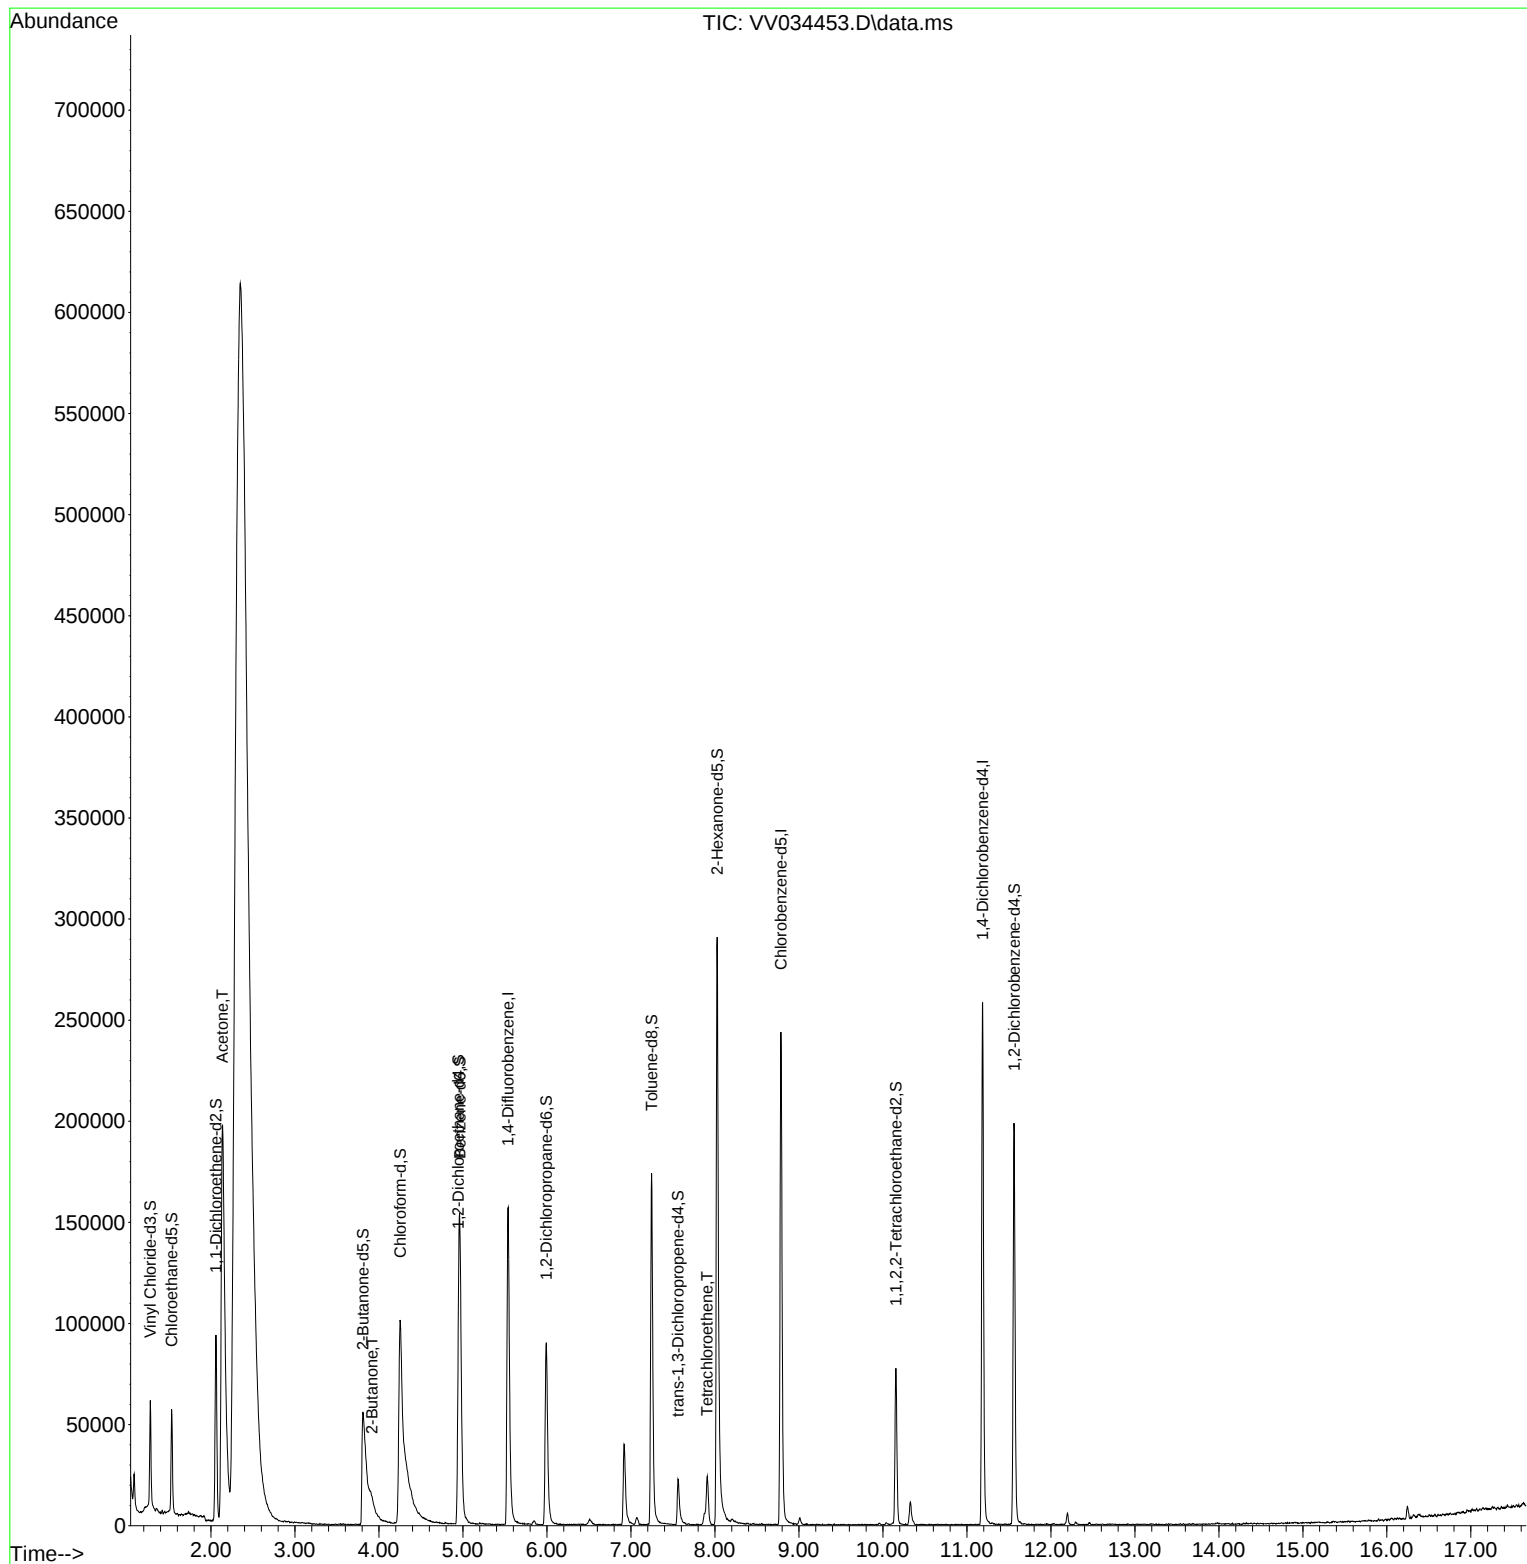

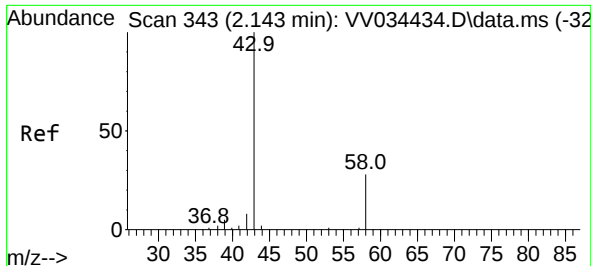

#13

Acetone

Concen: 195.304 ug/L

RT: 2.137 min Scan# 341

Delta R.T. -0.006 min

Lab File: VV034453.D

Acq: 27 Feb 2024 16:46

Instrument :

MSVOA_V

ClientSampleId :

JWAD8

Tgt Ion: 43 Resp: 41186

Ion Ratio Lower Upper

43 100





58 29.8 0.0 56.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 02/28/2024

Supervised By :Mahesh Dadoda 02/28/2024

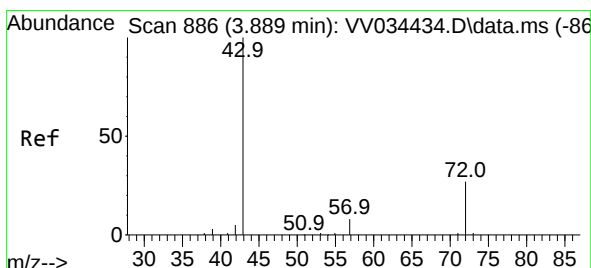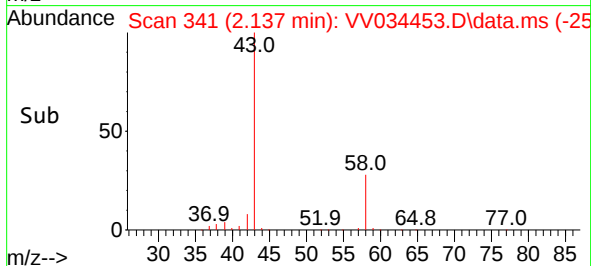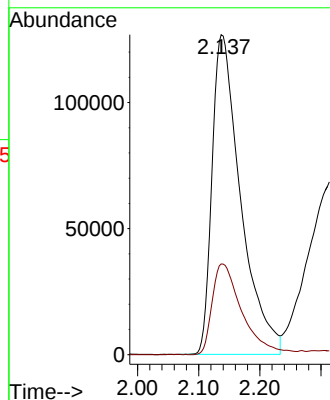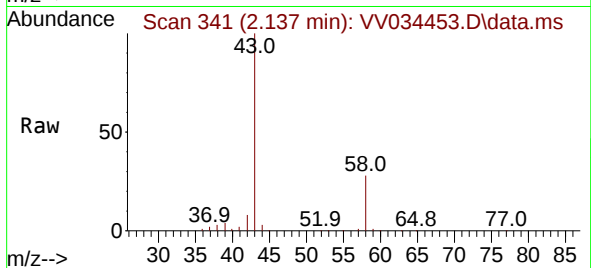

#21

2-Butanone

Concen: 15.027 ug/L m

RT: 3.915 min Scan# 894

Delta R.T. 0.026 min

Lab File: VV034453.D




Acq: 27 Feb 2024 16:46


Tgt Ion: 43 Resp: 34790

Ion Ratio Lower Upper

43 100


72 20.0 12.4 37.0

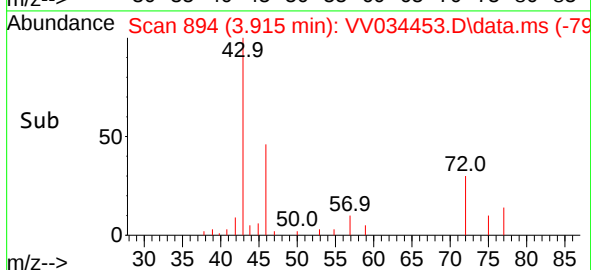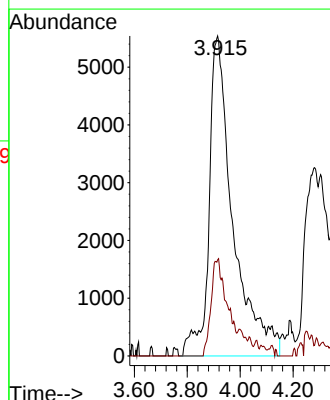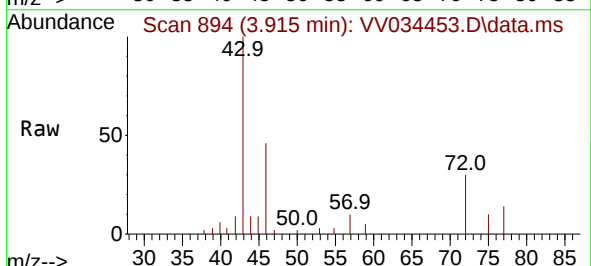

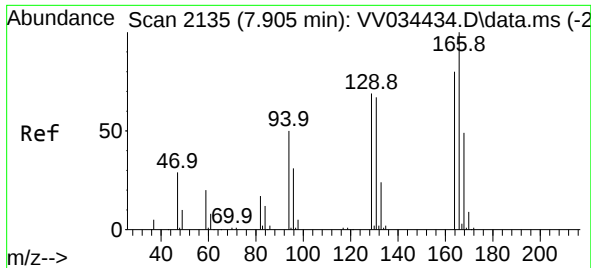

#47
Tetrachloroethene
Concen: 0.728 ug/L
RT: 7.905 min Scan# 2135
Delta R.T. -0.000 min
Lab File: VV034453.D
Acq: 27 Feb 2024 16:46

Instrument :
MSVOA_V
ClientSampleId :
JWAD8

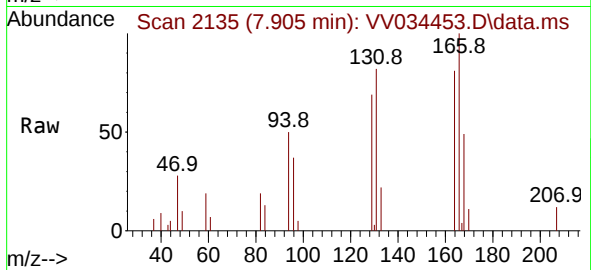

Tgt Ion:	164	Resp:	538
Ion	Ratio	Lower	Upper
164	100		
129	85.4	64.2	119.2
131	100.2	65.9	122.3
166	122.9	89.9	166.9

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 02/28/2024
Supervised By :Mahesh Dadoda 02/28/2024

