

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
 Data File : VV034449.D
 Acq On : 27 Feb 2024 15:11
 Operator : SY/MD
 Sample : P1566-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 JWAD0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	9	14	33	rVB2	21051	27320	3.45%	0.576%
2	1.278	67	74	91	rVB	53865	60114	7.59%	1.268%
3	1.532	146	153	167	rVB	52167	61724	7.79%	1.302%
4	2.060	305	317	328	rBV	92935	139092	17.55%	2.934%
5	2.124	328	337	356	rVB	48131	92471	11.67%	1.951%
6	2.272	366	383	420	rBV2	29374	136278	17.20%	2.875%
7	2.449	429	438	449	rVB	10765	17361	2.19%	0.366%
8	2.561	459	473	484	rBV2	7147	15842	2.00%	0.334%
9	3.805	843	860	902	rBV2	243913	792491	100.00%	16.719%
10	4.252	984	999	1033	rBB	72178	190441	24.03%	4.018%
11	4.960	1205	1219	1254	rBV2	155923	405708	51.19%	8.559%
12	5.538	1387	1399	1427	rBV	152412	322971	40.75%	6.814%
13	5.992	1526	1540	1564	rBV2	95318	203487	25.68%	4.293%
14	6.172	1587	1596	1614	rBV5	5202	11812	1.49%	0.249%
15	6.921	1818	1829	1847	rBV	38793	77447	9.77%	1.634%
16	7.072	1865	1876	1886	rBV5	5368	10523	1.33%	0.222%
17	7.246	1920	1930	1951	rBV	176167	309754	39.09%	6.535%
18	7.561	2020	2028	2048	rBV2	22343	43947	5.55%	0.927%
19	8.024	2164	2172	2205	rBV	279882	508110	64.12%	10.719%
20	8.786	2398	2409	2432	rBV	239658	398338	50.26%	8.404%
21	9.008	2469	2478	2493	rVB2	8003	13306	1.68%	0.281%
22	10.156	2820	2835	2850	rBV	76577	123167	15.54%	2.598%
23	10.326	2878	2888	2901	rVB3	8074	13493	1.70%	0.285%
24	11.188	3146	3156	3182	rBV	250700	395743	49.94%	8.349%
25	11.490	3237	3250	3262	rBV2	18603	38143	4.81%	0.805%
26	11.561	3262	3272	3288	rVB	199704	316956	39.99%	6.687%
27	14.574	4200	4209	4222	rBV5	7803	14032	1.77%	0.296%




Sum of corrected areas: 4740071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034449.D
Acq On : 27 Feb 2024 15:11
Operator : SY/MD
Sample : P1566-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

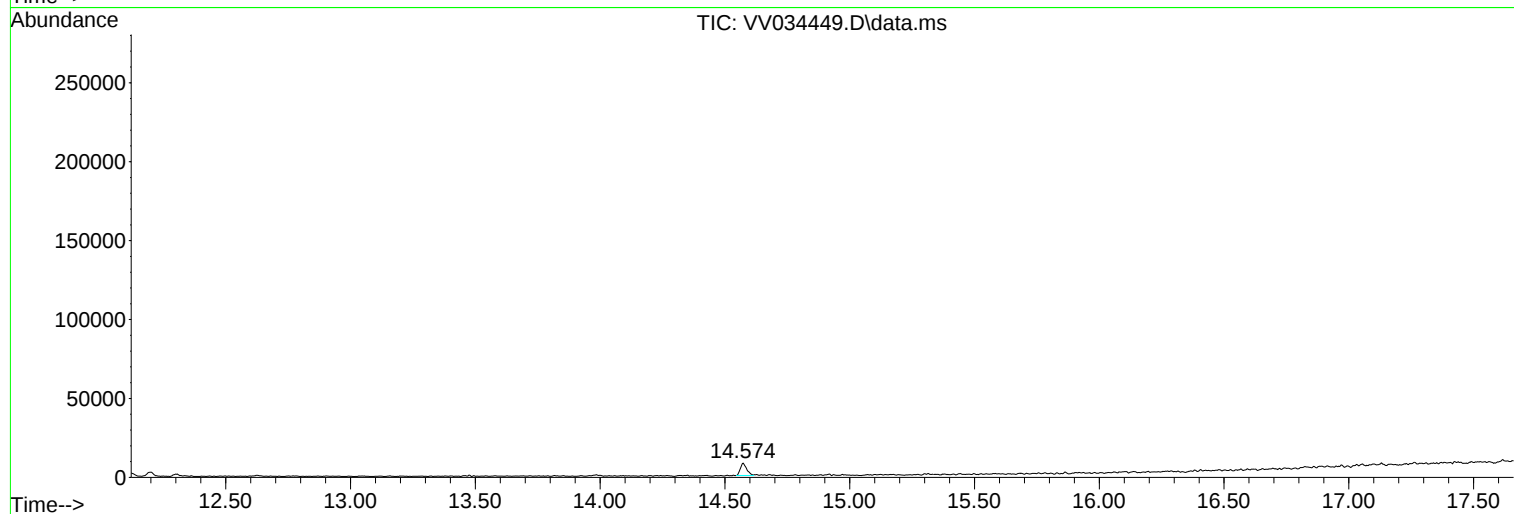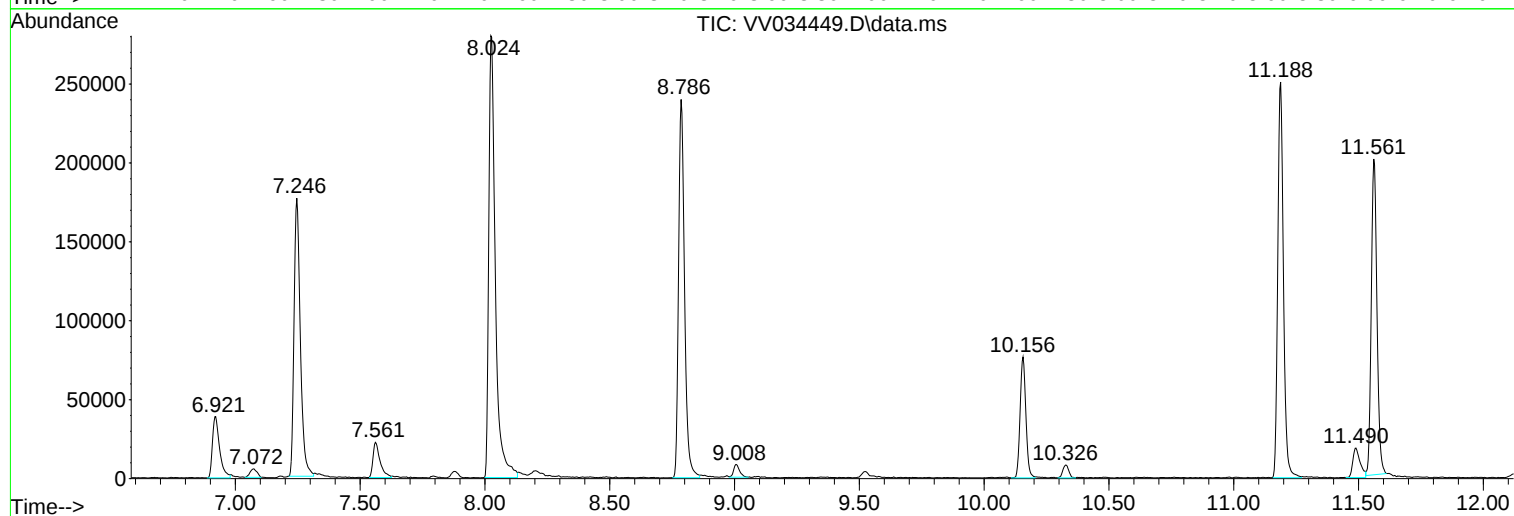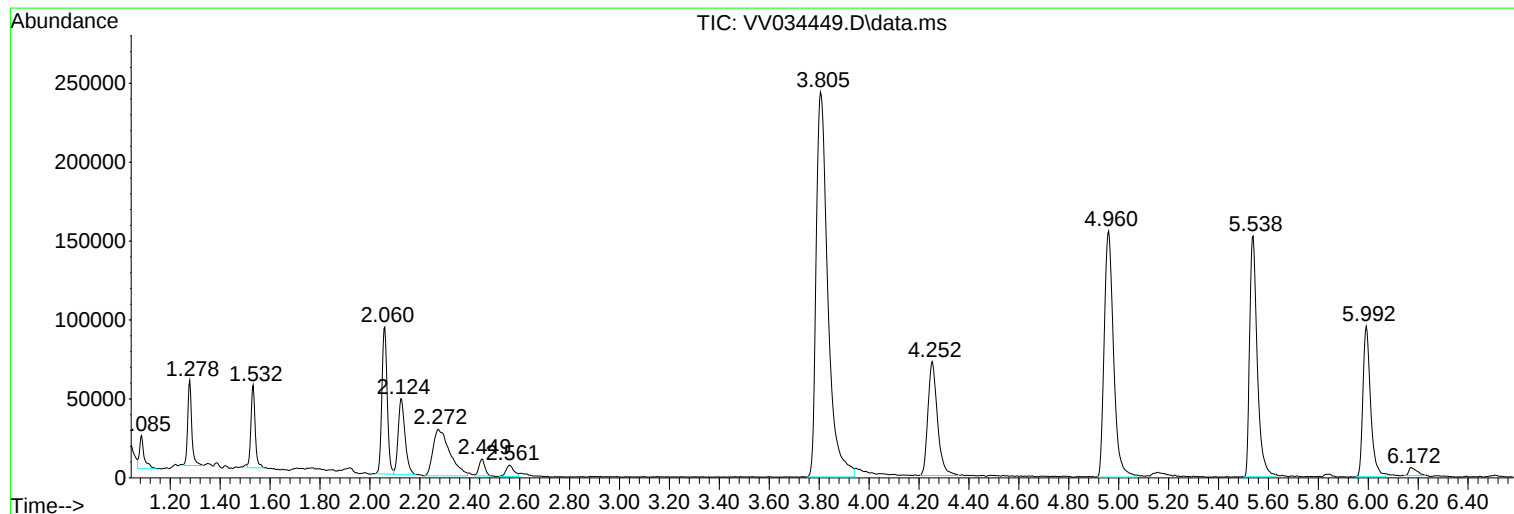

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034449.D
Acq On : 27 Feb 2024 15:11
Operator : SY/MD
Sample : P1566-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.272	2.11 ug/L	136278	1,4-Difluorobenzene	5.538

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

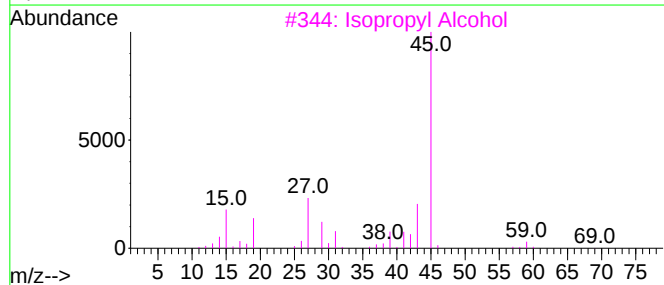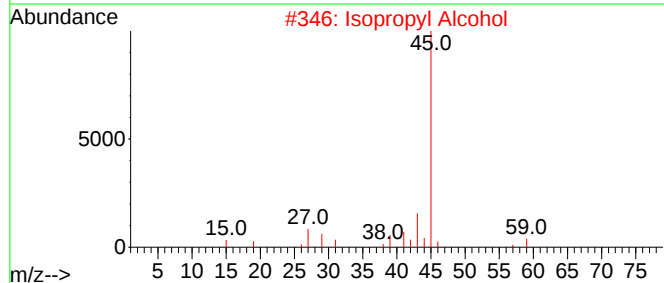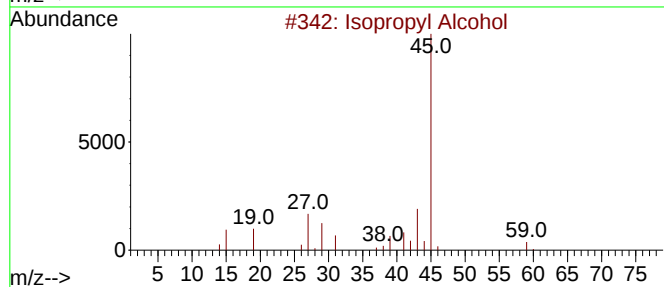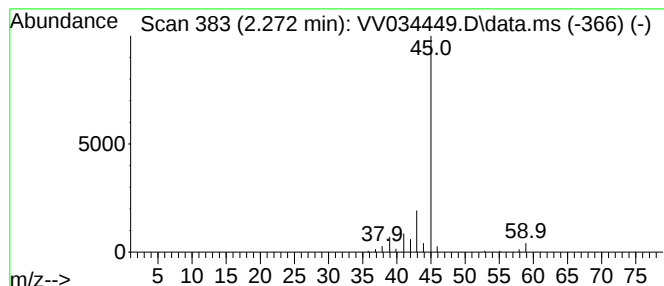

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034449.D
Acq On : 27 Feb 2024 15:11
Operator : SY/MD
Sample : P1566-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
JWAD0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.272	2.1	ug/L	136278	1	5.538	322971	5.0