
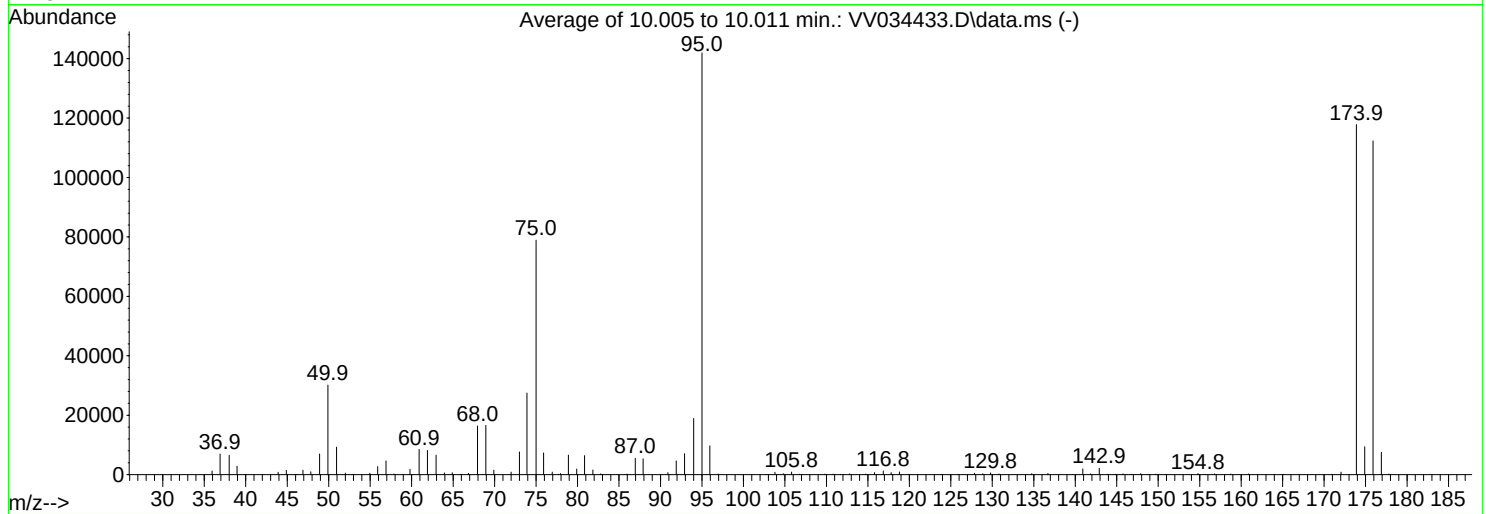


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022724\
Data File : VV034433.D
Acq On : 27 Feb 2024 08:32
Operator : SY/MD
Sample : BFB262
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB262

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR022624WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Feb 28 03:52:36 2024

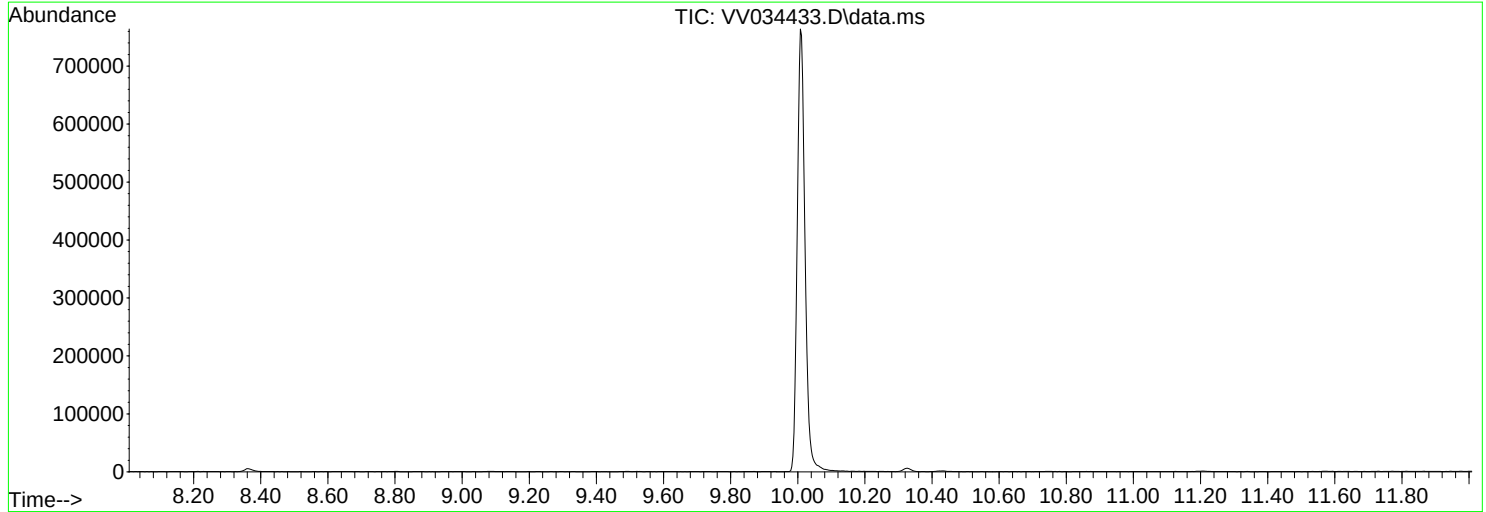

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	30141	PASS
75	95	30	80	55.6	78928	PASS
95	95	100	100	100.0	141952	PASS
96	95	5	9	6.8	9713	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.0	117845	PASS
175	174	5	9	8.0	9373	PASS
176	174	95	105	95.3	112304	PASS
177	176	5	10	6.7	7469	PASS

m/z	Abundance
39.90	277.0
43.90	257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
35.90	1233.0
36.90	6767.0
38.00	6363.0
39.00	2888.0
39.80	361.0
43.10	169.0
43.90	982.0
44.90	1409.0
46.20	208.0
46.90	1518.0
47.80	896.0
48.90	6658.0
49.90	29272.0
51.00	9158.0
52.00	513.0
52.80	111.0
55.00	500.0
55.90	2584.0
56.90	4315.0
57.80	246.0
59.80	1567.0
60.90	8155.0
61.90	7710.0
63.00	6431.0
64.00	627.0
64.90	608.0
65.90	108.0
66.80	343.0
67.90	15829.0
69.00	15874.0
69.90	1394.0
72.00	845.0
73.00	7482.0
73.90	26496.0
75.00	75568.0
75.90	7153.0
76.90	878.0
77.70	468.0
78.90	6254.0
79.90	1794.0
80.90	6254.0
81.90	1495.0
82.80	211.0
86.00	235.0
86.90	5195.0
87.90	5094.0
90.90	677.0
91.90	4317.0
92.90	6704.0
94.00	17960.0
95.00	134144.0
95.90	9321.0
97.10	226.0
103.80	782.0
104.80	348.0
105.80	801.0
106.80	126.0
109.80	128.0
110.80	189.0
112.10	128.0
112.80	206.0
114.80	181.0
115.80	661.0
116.80	1226.0
117.80	718.0
118.80	907.0
123.70	110.0
127.80	497.0
128.80	256.0
129.80	558.0
130.80	244.0
134.70	327.0
136.70	408.0
139.70	111.0
140.90	1891.0
141.80	292.0
142.90	2082.0
143.80	122.0
144.60	196.0
145.70	249.0
146.70	149.0
147.90	350.0
148.70	120.0
149.70	149.0
152.90	120.0
154.80	316.0
155.70	102.0
156.80	278.0
158.80	192.0
160.90	265.0
170.90	211.0
172.00	872.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

173.90	109000.0
174.90	8990.0
175.90	104336.0
176.90	6751.0
177.80	246.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
36.00	1272.0
36.90	7091.0
38.00	6725.0
38.90	2985.0
39.80	313.0
43.00	138.0
43.90	1106.0
44.90	1473.0
46.10	179.0
46.90	1574.0
47.90	967.0
48.90	7224.0
49.90	31232.0
50.90	9549.0
52.00	570.0
55.00	502.0
55.90	2754.0
56.90	4895.0
57.80	256.0
59.80	1830.0
60.90	8818.0
61.90	8473.0
62.90	6895.0
63.90	644.0
64.90	678.0
66.80	434.0
67.90	16848.0
69.00	17256.0
69.90	1603.0
72.00	921.0
73.00	8025.0
73.90	28280.0
75.00	81744.0
75.90	7657.0
77.00	876.0
77.90	501.0
78.90	6737.0
79.90	1978.0
80.80	6641.0
81.90	1649.0
82.80	256.0
86.00	203.0
86.90	5713.0
87.90	5436.0
90.90	743.0
91.90	4755.0
92.90	7205.0
94.00	19608.0
95.00	146816.0
96.00	10018.0
96.90	223.0
103.80	847.0
104.80	311.0
105.80	878.0
106.70	159.0
109.80	159.0
110.80	160.0
111.70	148.0
112.80	294.0
114.80	216.0
115.80	735.0
116.80	1276.0
117.80	755.0
118.80	955.0
123.70	111.0
125.80	115.0
127.80	533.0
128.80	313.0
129.80	607.0
130.80	254.0
134.70	337.0
136.70	473.0
139.70	125.0
140.90	2016.0
141.90	287.0
142.90	2234.0
143.90	105.0
144.80	155.0
145.70	282.0
146.80	142.0
147.90	344.0
148.70	113.0
149.70	193.0
151.90	130.0
152.90	125.0
154.80	390.0
155.70	108.0
156.80	289.0
158.80	232.0
160.90	260.0
171.00	190.0
172.10	852.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

173.90	121800.0
174.90	9663.0
175.90	116112.0
176.90	7744.0
177.80	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

m/z	Abundance
35.90	1175.0
36.90	7058.0
38.00	6546.0
38.90	2711.0
39.80	284.0
42.90	102.0
43.90	1169.0
44.90	1418.0
45.90	162.0
46.90	1508.0
47.90	1042.0
48.90	6945.0
49.90	29920.0
50.90	9082.0
52.00	521.0
54.90	478.0
55.90	2717.0
56.90	4715.0
57.90	227.0
59.80	1865.0
60.90	8494.0
61.90	8270.0
62.90	6433.0
63.90	595.0
64.90	593.0
66.90	472.0
68.00	16432.0
68.90	16712.0
69.90	1511.0
72.00	918.0
73.00	7432.0
73.90	27656.0
75.00	79472.0
75.90	7212.0
76.90	840.0
78.00	567.0
78.90	6724.0
79.90	1962.0
80.80	6413.0
81.80	1598.0
82.80	280.0
85.80	163.0
87.00	5583.0
87.90	5500.0
90.90	753.0
91.90	4860.0
92.90	7240.0
94.00	19216.0
95.00	144896.0
96.00	9801.0
96.90	238.0
102.70	102.0
103.80	830.0
104.80	274.0
105.80	887.0
106.70	168.0
109.80	174.0
110.80	129.0
111.70	155.0
112.80	319.0
114.70	196.0
115.80	787.0
116.90	1280.0
117.80	683.0
118.80	987.0
125.90	153.0
127.90	511.0
128.90	377.0
129.80	576.0
130.80	241.0
134.80	343.0
136.70	433.0
139.70	135.0
140.90	1898.0
141.90	267.0
142.90	2158.0
143.90	120.0
144.90	175.0
145.80	231.0
146.80	125.0
147.90	293.0
148.90	118.0
149.70	189.0
151.90	118.0
154.80	454.0
156.80	270.0
158.70	223.0
160.90	191.0
172.10	839.0
173.90	122736.0
174.90	9466.0
175.90	116464.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262

176.907913.0

177.80229.0

Instrument :
MSVOA_V
ClientSampleId :
BFB262