


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV022822\
Data File : VV024828.D
Acq On : 28 Feb 2022 09:41
Operator : SY/MD
Sample : BFB264
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB264

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Title : VOC Analysis
Last Update : Wed Mar 02 01:20:37 2022

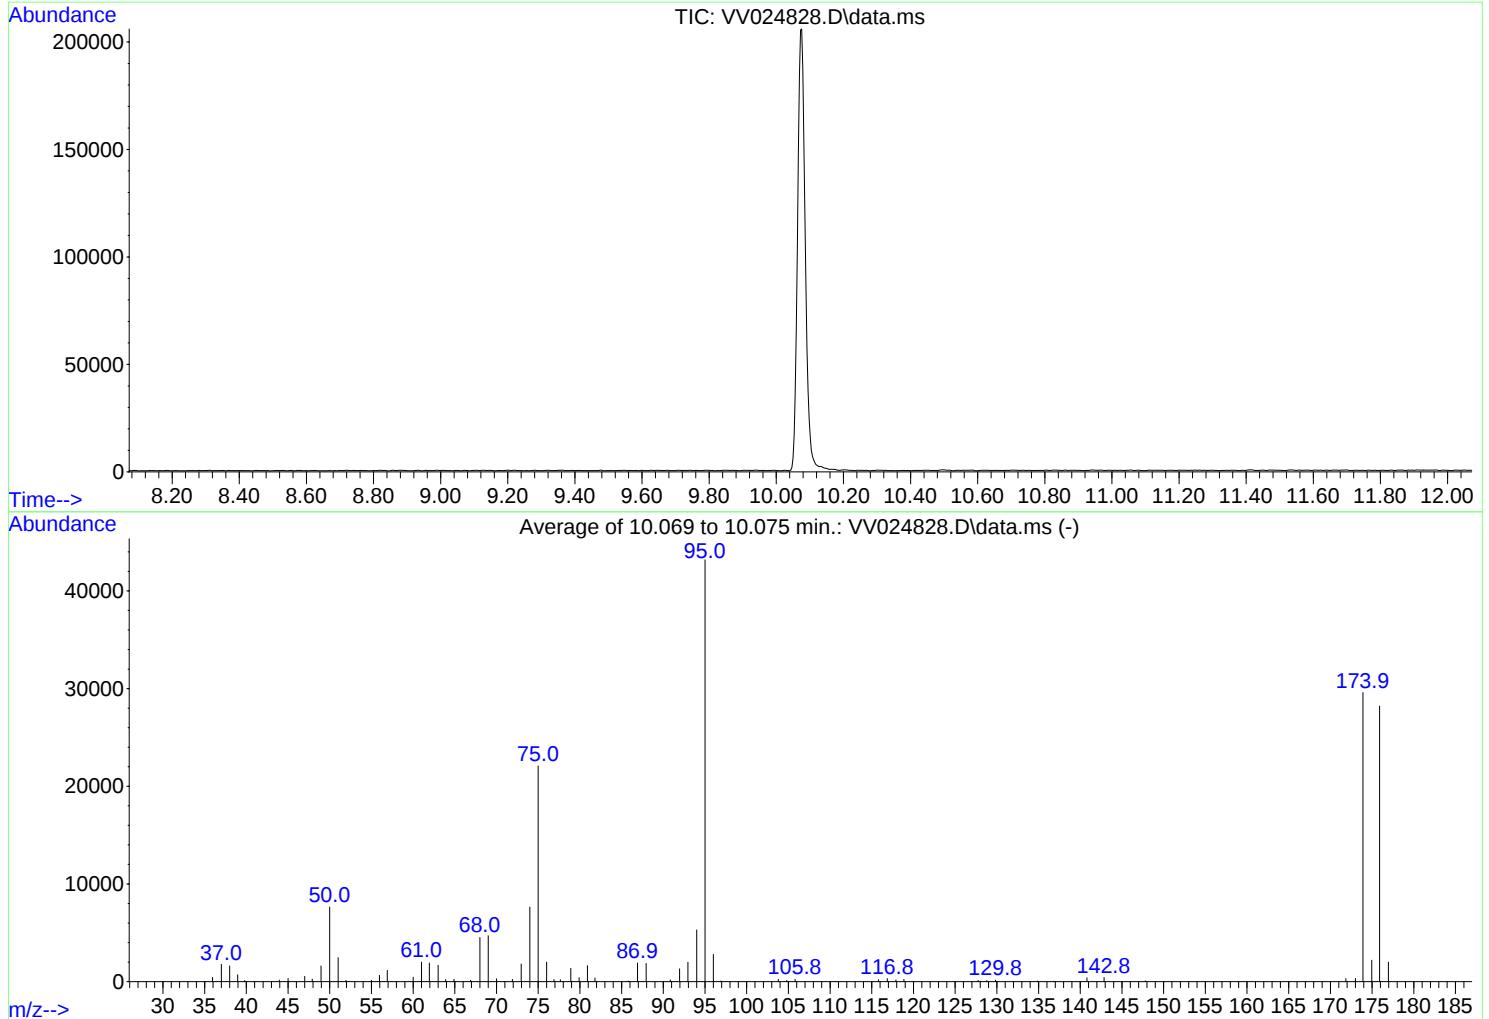

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7626	PASS
75	95	30	80	51.1	22077	PASS
95	95	100	100	100.0	43184	PASS
96	95	5	9	6.4	2784	PASS
173	174	0.00	2	1.1	326	PASS
174	95	50	120	68.5	29597	PASS
175	174	5	9	7.4	2190	PASS
176	174	95	105	95.3	28211	PASS
177	176	5	10	7.0	1978	PASS

m/z	Abundance
39.80	288.0
43.90	318.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
35.90	369.0
37.00	1644.0
38.00	1551.0
38.90	632.0
39.90	414.0
44.00	490.0
45.00	322.0
47.00	628.0
47.90	226.0
48.90	1543.0
50.00	7240.0
51.00	2317.0
51.90	130.0
55.00	122.0
56.00	661.0
56.90	1152.0
60.00	440.0
61.00	1848.0
62.00	1882.0
63.00	1549.0
63.90	203.0
64.90	232.0
66.90	143.0
68.00	4283.0
69.00	4457.0
70.00	294.0
71.90	197.0
73.00	1717.0
74.00	7072.0
75.00	20360.0
76.00	1884.0
76.90	202.0
77.60	189.0
78.90	1220.0
79.90	394.0
80.90	1578.0
81.80	326.0
86.90	1728.0
88.00	1856.0
90.80	132.0
91.90	1264.0
92.90	1837.0
94.00	4986.0
95.00	40176.0
96.00	2660.0
96.90	120.0
103.80	215.0
104.80	126.0
105.80	242.0
115.80	173.0
116.80	280.0
117.90	175.0
118.80	244.0
127.70	224.0
128.80	109.0
129.90	137.0
134.90	108.0
140.80	369.0
142.90	390.0
147.80	118.0
171.80	286.0
173.00	289.0
173.90	27104.0
175.00	2070.0
175.90	25320.0
176.90	1806.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
35.90	448.0
37.00	1838.0
38.00	1680.0
39.00	732.0
39.80	384.0
44.00	493.0
45.00	337.0
47.00	563.0
47.90	276.0
48.90	1692.0
50.00	7817.0
51.00	2523.0
51.90	143.0
55.00	152.0
56.00	648.0
56.90	1197.0
60.00	477.0
61.00	2058.0
62.00	1914.0
63.00	1751.0
63.90	210.0
64.90	252.0
66.90	165.0
68.00	4699.0
69.00	4914.0
70.00	311.0
71.90	226.0
73.00	1828.0
74.00	7928.0
75.00	22816.0
76.00	2089.0
76.90	212.0
77.60	220.0
78.90	1392.0
79.90	415.0
80.90	1711.0
81.80	395.0
85.80	123.0
86.90	1949.0
87.90	1935.0
90.90	184.0
92.00	1355.0
92.90	2053.0
94.00	5509.0
95.00	44792.0
96.00	2877.0
96.90	104.0
103.80	227.0
104.80	147.0
105.80	250.0
115.80	201.0
116.80	318.0
117.90	186.0
118.80	242.0
127.80	177.0
128.80	125.0
129.80	147.0
134.90	106.0
140.80	406.0
142.90	416.0
147.80	109.0
171.80	329.0
173.00	343.0
173.90	30712.0
174.90	2228.0
175.90	29096.0
177.00	2074.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264

m/z	Abundance
36.00	449.0
37.00	1815.0
38.00	1612.0
39.00	775.0
39.90	399.0
44.00	471.0
45.00	317.0
47.00	444.0
47.90	273.0
49.00	1600.0
50.00	7821.0
51.00	2534.0
52.00	137.0
55.00	138.0
55.90	608.0
56.90	1116.0
60.00	441.0
61.00	2086.0
61.90	1912.0
63.00	1736.0
63.90	212.0
64.90	278.0
66.90	153.0
68.00	4595.0
69.00	4749.0
70.00	297.0
71.90	260.0
72.90	1884.0
74.00	7892.0
75.00	23056.0
76.00	2020.0
76.90	218.0
77.70	198.0
78.90	1444.0
79.90	435.0
80.90	1636.0
81.80	429.0
85.80	101.0
86.90	2076.0
87.90	1816.0
90.90	215.0
92.00	1335.0
93.00	2062.0
94.00	5382.0
95.00	44584.0
96.00	2814.0
103.80	248.0
104.80	127.0
105.80	224.0
110.70	108.0
115.80	198.0
116.90	321.0
117.90	170.0
118.90	220.0
128.00	145.0
128.80	131.0
129.80	162.0
136.80	107.0
140.80	393.0
142.80	456.0
171.90	343.0
173.00	346.0
173.90	30976.0
174.90	2272.0
175.90	30216.0
177.00	2053.0

Instrument :
MSVOA_V
ClientSampleId :
BFB264