
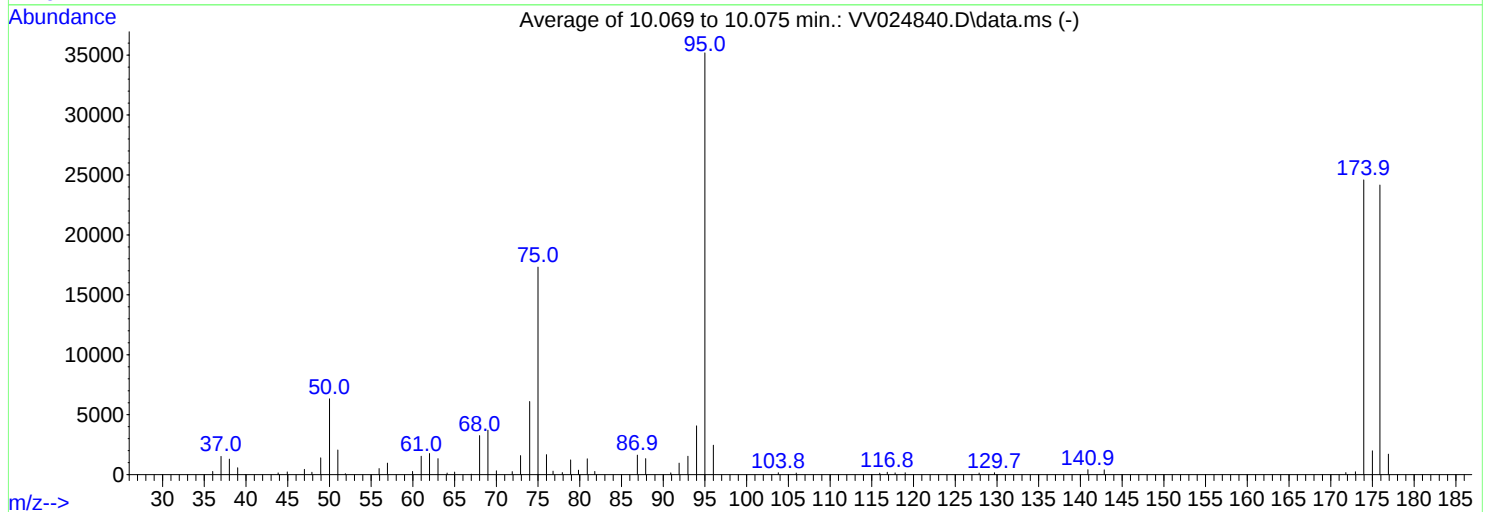


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030122\
Data File : VV024840.D
Acq On : 01 Mar 2022 09:51
Operator : SY/MD
Sample : BFB265
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB265

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Title : VOC Analysis
Last Update : Wed Mar 02 01:20:37 2022

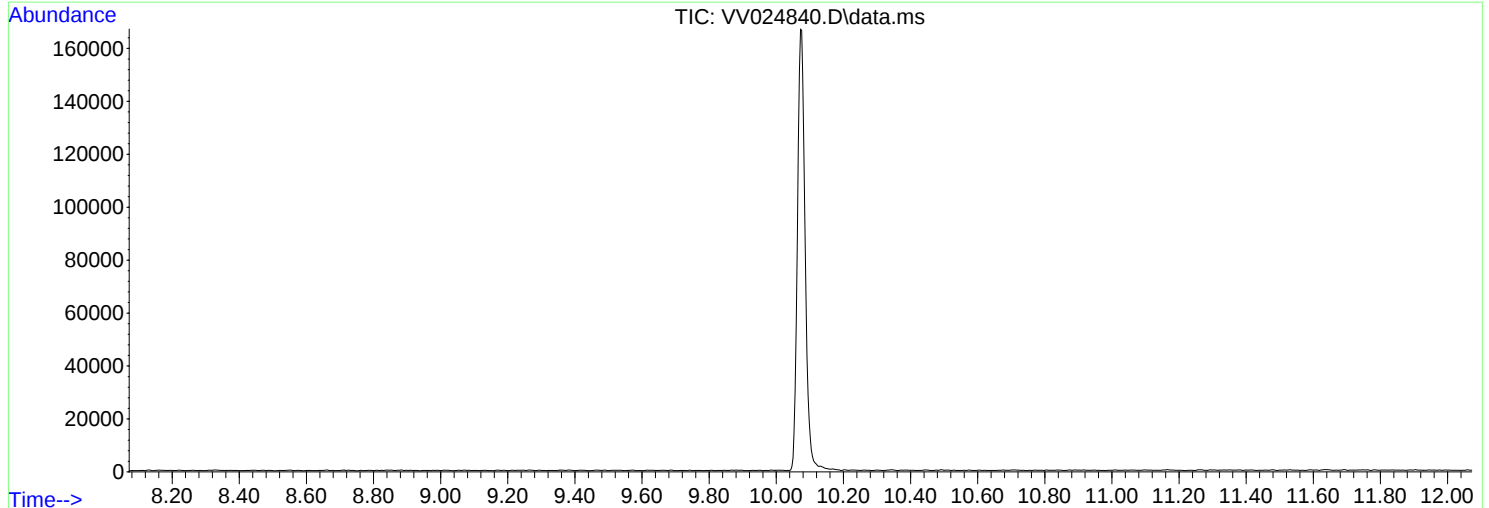

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	6323	PASS
75	95	30	80	49.2	17307	PASS
95	95	100	100	100.0	35187	PASS
96	95	5	9	7.0	2462	PASS
173	174	0.00	2	1.0	243	PASS
174	95	50	120	69.9	24592	PASS
175	174	5	9	8.1	1984	PASS
176	174	95	105	98.3	24165	PASS
177	176	5	10	7.1	1709	PASS

m/z	Abundance
39.90	317.0
43.80	254.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	259.0
37.00	1503.0
38.00	1224.0
39.00	563.0
39.90	325.0
43.90	419.0
44.90	232.0
47.00	433.0
47.90	182.0
49.00	1394.0
50.00	5895.0
51.00	1965.0
51.90	109.0
55.90	444.0
56.90	916.0
59.90	248.0
61.00	1488.0
62.00	1643.0
63.00	1190.0
64.20	111.0
65.00	222.0
68.00	3126.0
69.00	3621.0
70.00	286.0
71.90	211.0
72.90	1431.0
74.00	5837.0
75.00	16424.0
76.00	1516.0
76.80	234.0
77.90	145.0
78.90	1127.0
79.80	347.0
80.90	1257.0
81.80	253.0
86.90	1498.0
87.90	1173.0
90.90	168.0
91.90	930.0
93.00	1381.0
94.00	3982.0
95.00	33224.0
96.00	2400.0
103.80	132.0
105.90	151.0
115.90	119.0
116.90	186.0
117.80	123.0
119.00	138.0
127.90	138.0
129.70	140.0
140.90	443.0
142.90	363.0
171.80	170.0
172.90	234.0
173.90	22456.0
175.00	1826.0
175.90	22160.0
176.90	1642.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	275.0
37.00	1576.0
38.00	1338.0
39.00	592.0
39.90	342.0
43.90	385.0
45.00	226.0
47.00	473.0
47.90	209.0
48.90	1485.0
50.00	6504.0
51.00	2116.0
51.90	113.0
55.90	539.0
57.00	989.0
60.00	269.0
61.00	1601.0
62.00	1806.0
63.00	1389.0
64.10	117.0
65.00	229.0
67.00	106.0
68.00	3315.0
69.00	3839.0
70.00	340.0
71.90	279.0
72.90	1630.0
74.00	6317.0
75.00	17856.0
76.00	1715.0
76.80	307.0
77.90	190.0
78.90	1277.0
79.90	403.0
80.90	1373.0
81.80	272.0
86.90	1668.0
87.90	1369.0
90.90	152.0
91.90	1000.0
93.00	1581.0
94.00	4188.0
95.00	36344.0
96.00	2558.0
103.80	166.0
106.00	140.0
116.00	123.0
116.90	204.0
117.80	159.0
119.00	161.0
127.80	128.0
129.70	168.0
140.90	431.0
142.90	410.0
171.80	177.0
173.00	248.0
173.90	25424.0
175.00	2062.0
175.90	24936.0
176.90	1737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265

m/z	Abundance
36.00	272.0
37.00	1497.0
38.00	1320.0
39.00	572.0
40.00	324.0
43.90	383.0
45.00	215.0
47.00	409.0
47.90	193.0
48.90	1320.0
50.00	6570.0
51.00	2107.0
56.00	552.0
57.00	991.0
60.00	304.0
61.00	1533.0
62.00	1844.0
63.00	1417.0
64.00	157.0
65.00	197.0
68.00	3326.0
69.00	3672.0
70.00	322.0
71.90	275.0
72.90	1705.0
74.00	6143.0
75.00	17640.0
76.00	1767.0
76.80	324.0
77.90	178.0
78.90	1270.0
79.90	394.0
80.90	1322.0
81.80	274.0
86.90	1731.0
87.90	1462.0
90.90	123.0
91.90	958.0
92.90	1635.0
94.00	4048.0
95.00	35992.0
96.00	2427.0
103.80	177.0
106.00	124.0
116.00	110.0
116.80	220.0
117.80	177.0
119.00	178.0
127.80	119.0
129.70	170.0
140.90	361.0
142.80	424.0
171.80	171.0
173.00	247.0
174.00	25896.0
175.00	2063.0
175.90	25400.0
176.90	1747.0

Instrument :
MSVOA_V
ClientSampleId :
BFB265