


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030222\
 Data File : VV024847.D
 Acq On : 02 Mar 2022 10:02
 Operator : SY/MD
 Sample : BFB201
 Misc : 5.00g/10mL/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB201

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM030222SMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 03 02:51:32 2022

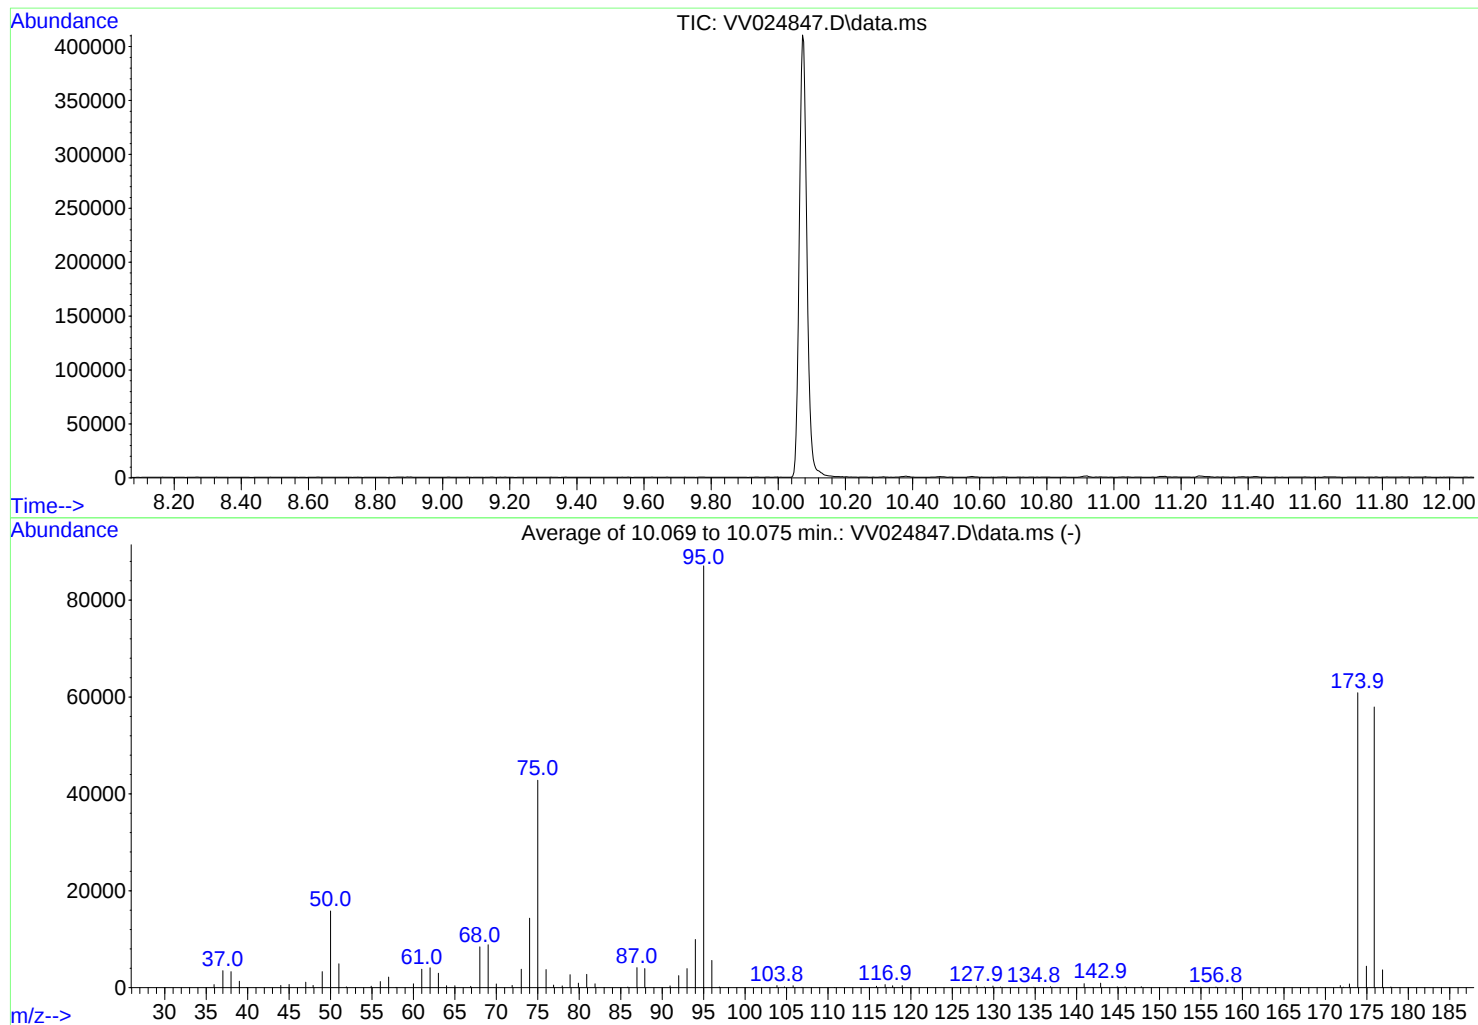

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	15834	PASS
75	95	30	80	49.1	42797	PASS
95	95	100	100	100.0	87080	PASS
96	95	5	9	6.4	5613	PASS
173	174	0.00	2	1.2	756	PASS
174	95	50	120	69.9	60885	PASS
175	174	5	9	7.3	4441	PASS
176	174	95	101	95.1	57928	PASS
177	176	5	9	6.3	3669	PASS

m/z	Abundance
39.90	312.0
44.00	298.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
35.90	600.0
37.00	3349.0
38.00	3193.0
39.00	1208.0
39.90	366.0
44.00	673.0
45.00	617.0
47.00	1105.0
47.90	481.0
49.00	3227.0
50.00	15083.0
51.00	4815.0
51.90	179.0
54.90	277.0
56.00	1291.0
57.00	2086.0
57.90	129.0
60.00	754.0
61.00	3674.0
62.00	3930.0
63.00	2844.0
64.00	400.0
65.00	423.0
66.90	244.0
68.00	8048.0
69.00	8573.0
70.00	722.0
71.90	486.0
73.00	3703.0
74.00	13812.0
75.00	40560.0
76.00	3656.0
76.90	514.0
78.00	343.0
78.90	2512.0
79.90	897.0
80.90	2612.0
81.90	763.0
85.90	124.0
86.90	3907.0
87.90	3791.0
91.00	357.0
92.00	2293.0
93.00	3667.0
94.00	9636.0
95.00	83120.0
96.00	5515.0
96.90	124.0
103.90	383.0
104.80	118.0
105.80	356.0
110.80	110.0
115.90	318.0
116.90	576.0
117.80	366.0
118.90	465.0
127.90	335.0
128.90	142.0
129.90	278.0
130.80	133.0
134.90	116.0
136.90	162.0
140.90	731.0
141.90	106.0
142.90	924.0
144.90	149.0
145.90	158.0
147.80	189.0
154.70	158.0
156.80	133.0
158.80	125.0
171.80	333.0
172.20	352.0
172.90	704.0
173.90	56328.0
174.90	4330.0
175.90	53184.0
176.90	3522.0
177.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
35.90	645.0
37.00	3654.0
38.00	3429.0
39.00	1357.0
39.90	355.0
44.00	769.0
45.00	677.0
47.00	1187.0
47.90	485.0
49.00	3487.0
50.00	16544.0
51.00	5114.0
51.90	183.0
54.90	302.0
56.00	1317.0
57.00	2239.0
57.90	112.0
60.00	823.0
61.00	3926.0
62.00	4208.0
63.00	3078.0
64.00	407.0
65.00	427.0
66.90	274.0
68.00	8685.0
69.00	9137.0
70.00	817.0
71.90	489.0
73.00	3895.0
74.00	14928.0
75.00	44464.0
76.00	3828.0
76.90	551.0
77.90	349.0
78.90	2770.0
79.90	957.0
80.90	2833.0
81.90	831.0
85.80	121.0
86.90	4231.0
87.90	4056.0
90.90	366.0
92.00	2549.0
93.00	4091.0
94.00	10174.0
95.00	90064.0
96.00	5829.0
96.90	133.0
103.90	458.0
104.80	163.0
105.80	412.0
106.90	105.0
115.90	303.0
116.90	642.0
117.80	410.0
118.90	455.0
127.90	368.0
128.80	132.0
129.90	352.0
130.80	131.0
134.80	104.0
136.80	201.0
140.90	849.0
142.90	948.0
144.90	180.0
145.90	181.0
147.80	199.0
154.90	153.0
156.80	141.0
158.80	104.0
171.80	429.0
172.90	798.0
173.90	62952.0
174.90	4556.0
175.90	59904.0
176.90	3783.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	603.0
37.00	3472.0
38.00	3337.0
39.00	1375.0
39.90	351.0
44.00	796.0
45.00	651.0
47.00	1076.0
47.90	460.0
49.00	3239.0
50.00	15874.0
51.00	4818.0
51.90	183.0
54.90	280.0
56.00	1196.0
57.00	2204.0
60.00	768.0
61.00	3760.0
62.00	4149.0
63.00	3048.0
64.00	365.0
65.00	332.0
66.90	259.0
68.00	8509.0
69.00	8886.0
70.00	766.0
71.90	447.0
73.00	3841.0
74.00	14286.0
75.00	43368.0
76.00	3734.0
76.90	505.0
77.90	369.0
78.90	2751.0
79.90	891.0
80.90	2817.0
81.90	831.0
83.00	103.0
85.90	135.0
87.00	4225.0
87.90	4004.0
90.90	360.0
92.00	2622.0
93.00	3992.0
94.00	10000.0
95.00	88056.0
96.00	5494.0
96.90	129.0
103.80	484.0
104.70	183.0
105.80	430.0
106.80	105.0
115.80	280.0
116.90	679.0
117.80	412.0
119.00	418.0
127.90	343.0
128.80	111.0
129.90	402.0
130.80	131.0
134.80	111.0
136.80	231.0
140.90	891.0
142.90	924.0
144.90	194.0
145.80	163.0
147.80	197.0
154.90	167.0
156.80	147.0
171.80	535.0
172.90	765.0
173.90	63376.0
175.00	4436.0
175.90	60696.0
176.90	3701.0
177.90	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201