
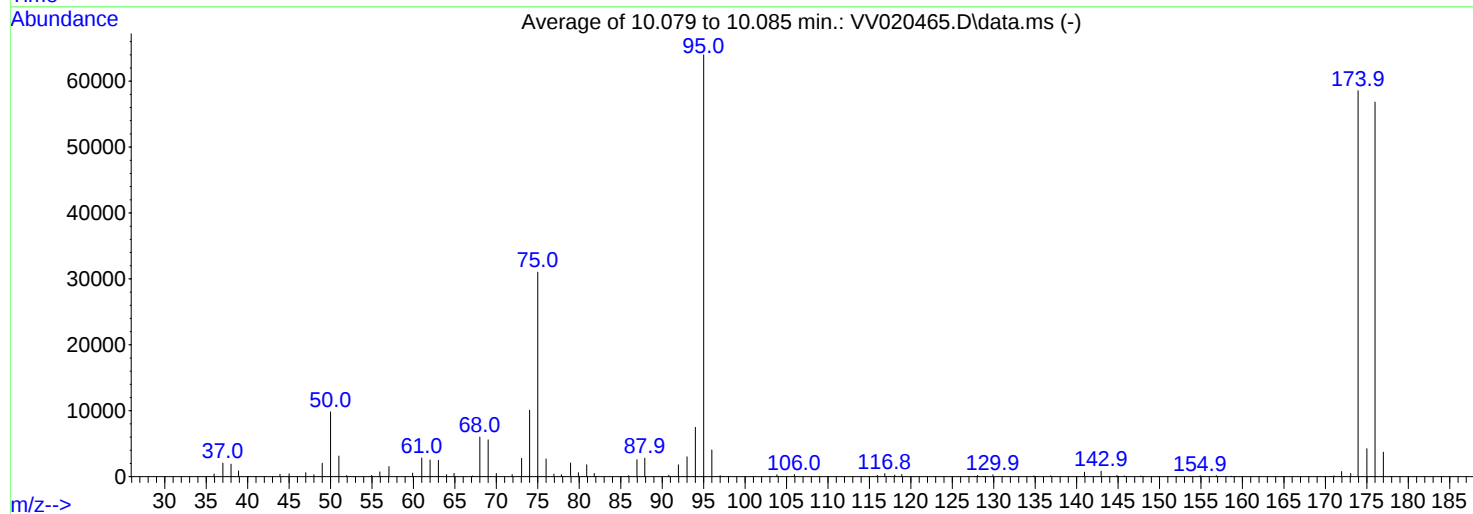


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030521\
 Data File : VV020465.D
 Acq On : 05 Mar 2021 10:33
 Operator : SY/MD
 Sample : BFB96
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB96

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM030521WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 05 13:10:43 2021

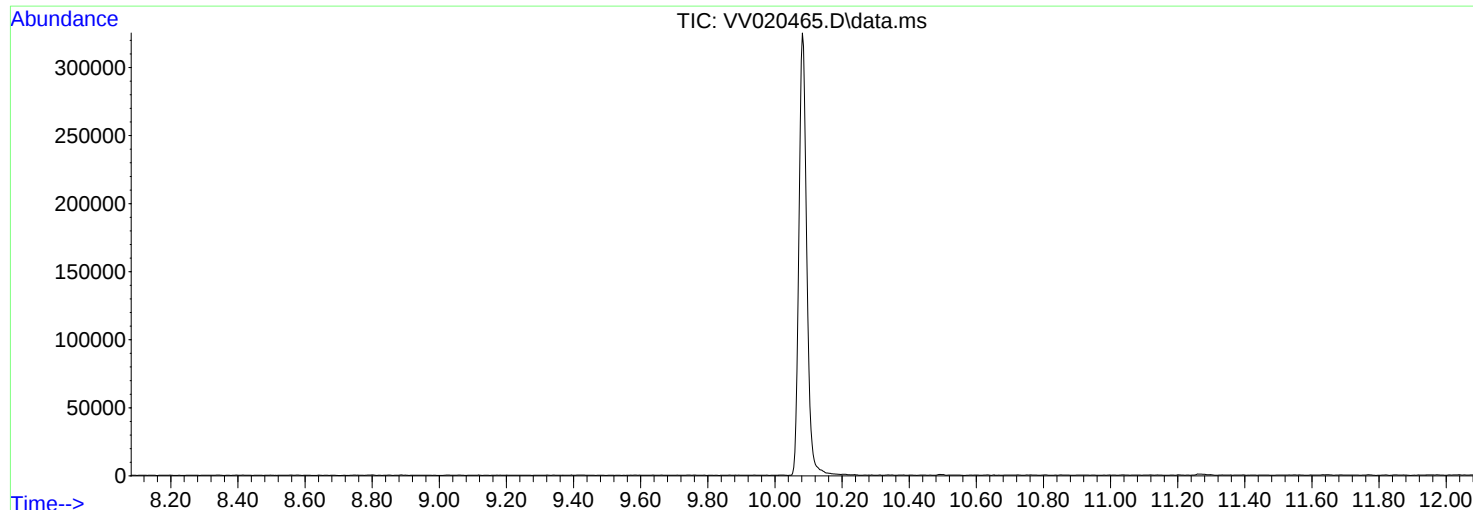

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	9821	PASS
75	95	30	80	48.5	31032	PASS
95	95	100	100	100.0	63995	PASS
96	95	5	9	6.3	4049	PASS
173	174	0.00	2	0.8	497	PASS
174	95	50	120	91.5	58555	PASS
175	174	5	9	7.2	4244	PASS
176	174	95	101	97.0	56821	PASS
177	176	5	9	6.6	3724	PASS

m/z	Abundance
36.00	415.0
37.00	2197.0
38.00	1825.0
38.90	864.0
40.00	179.0
43.90	650.0
45.00	455.0
47.00	530.0
48.00	316.0
49.00	2042.0
50.00	9667.0
51.00	3022.0
52.00	181.0
54.90	173.0
55.90	790.0
57.10	1478.0
59.90	552.0
61.00	2733.0
62.00	2545.0
63.00	2480.0
63.90	330.0
64.90	527.0
68.00	5878.0
69.00	5330.0
70.00	437.0
71.90	301.0
73.00	2864.0
74.00	9632.0
75.00	30496.0
76.00	2635.0
77.00	343.0
77.80	294.0
78.90	1966.0
79.90	562.0
80.90	1794.0
81.80	462.0
85.90	181.0
86.90	2615.0
87.90	2628.0
90.70	241.0
92.00	1805.0
93.00	3013.0
94.00	7307.0
95.00	62920.0
96.00	4130.0
96.90	131.0
103.90	307.0
105.00	103.0
105.90	312.0
115.90	242.0
116.80	489.0
118.10	285.0
118.90	306.0
128.00	180.0
130.00	230.0
134.90	116.0
136.90	123.0
141.00	685.0
142.90	860.0
144.90	208.0
145.80	116.0
147.70	146.0
154.90	150.0
156.80	152.0
158.70	118.0
171.10	114.0
172.00	653.0
173.90	55480.0
175.00	4117.0
176.00	54136.0
177.00	3567.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
36.00	413.0
37.00	2084.0
38.00	1944.0
38.90	906.0
40.00	160.0
43.90	648.0
45.00	444.0
47.00	613.0
48.00	310.0
49.00	2089.0
50.00	10099.0
51.00	3272.0
51.90	182.0
52.80	101.0
55.00	194.0
55.90	718.0
57.00	1541.0
59.90	553.0
61.00	2949.0
62.00	2570.0
63.00	2609.0
64.00	322.0
64.90	503.0
67.10	188.0
68.00	6168.0
69.00	5709.0
70.00	505.0
71.90	322.0
73.10	2841.0
74.00	10366.0
75.00	32056.0
76.00	2781.0
77.00	411.0
77.90	292.0
78.90	2102.0
79.90	640.0
80.90	1813.0
81.80	493.0
85.90	149.0
86.90	2633.0
87.90	2931.0
90.80	224.0
92.00	1856.0
93.00	3105.0
94.00	7658.0
95.00	66216.0
96.00	4176.0
97.00	153.0
103.80	299.0
106.00	344.0
115.90	230.0
116.80	482.0
118.00	255.0
118.90	356.0
128.00	203.0
129.90	284.0
134.80	118.0
136.80	113.0
141.00	721.0
142.90	841.0
144.90	191.0
145.80	120.0
147.80	133.0
154.90	187.0
156.80	157.0
158.70	111.0
170.70	107.0
171.10	111.0
171.90	769.0
173.10	779.0
174.00	60424.0
175.00	4373.0
176.00	58752.0
177.00	3815.0
177.90	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

m/z	Abundance
35.90	393.0
37.00	1953.0
38.00	1885.0
38.90	880.0
40.00	166.0
44.00	625.0
45.00	431.0
47.00	660.0
48.00	272.0
49.00	1979.0
50.00	9696.0
51.00	3101.0
51.90	130.0
55.00	186.0
56.00	665.0
57.00	1593.0
59.90	485.0
61.00	2874.0
62.00	2455.0
63.00	2346.0
64.10	331.0
64.90	479.0
67.10	210.0
68.00	5985.0
69.00	5722.0
70.00	519.0
71.90	336.0
73.10	2623.0
74.00	10197.0
75.00	30544.0
76.00	2669.0
76.90	408.0
77.90	316.0
79.00	2100.0
79.90	640.0
80.90	1780.0
81.80	538.0
86.00	113.0
87.00	2464.0
87.90	2812.0
90.90	226.0
91.90	1723.0
93.00	2937.0
94.00	7462.0
95.00	62848.0
96.00	3840.0
97.10	151.0
103.80	301.0
105.90	329.0
116.00	198.0
116.90	449.0
118.00	207.0
118.90	401.0
127.70	189.0
128.10	209.0
128.80	128.0
129.80	329.0
134.80	137.0
136.80	100.0
140.90	664.0
143.00	752.0
144.80	160.0
145.10	167.0
145.70	122.0
148.00	121.0
149.80	113.0
154.90	188.0
156.90	179.0
159.10	110.0
171.00	126.0
171.90	913.0
173.00	712.0
174.00	59760.0
175.00	4243.0
176.00	57576.0
177.00	3790.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96

Scan 2800 (10.043 min): VV020465.D\data.ms
BFB96

m/z	Abundance
40.00	155.0
43.90	267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB96