


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV030819\
 Data File : VV009540.D
 Acq On : 08 Mar 2019 13:59
 Operator : SY/MD
 Sample : BFB72
 Misc : 5.00G/10ML/MSVOA_V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB72

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM030519S.M
 Title : VOC Analysis
 Last Update : Tue Mar 12 04:11:52 2019

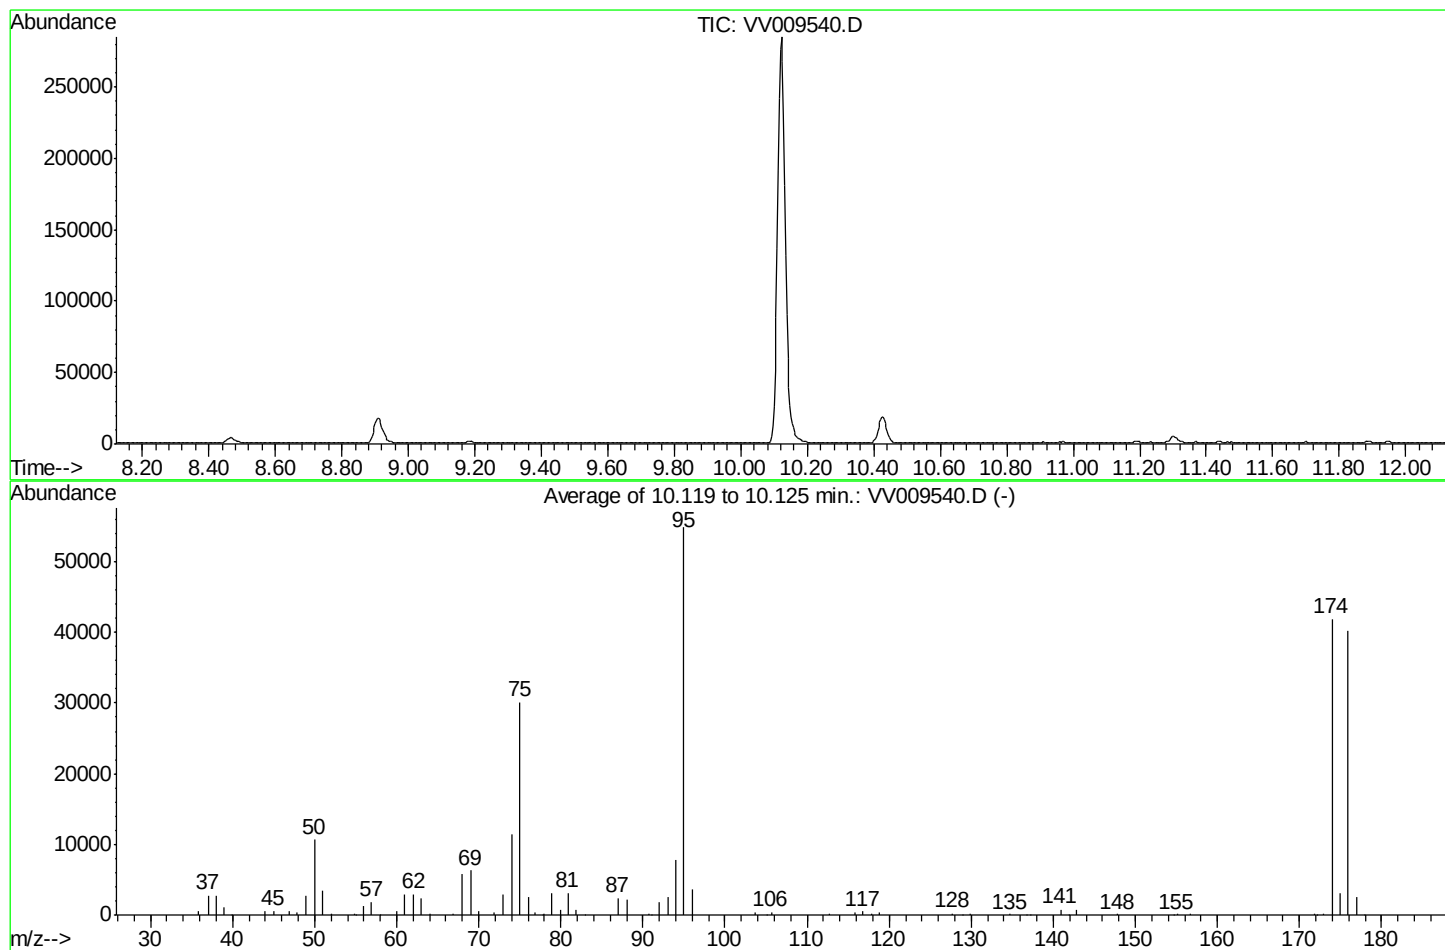

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	10661	PASS
75	95	30	80	54.8	30082	PASS
95	95	100	100	100.0	54874	PASS
96	95	5	9	6.8	3714	PASS
173	174	0.00	2	0.5	203	PASS
174	95	50	120	76.4	41933	PASS
175	174	5	9	7.4	3092	PASS
176	174	95	101	96.1	40288	PASS
177	176	5	9	6.2	2485	PASS

m/z	Abundance
39.90	658.0
44.00	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	473.0
37.00	2546.0
38.00	2538.0
39.00	915.0
39.90	669.0
44.00	632.0
45.00	583.0
47.00	553.0
47.90	291.0
49.00	2625.0
50.00	9922.0
51.00	3372.0
52.00	189.0
55.00	134.0
56.00	1287.0
57.00	1791.0
60.00	587.0
61.00	2791.0
62.00	2685.0
63.00	2319.0
64.00	240.0
67.00	200.0
68.00	5557.0
69.00	5904.0
70.00	539.0
71.80	286.0
73.00	2888.0
74.00	10732.0
75.00	29256.0
76.00	2431.0
76.90	359.0
78.00	373.0
78.90	3013.0
80.00	732.0
80.90	3072.0
81.90	669.0
87.00	2394.0
88.00	2202.0
91.00	289.0
92.00	1695.0
93.00	2611.0
94.00	7466.0
95.00	52992.0
96.00	3596.0
103.70	363.0
105.70	332.0
112.80	182.0
115.90	258.0
116.80	523.0
117.90	235.0
118.90	463.0
127.70	230.0
129.80	179.0
134.70	114.0
136.70	147.0
141.00	762.0
141.90	115.0
142.80	636.0
147.90	147.0
154.70	105.0
155.10	113.0
156.70	164.0
172.10	283.0
174.00	40864.0
174.90	2827.0
175.90	40168.0
176.90	2512.0
177.90	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	478.0
37.00	2932.0
38.00	2737.0
39.00	1078.0
39.90	671.0
44.00	700.0
45.00	618.0
46.90	628.0
47.90	310.0
49.00	2836.0
50.00	10994.0
51.00	3573.0
52.00	184.0
54.80	144.0
56.00	1320.0
57.00	1868.0
58.00	112.0
59.90	635.0
61.00	2917.0
62.00	2999.0
63.00	2468.0
64.00	245.0
66.90	196.0
68.00	6047.0
69.00	6515.0
70.10	538.0
71.80	293.0
73.00	2907.0
74.00	11802.0
75.00	30864.0
76.00	2694.0
76.80	426.0
78.00	355.0
78.90	3150.0
80.00	841.0
80.90	3205.0
81.90	717.0
86.90	2479.0
88.00	2184.0
90.80	297.0
92.00	1864.0
93.00	2672.0
94.00	8079.0
95.00	56488.0
96.00	3839.0
103.70	328.0
105.10	114.0
105.70	397.0
112.80	164.0
115.90	311.0
116.80	473.0
117.90	270.0
118.90	455.0
127.70	236.0
129.80	189.0
134.70	122.0
136.80	125.0
140.90	790.0
141.90	102.0
142.90	665.0
147.80	124.0
155.10	136.0
156.70	144.0
171.90	238.0
174.00	43448.0
174.90	3101.0
175.90	41656.0
177.00	2549.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72

m/z	Abundance
35.90	473.0
37.00	2926.0
38.00	2701.0
39.00	1071.0
39.90	650.0
44.00	703.0
45.00	654.0
46.90	660.0
47.90	314.0
49.00	2724.0
50.00	11067.0
51.00	3408.0
52.10	166.0
54.80	172.0
55.90	1207.0
56.90	1884.0
58.00	121.0
59.90	597.0
61.00	2787.0
62.10	3068.0
63.00	2348.0
64.00	238.0
66.80	154.0
68.00	5895.0
69.00	6439.0
70.10	503.0
72.00	314.0
73.00	2662.0
74.00	11505.0
75.00	30128.0
76.00	2630.0
76.80	442.0
77.80	288.0
78.90	3052.0
79.90	866.0
80.90	3079.0
81.90	713.0
82.90	122.0
86.90	2365.0
88.00	2000.0
90.80	318.0
92.00	1768.0
93.00	2482.0
94.00	7718.0
95.00	55144.0
96.00	3709.0
103.70	250.0
105.70	380.0
112.70	104.0
115.90	301.0
116.90	398.0
117.90	300.0
118.80	405.0
127.70	208.0
128.90	133.0
129.90	196.0
134.80	111.0
137.20	109.0
140.90	802.0
142.90	677.0
147.80	117.0
155.10	144.0
171.90	198.0
173.00	610.0
174.00	41488.0
175.00	3350.0
175.90	39040.0
177.00	2395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB72