
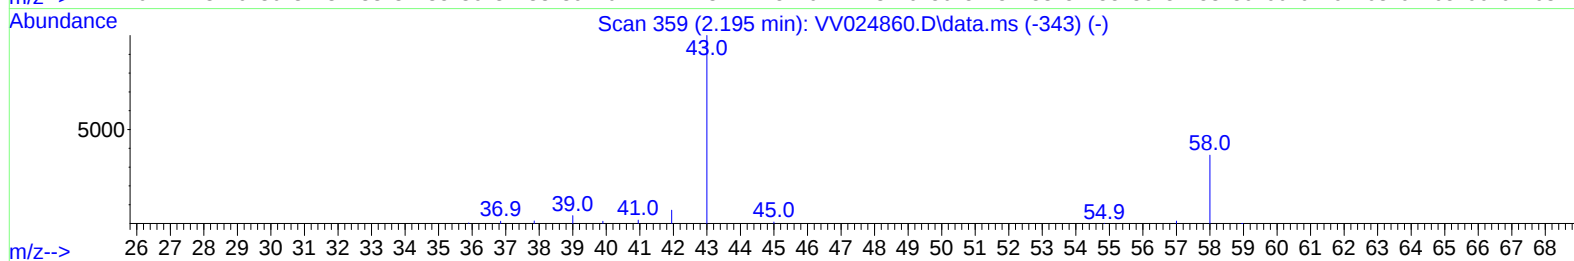
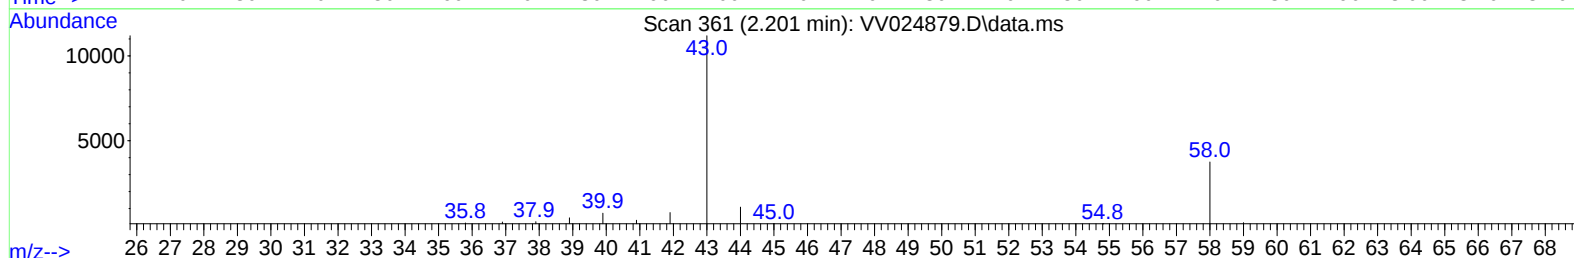


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV030822\  
 Data File : VV024879.D  
 Acq On : 09 Mar 2022 11:06  
 Operator : SY/MD  
 Sample : VSTDCCC005  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 10 04:47:10 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR021722WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Wed Mar 09 05:01:56 2022  
 Response via : Initial Calibration

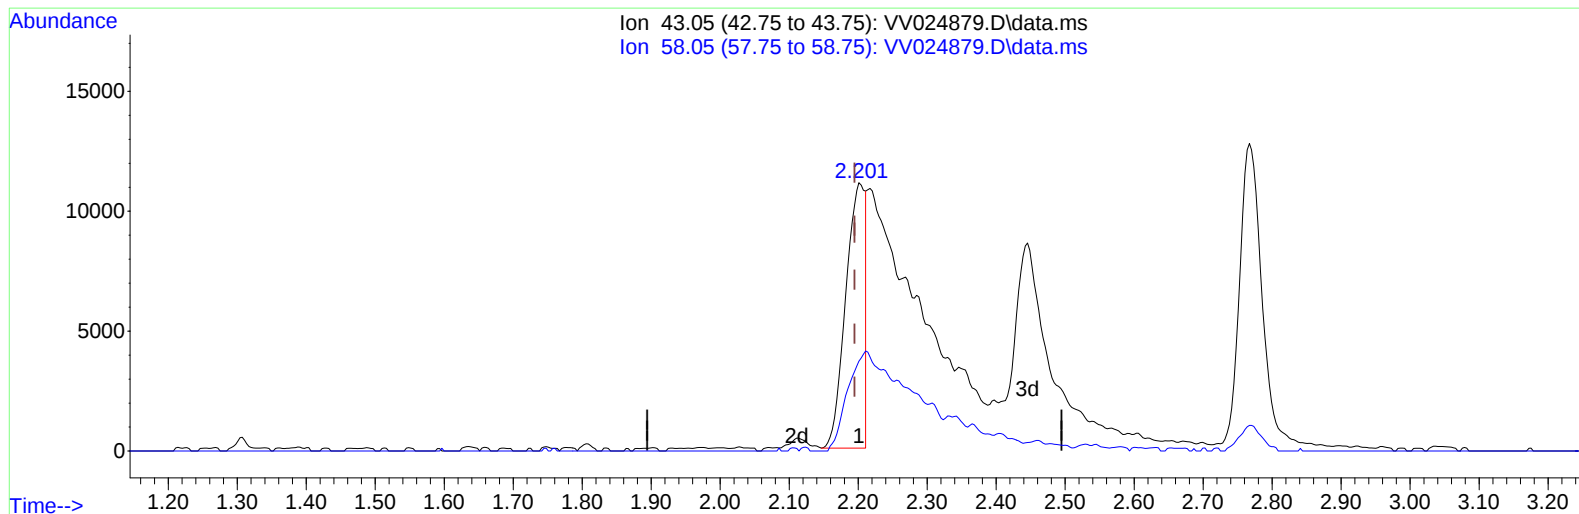

TIC: VV024879.D\data.ms

**(13) Acetone (T)****2.201min (+ 0.007) 11.11 ug/L****response 21858**

| Ion   | Exp%   | Act%    |
|-------|--------|---------|
| 43.05 | 100.00 | 100.00  |
| 58.05 | 31.80  | 106.89# |
| 0.00  | 0.00   | 0.00    |
| 0.00  | 0.00   | 0.00    |