
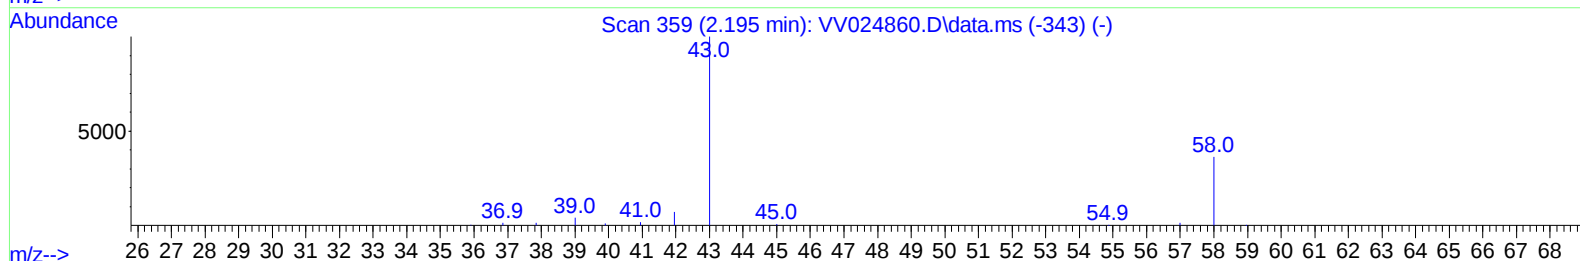
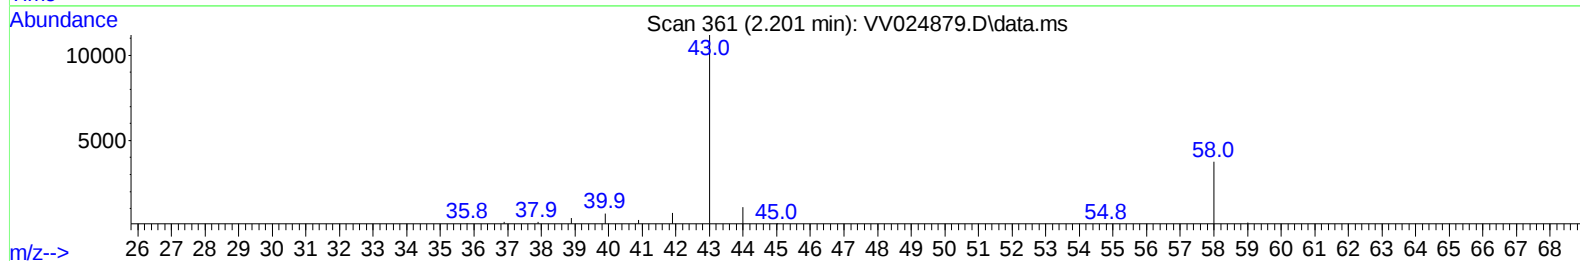


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024879.D
Acq On : 09 Mar 2022 11:06
Operator : SY/MD
Sample : VSTDCCC005
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 10 04:47:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 09 05:01:56 2022
Response via : Initial Calibration

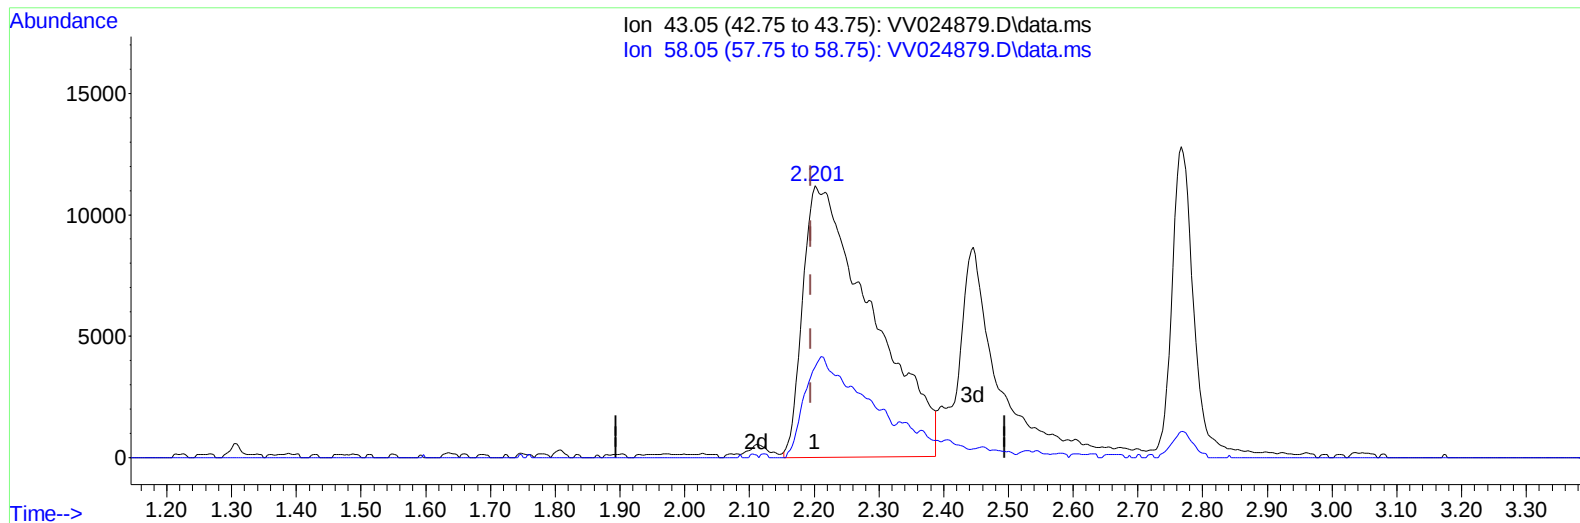

TIC: VV024879.D\data.ms

(13) Acetone (T)

2.201min (+ 0.007) 41.96 ug/L m

response 82548

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.80	28.30
0.00	0.00	0.00
0.00	0.00	0.00