

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030822\
 Data File : VW024862.D
 Acq On : 08 Mar 2022 11:09
 Operator : SY/MD
 Sample : N1811-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDA0

Quant Time: Mar 09 05:02:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 09 05:01:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	209256	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	189358	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	82673	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	69996	3.944	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.800%	
7) Chloroethane-d5	1.564	69	60248	4.138	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	82.800%	
11) 1,1-Dichloroethene-d2	2.105	63	91037	2.799	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	56.000%#	
20) 2-Butanone-d5	3.899	46	118175	46.613	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	93.220%	
24) Chloroform-d	4.343	84	126128	4.554	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
26) 1,2-Dichloroethane-d4	5.027	65	57104	4.626	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.600%	
32) Benzene-d6	5.043	84	264779	4.847	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.000%	
36) 1,2-Dichloropropane-d6	6.063	67	80401	5.001	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.000%	
41) Toluene-d8	7.310	98	225117	4.535	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.619	79	26692	4.984	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.600%	
46) 2-Hexanone-d5	8.085	63	93447	44.344	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	88.680%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	43849	4.526	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	90.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	68966	4.821	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.400%	
Target Compounds						
25) Chloroform	4.368	83	6021	0.198	ug/L	Qvalue 93




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024862.D
Acq On : 08 Mar 2022 11:09
Operator : SY/MD
Sample : N1811-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDA0

Quant Time: Mar 09 05:02:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 09 05:01:56 2022
Response via : Initial Calibration

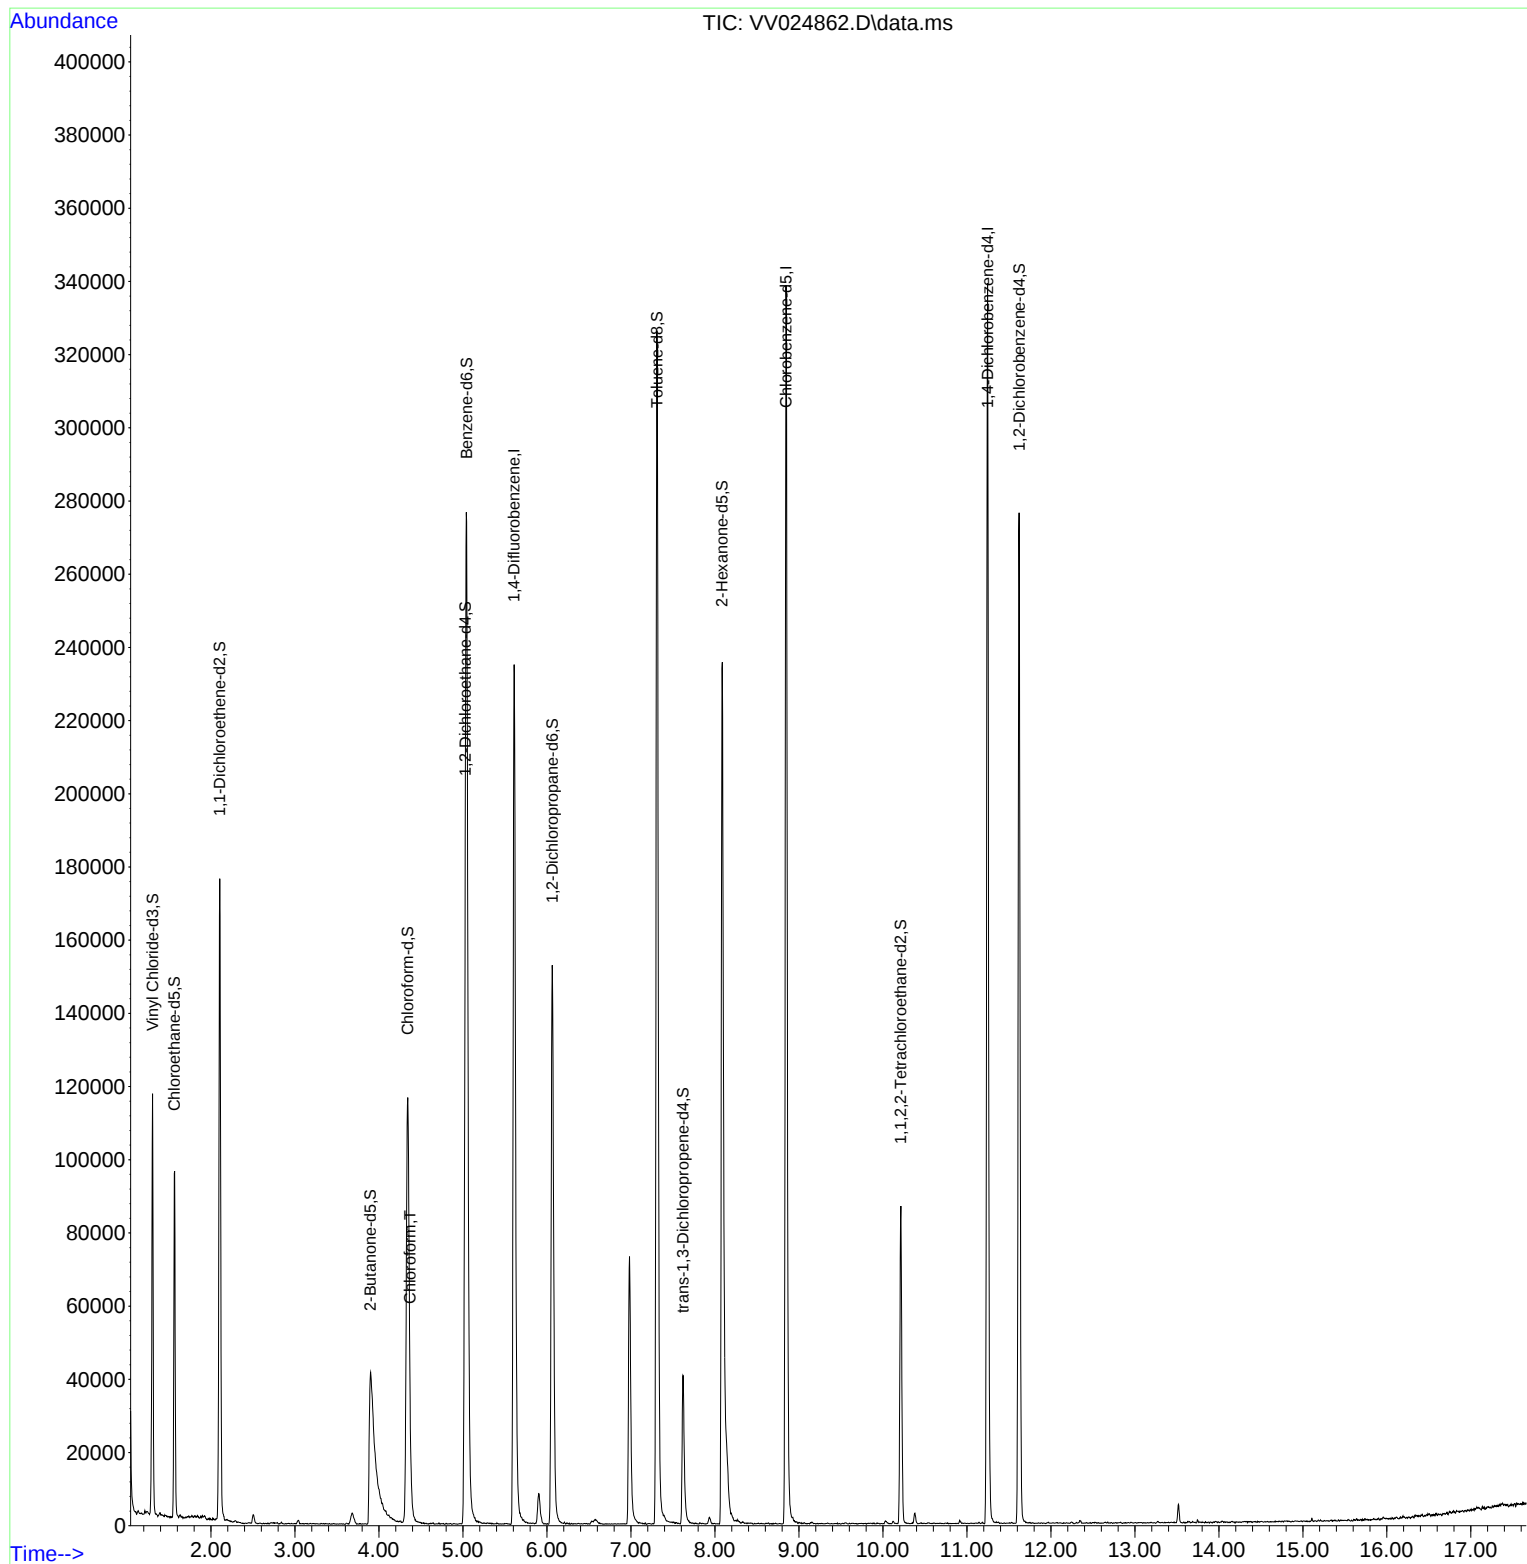

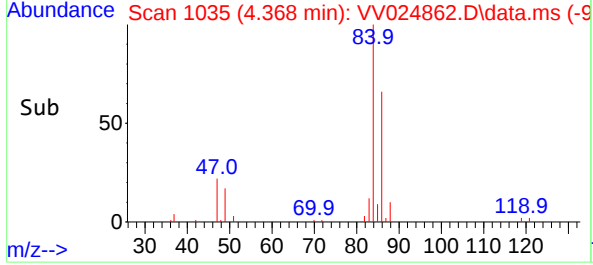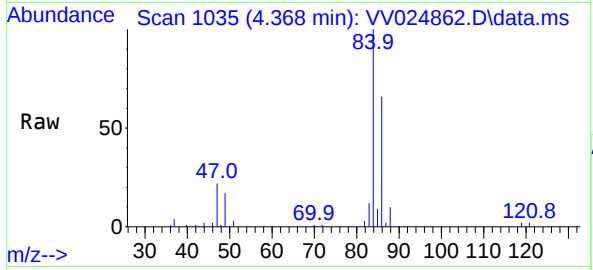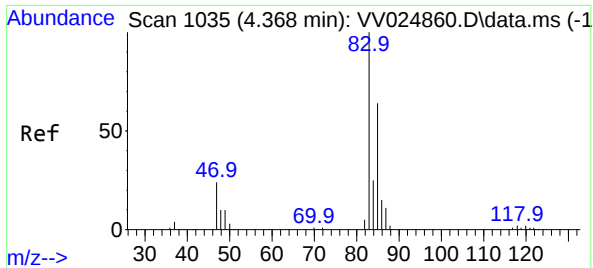

#25
 Chloroform
 Concen: 0.198 ug/L
 RT: 4.368 min Scan# 10
 Delta R.T. 0.000 min
 Lab File: VV024862.D
 Acq: 08 Mar 2022 11:09

Tgt Ion: 83 Resp: 6021
 Ion Ratio Lower Upper
 83 100
 85 70.8 45.5 84.5

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDA0

