

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030822\
 Data File : VW024863.D
 Acq On : 08 Mar 2022 11:33
 Operator : SY/MD
 Sample : N1811-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDA8

Quant Time: Mar 09 05:02:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 09 05:01:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	202637	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	186549	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	82540	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70843	4.122	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	82.400%	
7) Chloroethane-d5	1.568	69	61454	4.358	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	87.200%	
11) 1,1-Dichloroethene-d2	2.108	63	94085	2.987	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	59.800%#	
20) 2-Butanone-d5	3.899	46	127165	51.798	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	103.600%	
24) Chloroform-d	4.349	84	130668	4.872	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.400%	
26) 1,2-Dichloroethane-d4	5.034	65	58433	4.888	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
32) Benzene-d6	5.050	84	274821	5.107	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.200%	
36) 1,2-Dichloropropane-d6	6.069	67	83217	5.254	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.000%	
41) Toluene-d8	7.313	98	232566	4.756	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.200%	
43) trans-1,3-Dichloroprop...	7.622	79	27343	5.182	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	103.600%	
46) 2-Hexanone-d5	8.088	63	97195	46.817	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.640%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46759	4.899	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	72503	5.077	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.600%	
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	3.918	96	2162	0.133	ug/L	96
25) Chloroform	4.375	83	2683	0.091	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024863.D
Acq On : 08 Mar 2022 11:33
Operator : SY/MD
Sample : N1811-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDA8

Quant Time: Mar 09 05:02:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 09 05:01:56 2022
Response via : Initial Calibration

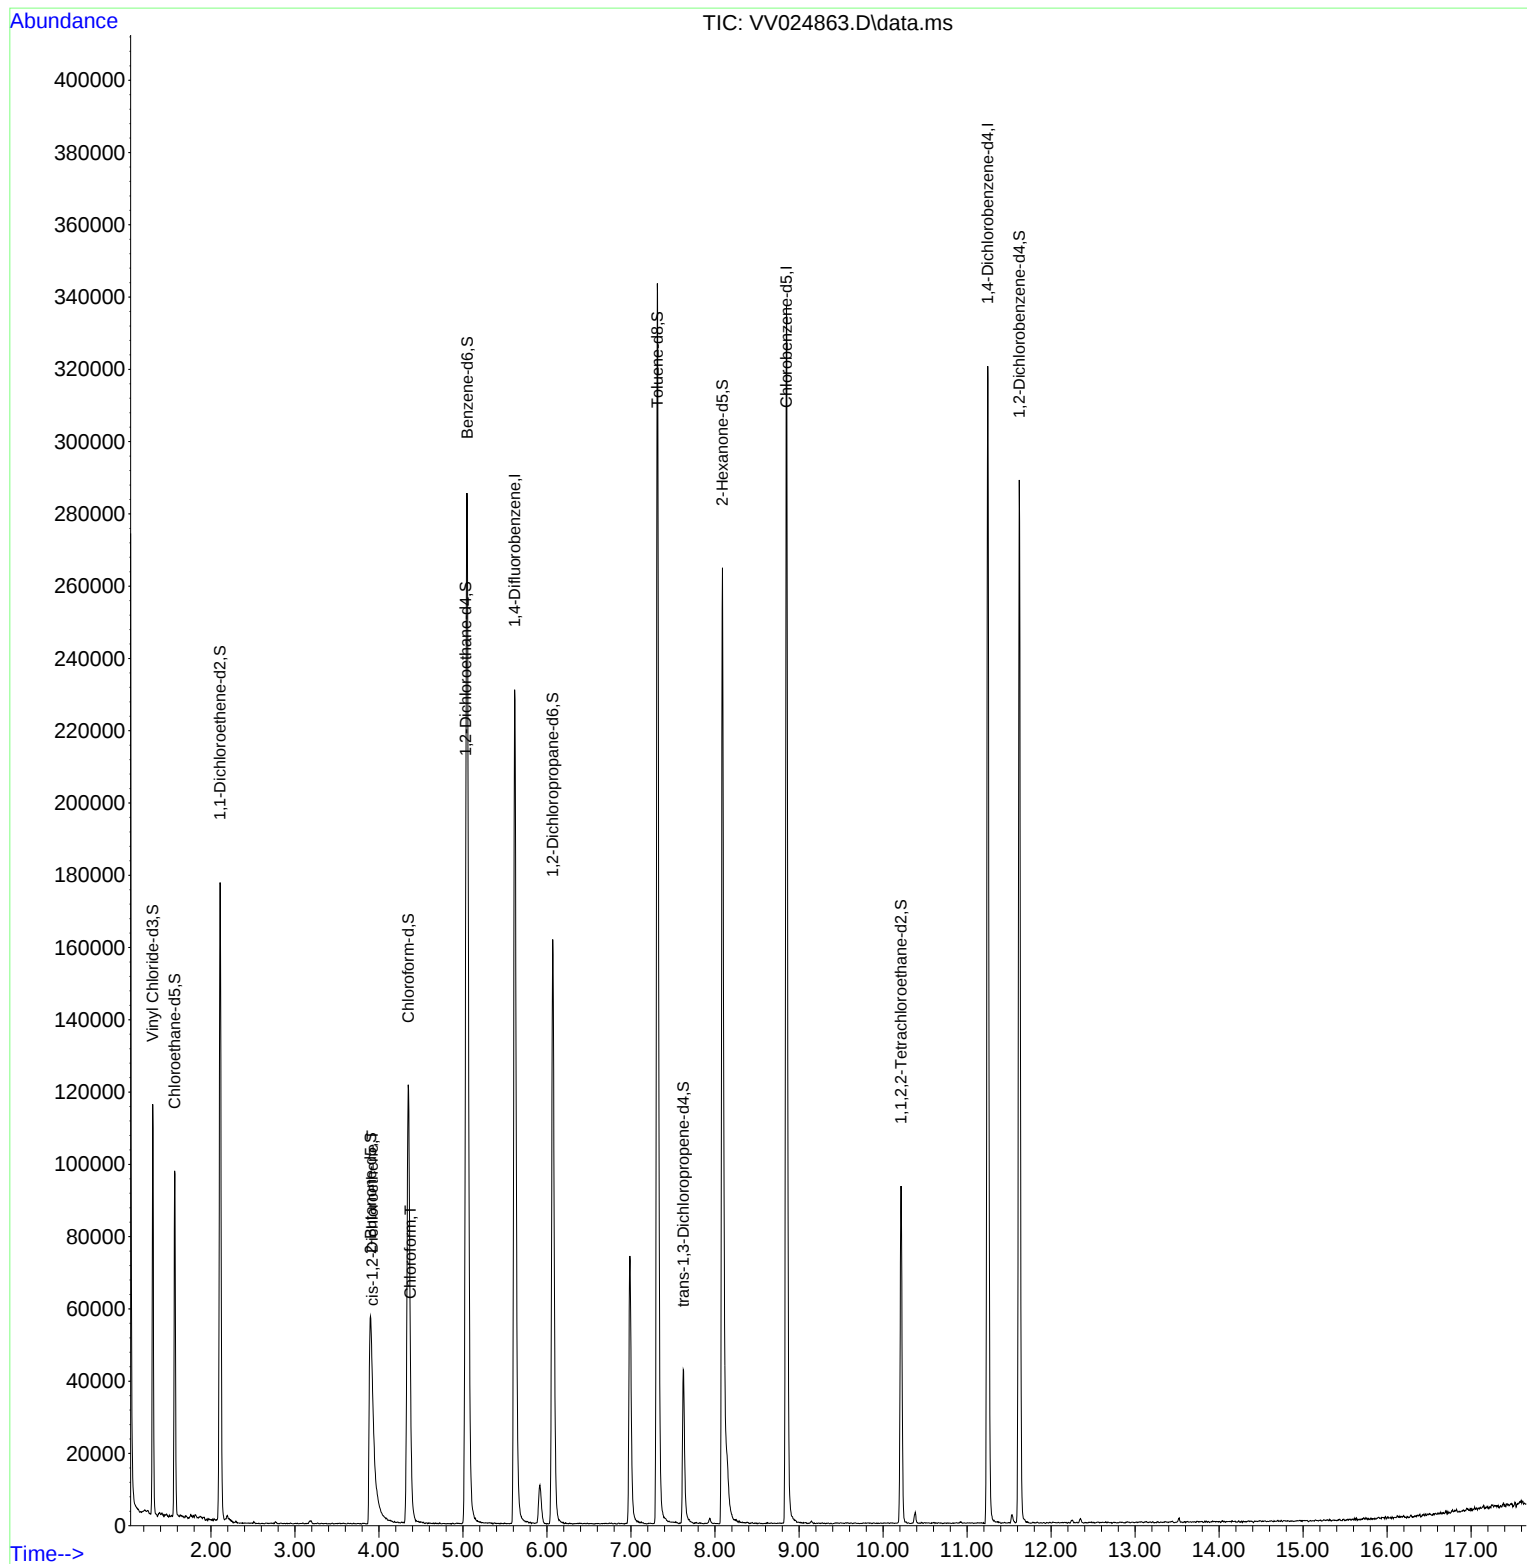

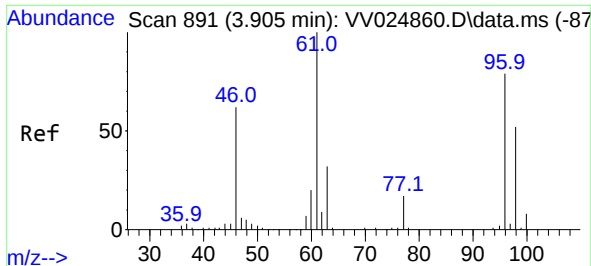

#22

cis-1,2-Dichloroethene

Concen: 0.133 ug/L

RT: 3.918 min Scan# 891

Delta R.T. 0.013 min

Lab File: VV024863.D

Acq: 08 Mar 2022 11:33

Instrument :

MSVOA_V

ClientSampleId :

GBDA8





Tgt Ion: 96 Resp: 2162

Ion Ratio Lower Upper

96 100

61 123.6 89.7 166.5

68 0.0 0.0 0.0

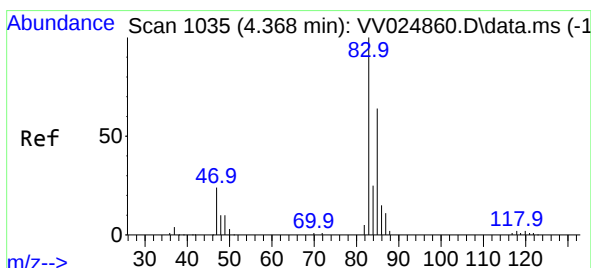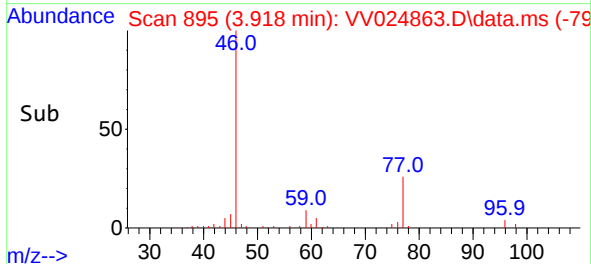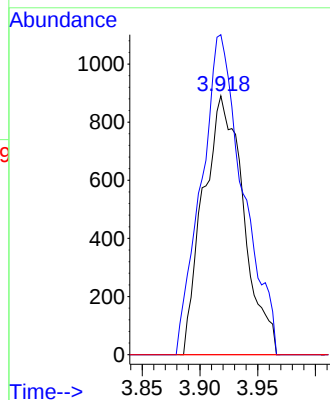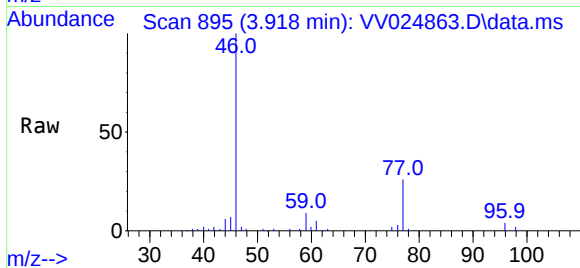

#25

Chloroform

Concen: 0.091 ug/L

RT: 4.375 min Scan# 1037

Delta R.T. 0.007 min

Lab File: VV024863.D

Acq: 08 Mar 2022 11:33

Tgt Ion: 83 Resp: 2683

Ion Ratio Lower Upper

83 100

85 68.7 45.5 84.5

