

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030822\
 Data File : VW024865.D
 Acq On : 08 Mar 2022 12:19
 Operator : SY/MD
 Sample : N1811-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDB1

Quant Time: Mar 09 05:03:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 09 05:01:56 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	211818	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	192132	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	84593	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70389	3.918	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	78.400%	
7) Chloroethane-d5	1.568	69	62239	4.223	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.400%	
11) 1,1-Dichloroethene-d2	2.108	63	91284	2.773	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	55.400%#	
20) 2-Butanone-d5	3.899	46	127588	49.718	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	99.440%	
24) Chloroform-d	4.352	84	132125	4.713	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
26) 1,2-Dichloroethane-d4	5.034	65	58831	4.708	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	94.200%	
32) Benzene-d6	5.050	84	271014	4.889	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.800%	
36) 1,2-Dichloropropane-d6	6.069	67	83313	5.108	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.200%	
41) Toluene-d8	7.317	98	233449	4.635	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
43) trans-1,3-Dichloroprop...	7.625	79	26491	4.875	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	97.600%	
46) 2-Hexanone-d5	8.088	63	98100	45.880	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.760%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	46805	4.761	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	95.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	72670	4.965	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.200%	
Target Compounds						
22) cis-1,2-Dichloroethene	3.924	96	1333	0.078	ug/L	80
34) Trichloroethene	5.918	95	26823	1.557	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024865.D
Acq On : 08 Mar 2022 12:19
Operator : SY/MD
Sample : N1811-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB1

Quant Time: Mar 09 05:03:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 09 05:01:56 2022
Response via : Initial Calibration

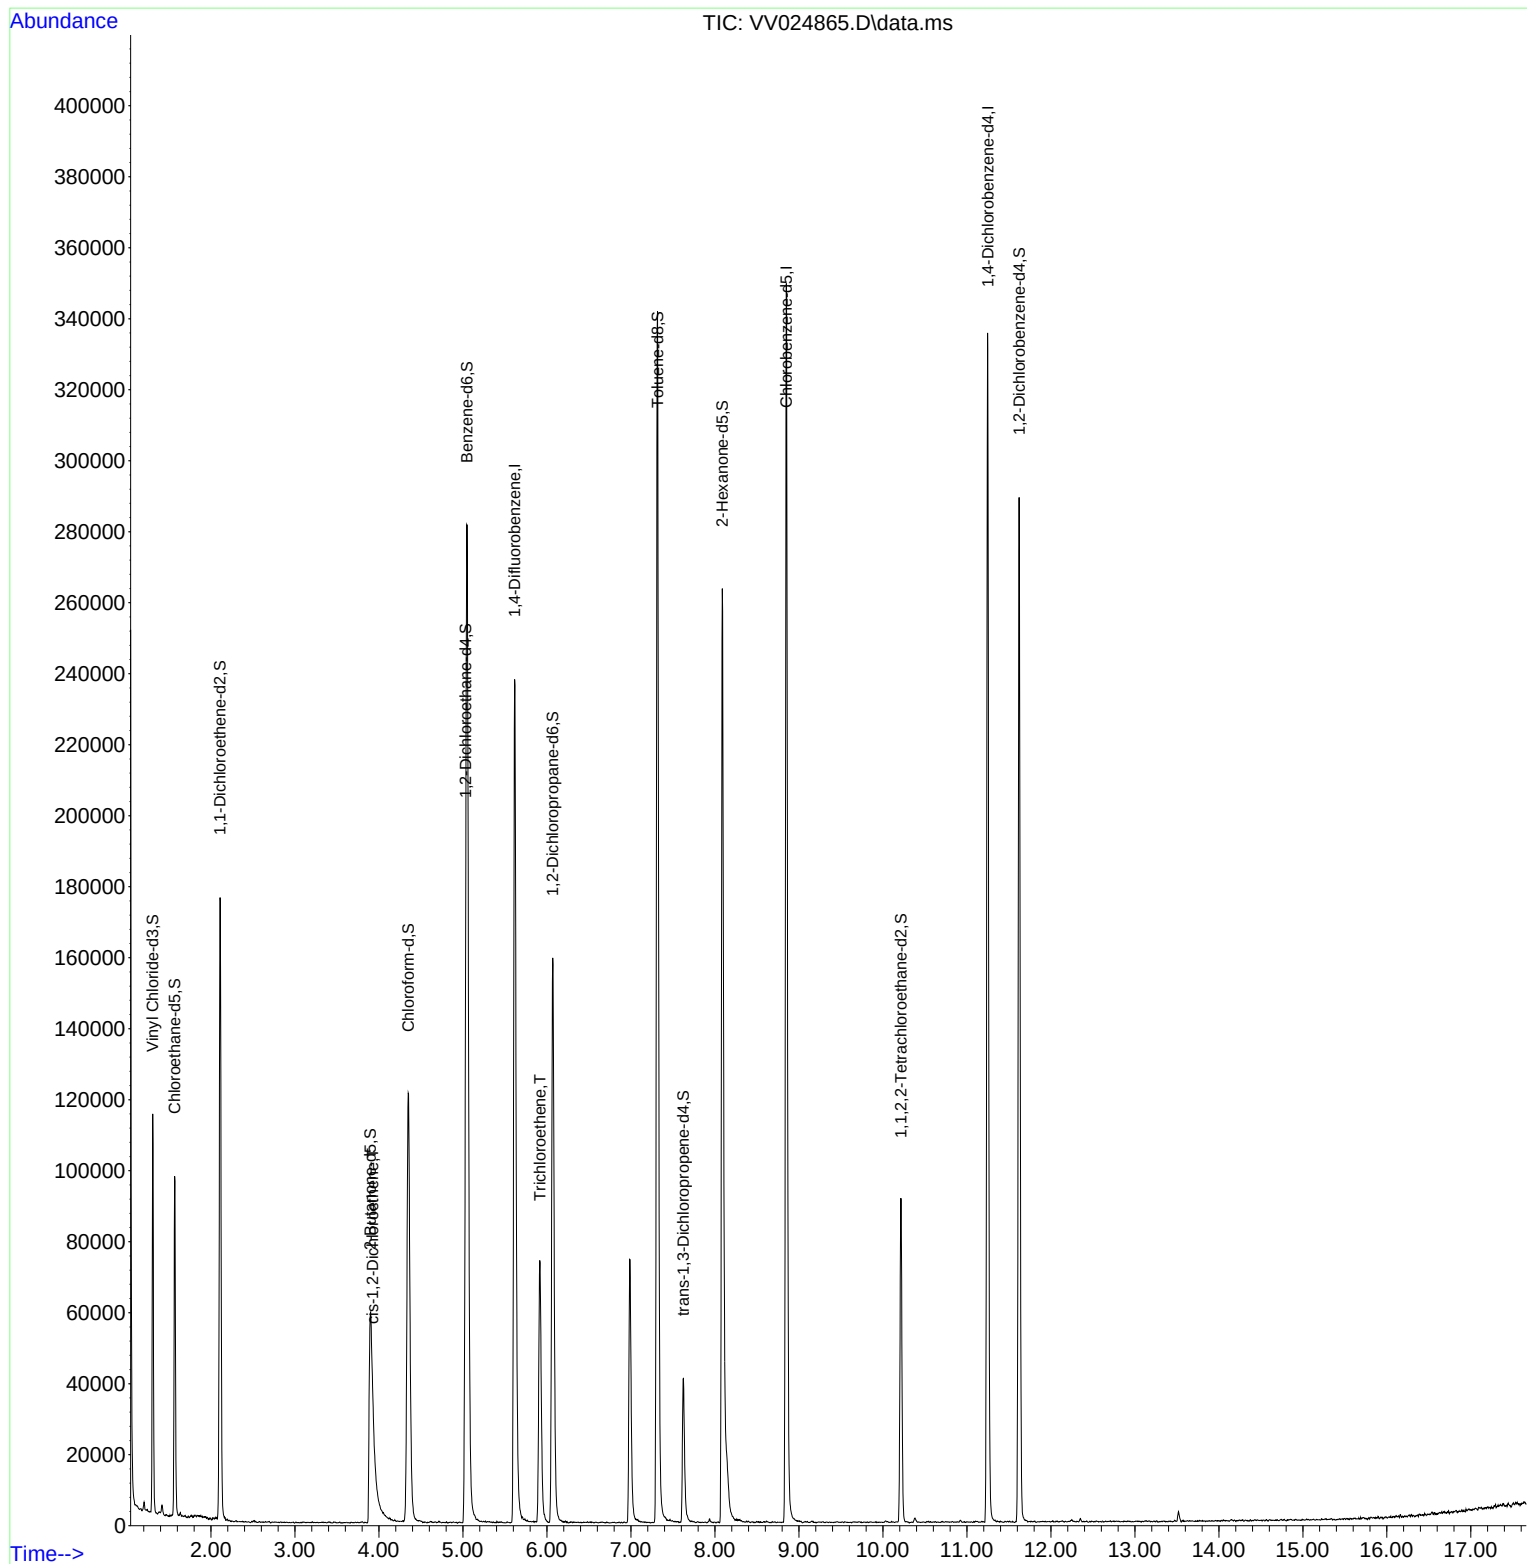

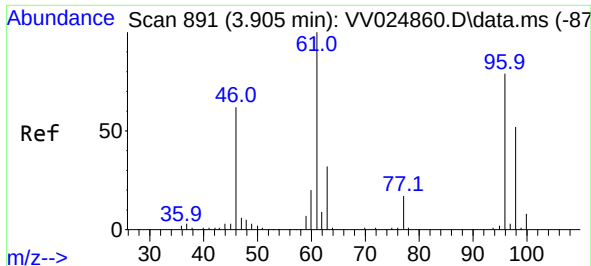

#22

cis-1,2-Dichloroethene

Concen: 0.078 ug/L

RT: 3.924 min Scan# 891

Delta R.T. 0.019 min

Lab File: VV024865.D

Acq: 08 Mar 2022 12:19

Instrument :

MSVOA_V

ClientSampleId :

GBDB1





Tgt Ion: 96 Resp: 1333

Ion Ratio Lower Upper

96 100

61 104.6 89.7 166.5

68 0.0 0.0 0.0

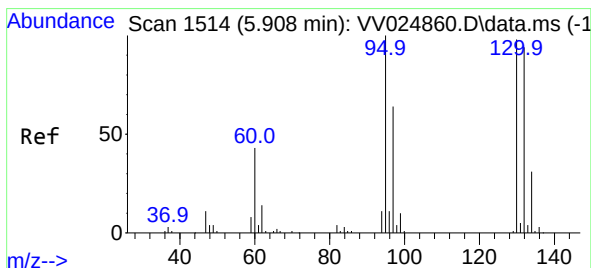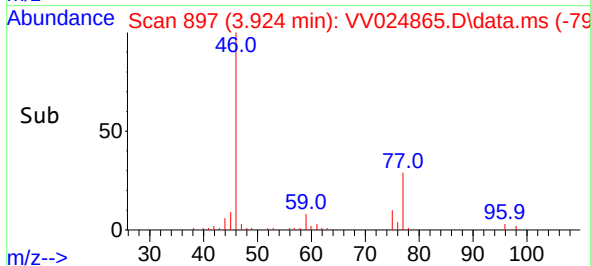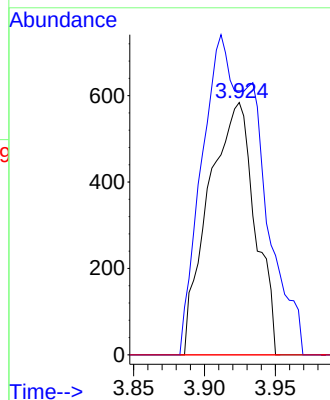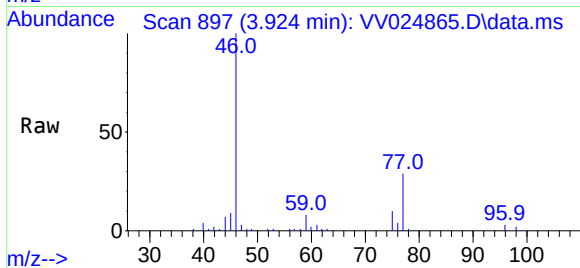

#34

Trichloroethene

Concen: 1.557 ug/L

RT: 5.918 min Scan# 1517

Delta R.T. 0.010 min

Lab File: VV024865.D

Acq: 08 Mar 2022 12:19

Tgt Ion: 95 Resp: 26823

Ion Ratio Lower Upper

95 100

97 60.6 44.2 82.0

132 87.7 62.1 115.3

130 95.3 65.8 122.2

