

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW030822\
 Data File : VW024867.D
 Acq On : 08 Mar 2022 13:06
 Operator : SY/MD
 Sample : N1811-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GBDB3

Quant Time: Mar 09 05:03:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 09 05:01:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	192999	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	175911	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	77972	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	70768	4.323	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	86.400%
7) Chloroethane-d5	1.568	69	61253	4.561	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.111	63	92080	3.069	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.400%
20) 2-Butanone-d5	3.899	46	132932	56.851	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.700%
24) Chloroform-d	4.349	84	130314	5.102	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
26) 1,2-Dichloroethane-d4	5.034	65	58927	5.176	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.600%
32) Benzene-d6	5.050	84	273448	5.388	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.800%
36) 1,2-Dichloropropane-d6	6.069	67	82256	5.508	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.200%
41) Toluene-d8	7.317	98	232189	5.035	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.800%
43) trans-1,3-Dichloroprop...	7.622	79	26736	5.374	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	107.400%
46) 2-Hexanone-d5	8.088	63	98200	50.162	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.320%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	46211	5.134	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	71905	5.330	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.600%
Target Compounds						
25) Chloroform	4.378	83	5544	0.197	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024867.D
Acq On : 08 Mar 2022 13:06
Operator : SY/MD
Sample : N1811-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GBDB3

Quant Time: Mar 09 05:03:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 09 05:01:56 2022
Response via : Initial Calibration

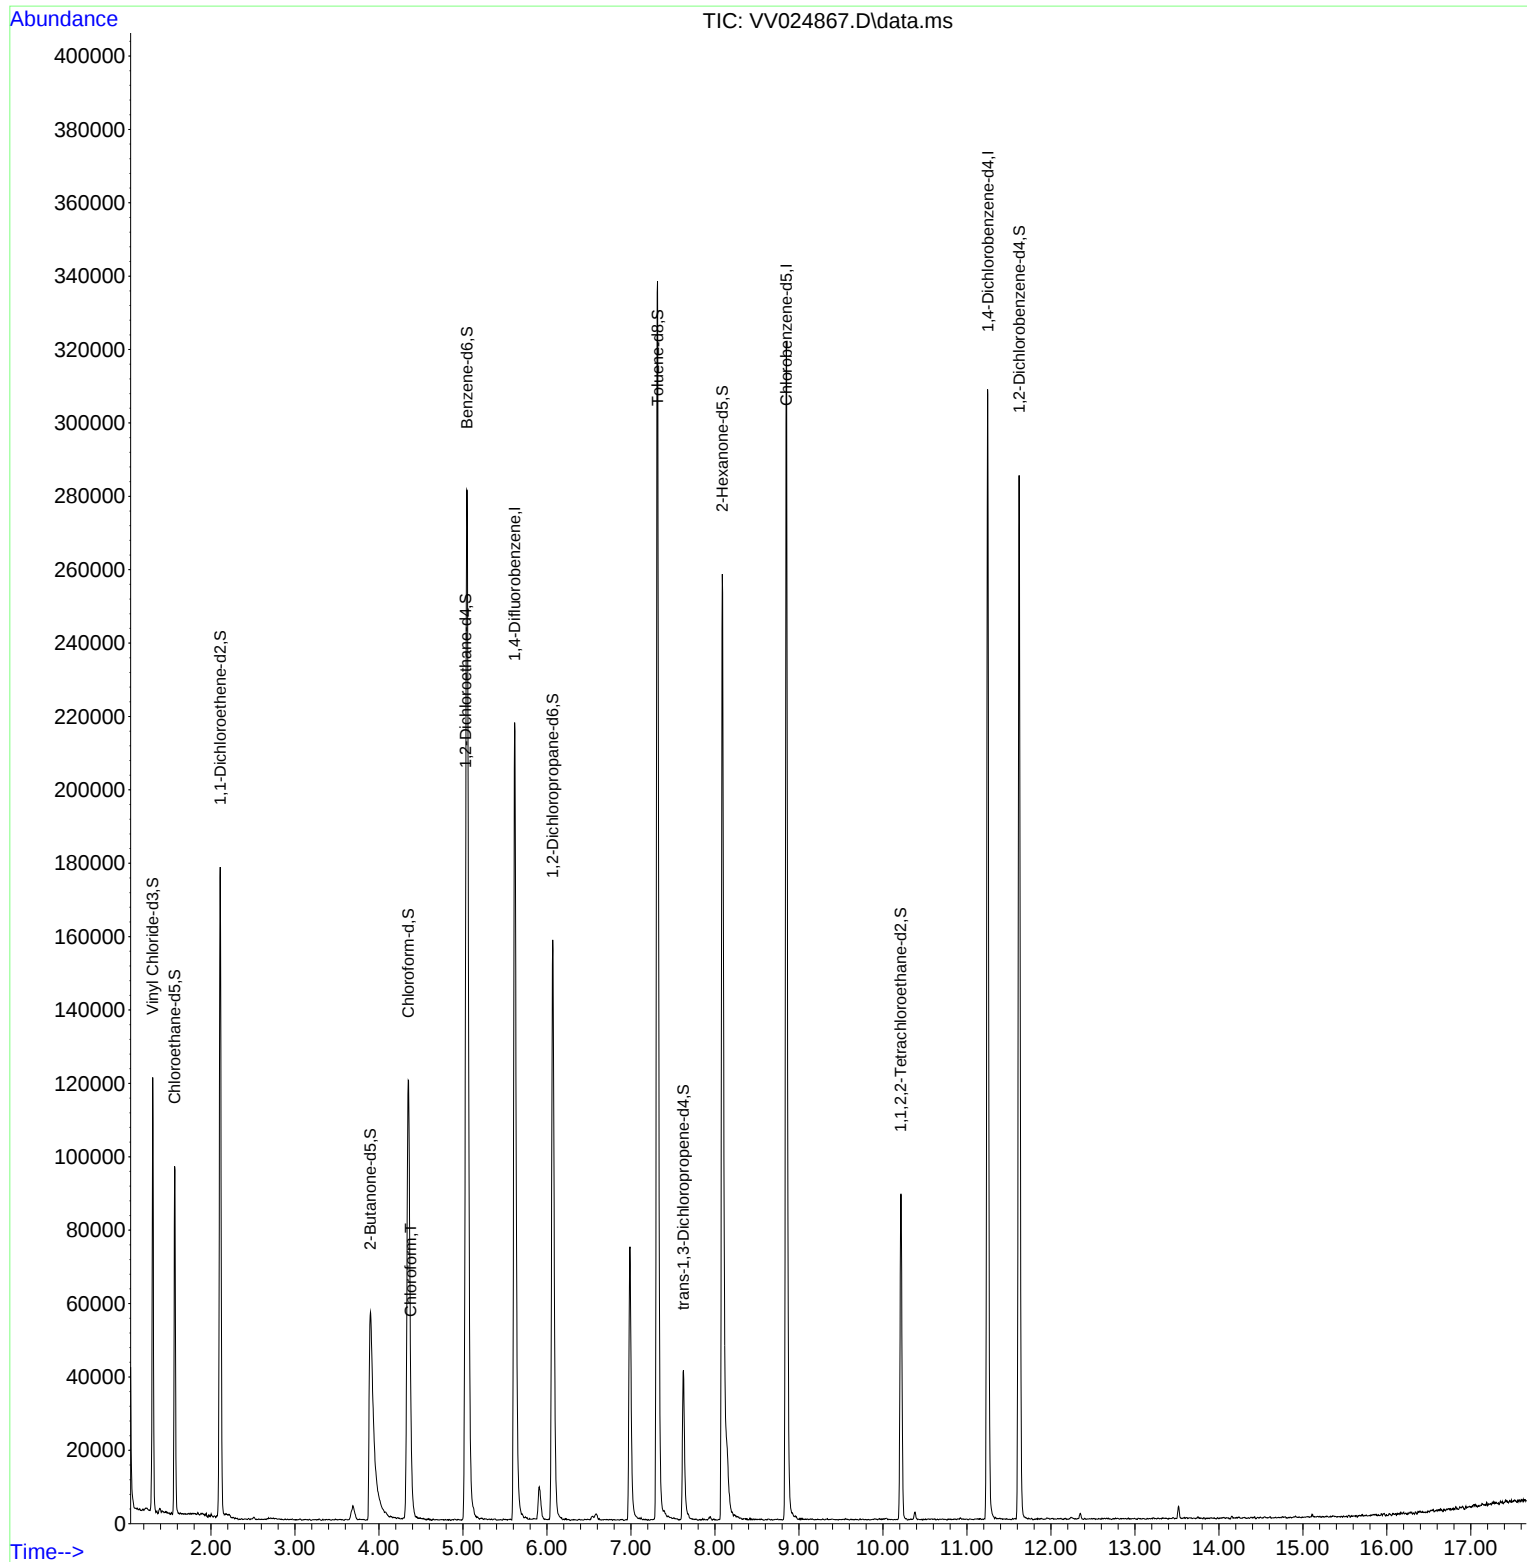

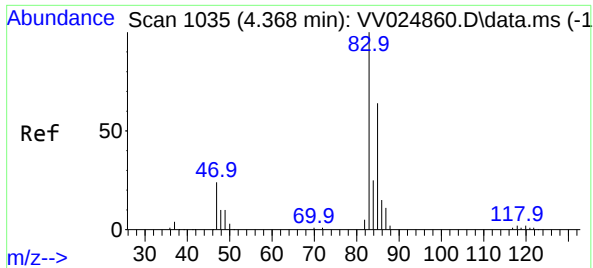

#25
Chloroform
Concen: 0.197 ug/L
RT: 4.378 min Scan# 10
Delta R.T. 0.010 min
Lab File: VV024867.D
Acq: 08 Mar 2022 13:06

Instrument :
MSVOA_V
ClientSampleId :
GBDB3

Tgt Ion: 83 Resp: 5544
Ion Ratio Lower Upper
83 100
85 64.0 45.5 84.5

