

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
 Data File : VV024876.D
 Acq On : 08 Mar 2022 16:36
 Operator : SY/MD
 Sample : N1811-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Mar 09 05:05:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Mar 09 05:01:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	181438	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	166989	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73675	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	56454	3.668	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.400%	
7) Chloroethane-d5	1.568	69	52102	4.127	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	82.600%	
11) 1,1-Dichloroethene-d2	2.108	63	72961	2.587	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	51.800%#	
20) 2-Butanone-d5	3.908	46	121032	55.060	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	110.120%	
24) Chloroform-d	4.349	84	115565	4.813	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.200%	
26) 1,2-Dichloroethane-d4	5.034	65	52426	4.898	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.000%	
32) Benzene-d6	5.050	84	231826	4.812	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.200%	
36) 1,2-Dichloropropane-d6	6.069	67	72460	5.111	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.200%	
41) Toluene-d8	7.316	98	187516	4.284	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.600%	
43) trans-1,3-Dichloroprop...	7.625	79	21026	4.452	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.091	63	94203	50.691	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	101.380%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	44062	5.157	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	61217	4.802	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.000%	
Target Compounds					Qvalue	
25) Chloroform	4.371	83	3047	0.115	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024876.D
Acq On : 08 Mar 2022 16:36
Operator : SY/MD
Sample : N1811-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Mar 09 05:05:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Mar 09 05:01:56 2022
Response via : Initial Calibration

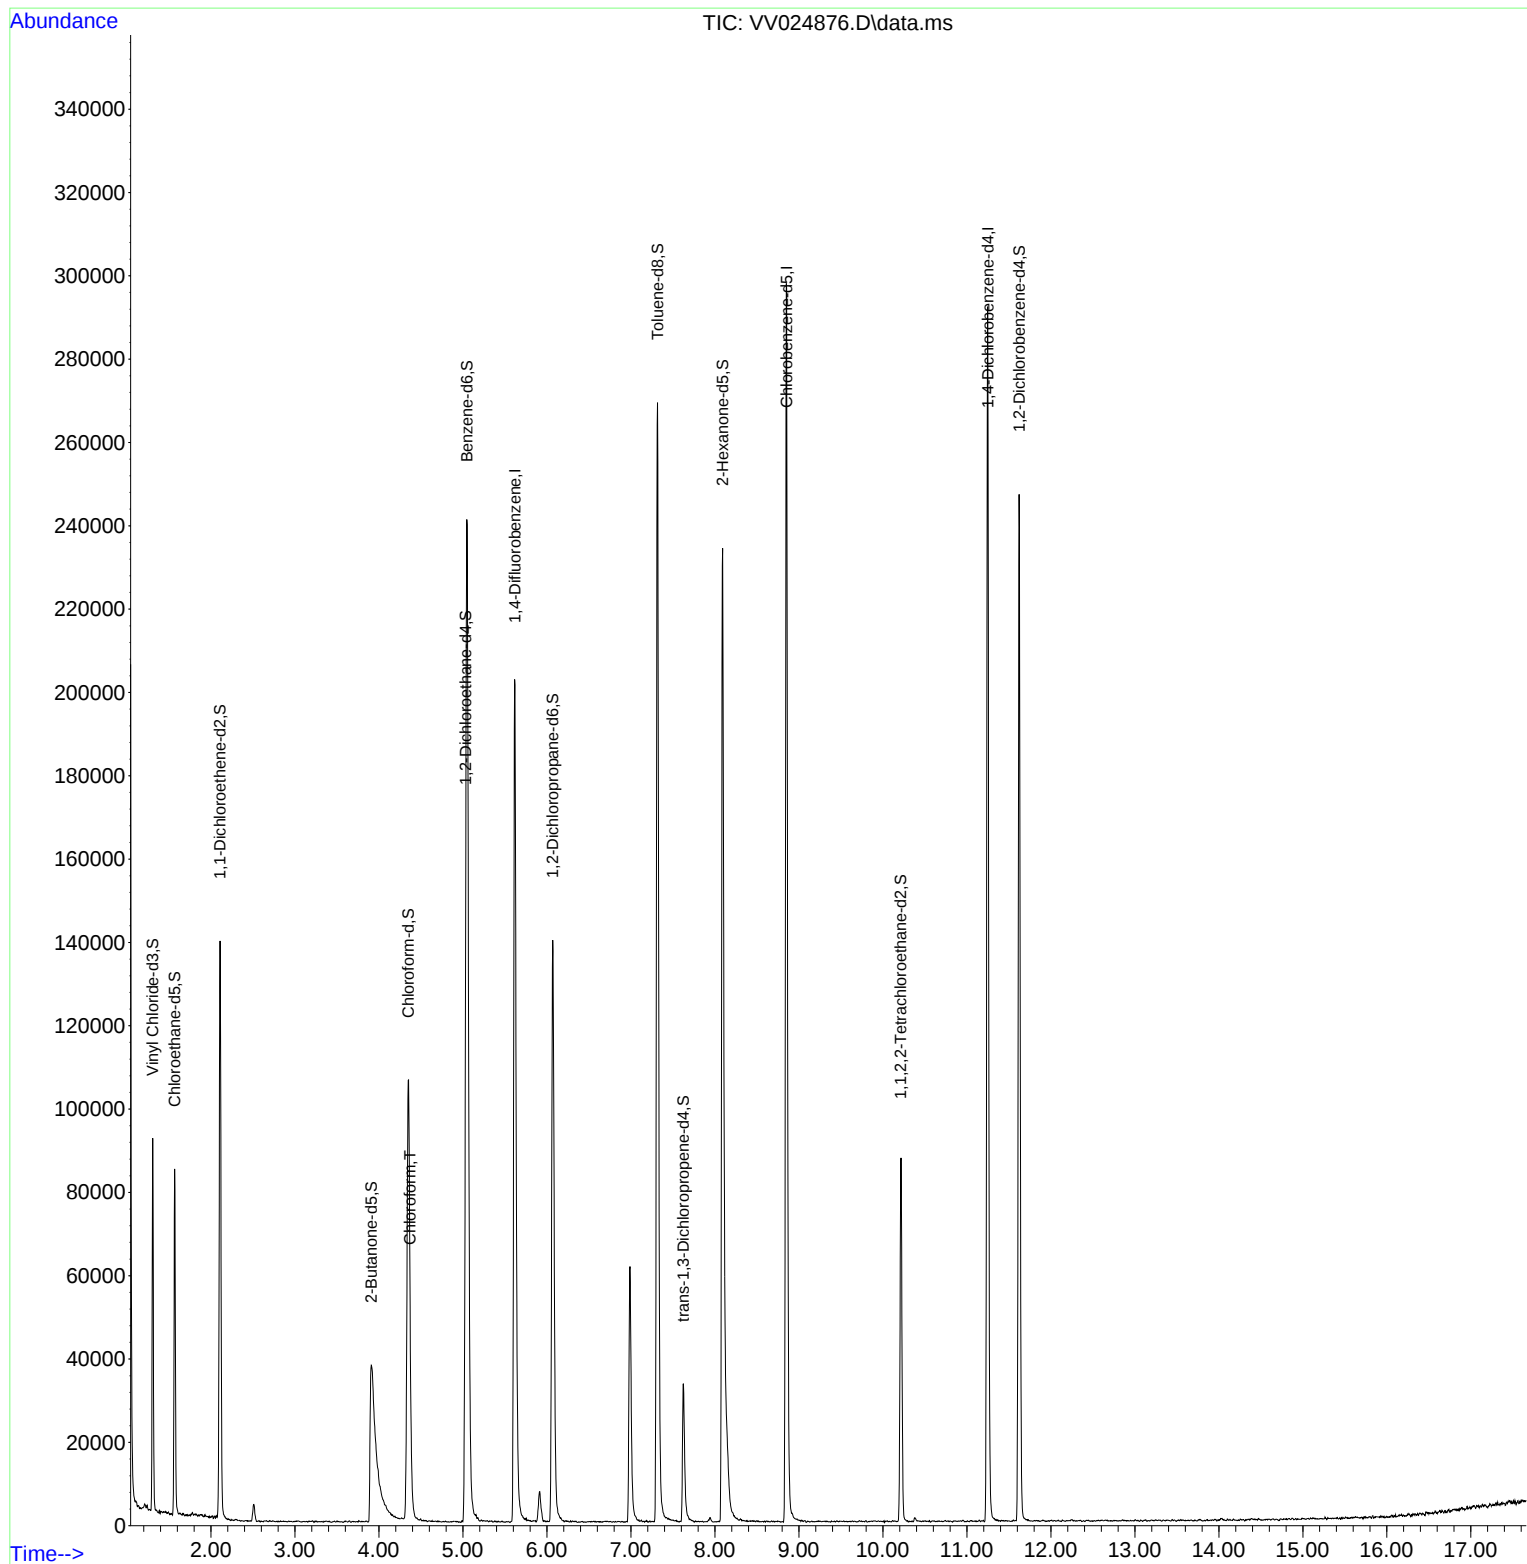

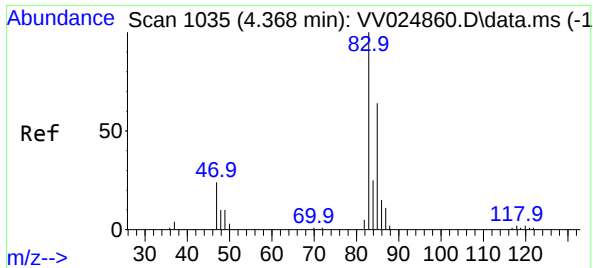

#25
Chloroform
Concen: 0.115 ug/L
RT: 4.371 min Scan# 10
Delta R.T. 0.003 min
Lab File: VV024876.D
Acq: 08 Mar 2022 16:36

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 83 Resp: 3047
Ion Ratio Lower Upper
83 100
85 75.2 45.5 84.5

