

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
 Data File : VV024871.D
 Acq On : 08 Mar 2022 14:40
 Operator : SY/MD
 Sample : VIBLK261
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK261

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV024871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	101	rVB	107456	107096	16.12%	2.070%
2	1.568	156	164	176	rBV	91113	102072	15.37%	1.973%
3	2.108	321	332	353	rVB	164346	237019	35.68%	4.582%
4	2.510	449	457	466	rBV	6726	10752	1.62%	0.208%
5	3.905	881	891	951	rBV2	42215	201637	30.36%	3.898%
6	4.349	1014	1029	1062	rBV	114468	287269	43.25%	5.553%
7	5.047	1231	1246	1277	rBV2	268047	664198	100.00%	12.840%
8	5.616	1406	1423	1453	rBV	198284	412988	62.18%	7.984%
9	5.912	1503	1515	1533	rVB5	9747	24055	3.62%	0.465%
10	6.069	1550	1564	1592	rBV	151537	313092	47.14%	6.053%
11	6.989	1837	1850	1871	rBV	71044	131601	19.81%	2.544%
12	7.317	1937	1952	1975	rBV	318571	562909	84.75%	10.882%
13	7.625	2038	2048	2070	rBV	39546	71358	10.74%	1.379%
14	8.092	2182	2193	2231	rBV	248954	509115	76.65%	9.842%
15	8.850	2418	2429	2458	rBV	295744	489817	73.75%	9.469%
16	10.214	2843	2853	2868	rBV	90458	142458	21.45%	2.754%
17	11.246	3164	3174	3199	rBV	292274	454936	68.49%	8.795%
18	11.622	3278	3291	3311	rBV	275524	433503	65.27%	8.380%
19	13.506	3864	3877	3889	rBV2	5726	9543	1.44%	0.184%
20	13.744	3943	3951	3961	rBV4	4839	7408	1.12%	0.143%




Sum of corrected areas: 5172826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024871.D
Acq On : 08 Mar 2022 14:40
Operator : SY/MD
Sample : VIBLK261
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

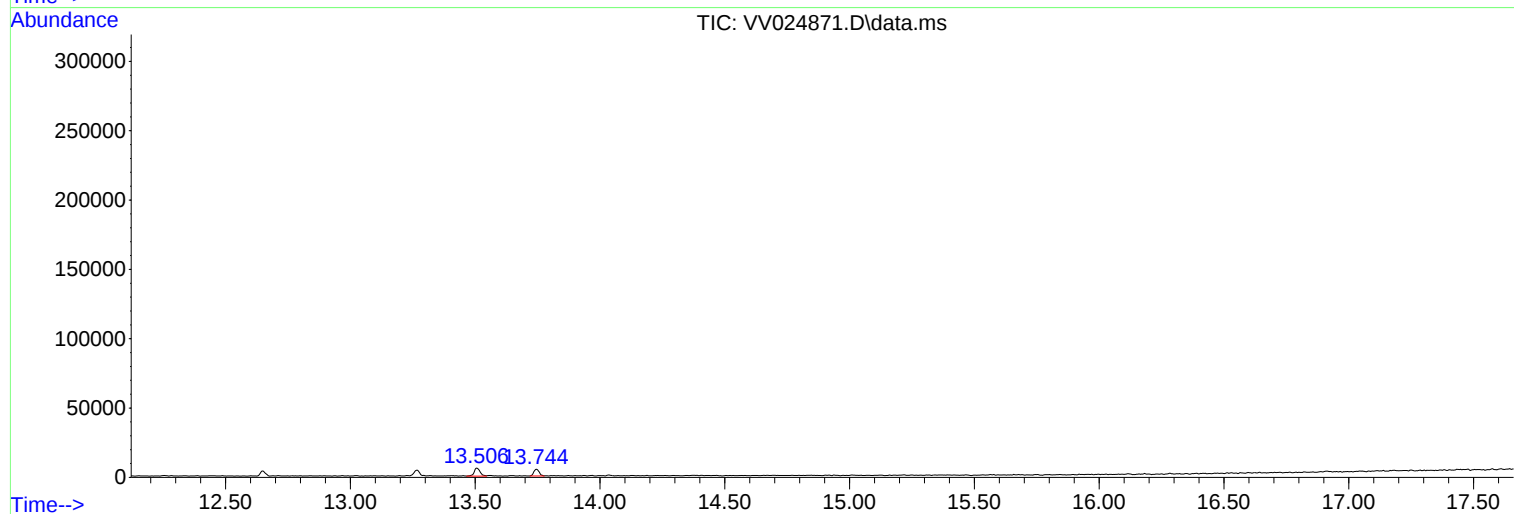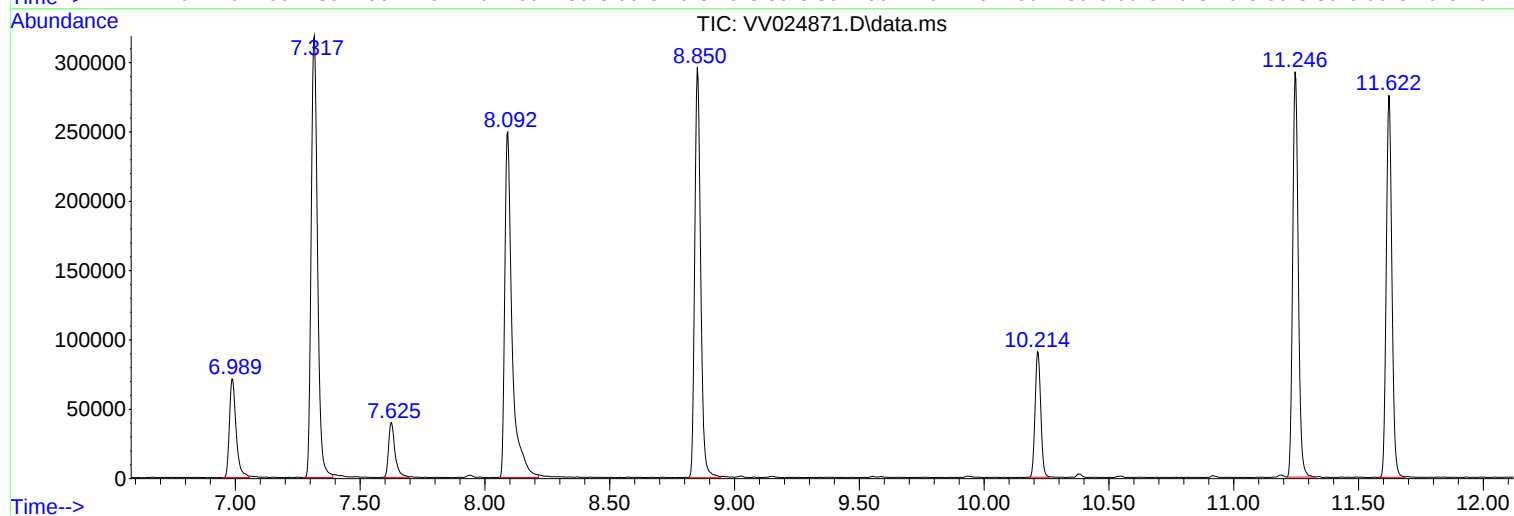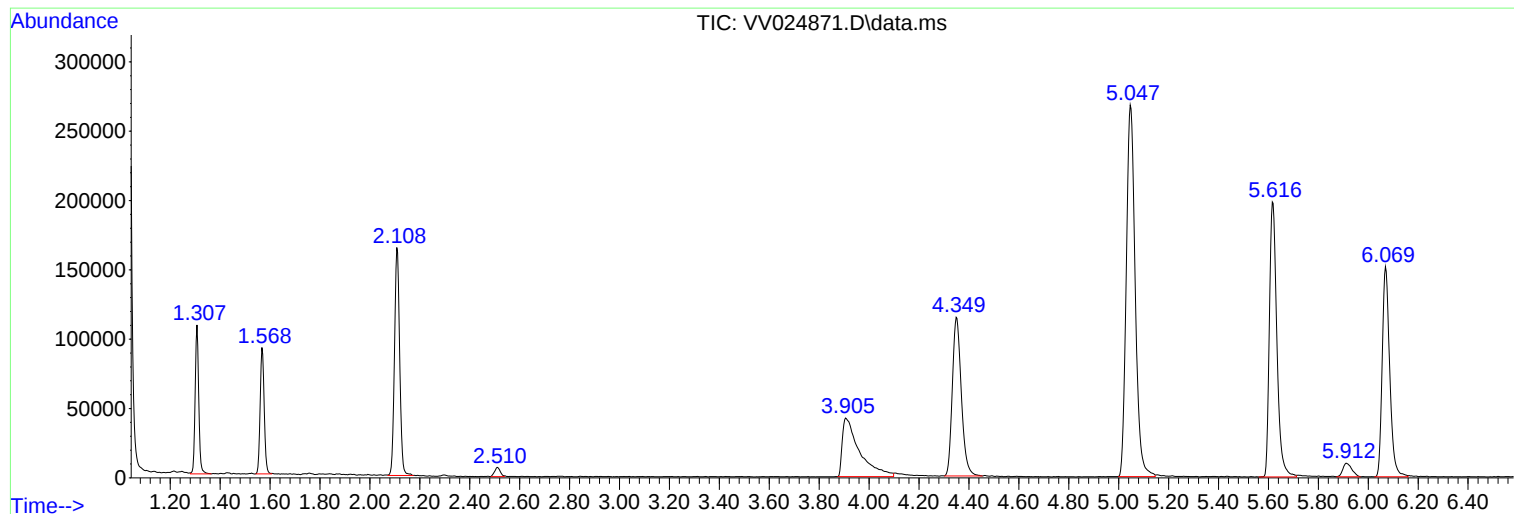

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024871.D
Acq On : 08 Mar 2022 14:40
Operator : SY/MD
Sample : VIBLK261
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
Data File : VV024871.D
Acq On : 08 Mar 2022 14:40
Operator : SY/MD
Sample : VIBLK261
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc