
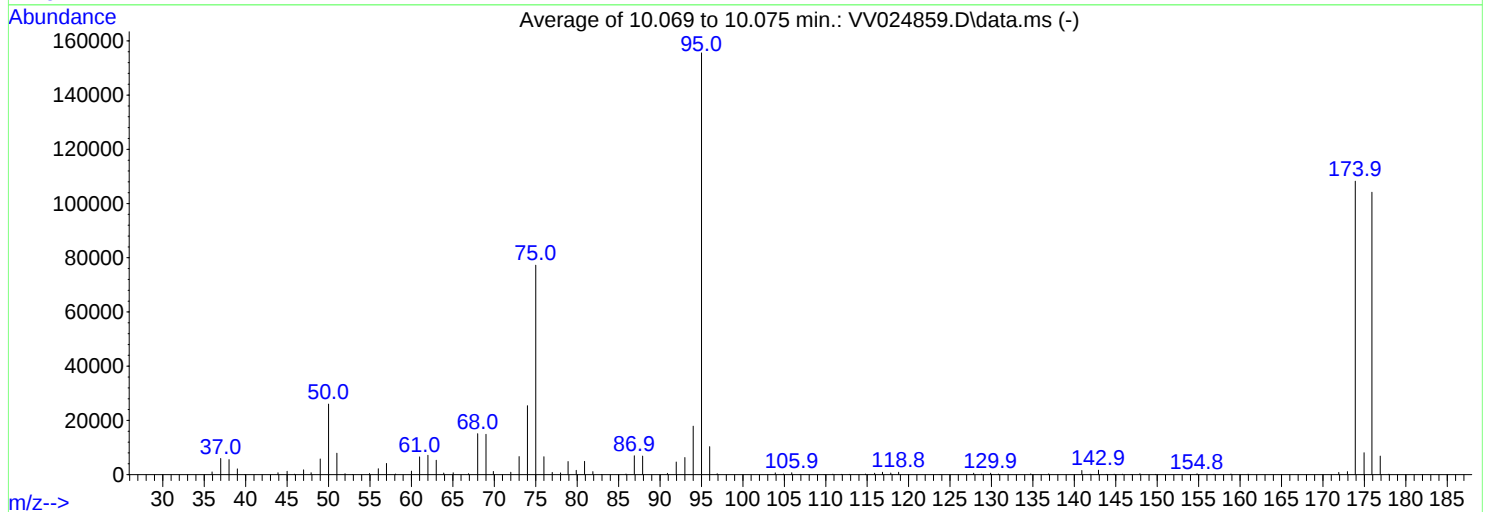


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
 Data File : VV024859.D
 Acq On : 08 Mar 2022 08:51
 Operator : SY/MD
 Sample : BFB277
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB277

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Mar 10 04:55:47 2022

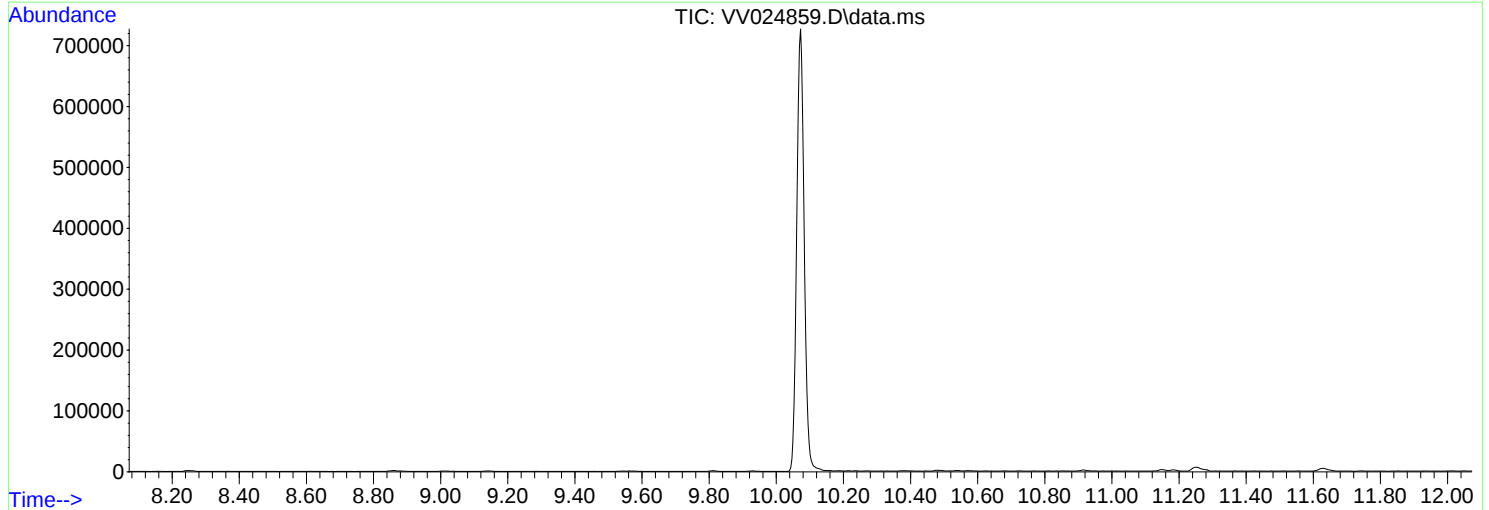

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	26016	PASS
75	95	30	80	49.7	77269	PASS
95	95	100	100	100.0	155584	PASS
96	95	5	9	6.6	10345	PASS
173	174	0.00	2	1.0	1128	PASS
174	95	50	120	69.6	108224	PASS
175	174	5	9	7.5	8093	PASS
176	174	95	105	96.3	104171	PASS
177	176	5	10	6.6	6847	PASS

m/z	Abundance
39.90	479.0
43.90	285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
35.90	939.0
37.00	5942.0
38.00	5621.0
39.00	2100.0
40.00	565.0
43.90	1062.0
45.00	1310.0
45.90	157.0
47.00	1783.0
47.90	800.0
49.00	5874.0
50.00	26280.0
51.00	7831.0
52.00	341.0
52.90	156.0
55.00	386.0
56.00	2230.0
57.00	4034.0
58.10	191.0
60.00	1308.0
61.00	6860.0
62.00	7408.0
63.00	5319.0
63.90	639.0
65.00	747.0
66.90	355.0
68.00	15360.0
69.00	14935.0
69.90	1239.0
72.00	963.0
73.00	6719.0
74.00	25528.0
75.00	77480.0
76.00	6752.0
77.00	850.0
78.00	654.0
78.90	4860.0
79.90	1580.0
80.90	4764.0
81.90	1128.0
82.90	140.0
85.90	249.0
86.90	7061.0
87.90	6829.0
90.90	474.0
91.90	4632.0
93.00	6175.0
94.00	18064.0
95.00	154880.0
96.00	10697.0
96.90	384.0
103.90	608.0
104.90	247.0
105.90	707.0
106.90	125.0
109.80	114.0
110.80	199.0
111.90	139.0
112.90	157.0
114.80	220.0
115.90	526.0
116.80	859.0
117.80	585.0
118.80	927.0
123.80	104.0
127.80	476.0
128.80	168.0
129.90	463.0
130.90	220.0
134.80	242.0
136.90	246.0
140.90	1598.0
141.90	123.0
142.90	1567.0
143.90	116.0
144.80	176.0
145.80	173.0
147.90	350.0
149.80	158.0
154.80	406.0
156.80	208.0
158.90	221.0
161.00	158.0
171.90	893.0
172.90	1144.0
173.90	104440.0
175.00	8172.0
175.90	101448.0
176.90	6708.0
178.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
36.00	1022.0
37.00	6244.0
38.00	5746.0
39.00	2153.0
40.00	575.0
44.00	1006.0
45.00	1302.0
45.90	182.0
47.00	1817.0
47.90	725.0
49.00	5973.0
50.00	26992.0
51.00	8139.0
52.00	370.0
52.90	113.0
55.00	412.0
56.00	2261.0
57.00	4269.0
58.10	225.0
60.00	1348.0
61.00	6639.0
62.00	7383.0
63.00	5493.0
63.90	634.0
65.10	716.0
66.90	338.0
68.00	15752.0
69.00	15303.0
69.90	1220.0
72.00	962.0
73.00	6915.0
74.00	26232.0
75.00	79856.0
76.00	6889.0
77.00	881.0
78.00	674.0
78.90	5018.0
79.90	1634.0
80.90	5036.0
81.90	1200.0
83.00	125.0
85.90	250.0
86.90	7215.0
87.90	7207.0
90.90	506.0
91.90	4857.0
93.00	6504.0
94.00	18376.0
95.00	160960.0
96.00	10678.0
96.90	371.0
103.90	658.0
104.90	244.0
105.90	774.0
106.90	143.0
109.80	113.0
110.80	194.0
111.90	148.0
112.80	160.0
114.80	228.0
115.90	541.0
116.80	873.0
117.90	589.0
118.80	923.0
127.80	543.0
128.80	213.0
129.90	551.0
130.90	246.0
134.70	285.0
136.90	311.0
140.90	1588.0
141.90	171.0
142.90	1743.0
143.80	111.0
144.80	180.0
145.80	201.0
146.80	114.0
147.90	356.0
149.80	150.0
154.80	380.0
156.80	208.0
158.90	248.0
161.00	160.0
171.90	872.0
173.00	1167.0
173.90	111728.0
175.00	8328.0
175.90	107936.0
176.90	7100.0
177.90	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277

m/z	Abundance
36.00	1064.0
37.00	5717.0
38.00	5313.0
39.00	2074.0
39.90	562.0
44.00	888.0
45.00	1067.0
45.90	145.0
47.00	1690.0
47.90	597.0
49.00	5443.0
50.00	24776.0
51.00	7745.0
52.00	340.0
54.90	421.0
56.00	2121.0
57.00	4089.0
58.10	240.0
60.00	1309.0
61.00	6179.0
62.00	6632.0
63.00	5085.0
63.90	533.0
65.10	607.0
66.90	317.0
68.00	14233.0
69.00	14449.0
69.90	1076.0
72.00	796.0
73.00	6354.0
74.00	24584.0
75.00	74472.0
76.00	6160.0
77.00	827.0
78.00	641.0
78.90	4619.0
79.90	1530.0
80.90	4844.0
81.90	1147.0
85.90	202.0
86.90	6658.0
87.90	6594.0
90.90	502.0
92.00	4483.0
93.00	6370.0
94.00	17224.0
95.00	150912.0
96.00	9661.0
96.90	288.0
103.90	633.0
104.90	224.0
105.90	720.0
106.90	160.0
110.90	152.0
111.90	139.0
112.80	137.0
114.80	218.0
115.90	503.0
116.90	879.0
117.90	583.0
118.80	841.0
127.90	554.0
128.80	234.0
129.90	569.0
130.80	257.0
134.70	301.0
136.90	338.0
140.90	1435.0
141.90	200.0
142.90	1678.0
143.80	104.0
144.80	187.0
145.80	231.0
146.90	109.0
147.90	339.0
149.80	145.0
154.80	330.0
156.90	183.0
158.90	200.0
160.90	154.0
171.90	765.0
173.00	1072.0
173.90	108504.0
174.90	7778.0
175.90	103128.0
176.90	6732.0
177.90	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB277