


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV030822\
 Data File : VV024878.D
 Acq On : 09 Mar 2022 09:37
 Operator : SY/MD
 Sample : BFB278
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB278

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR021722WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Mar 10 04:55:47 2022

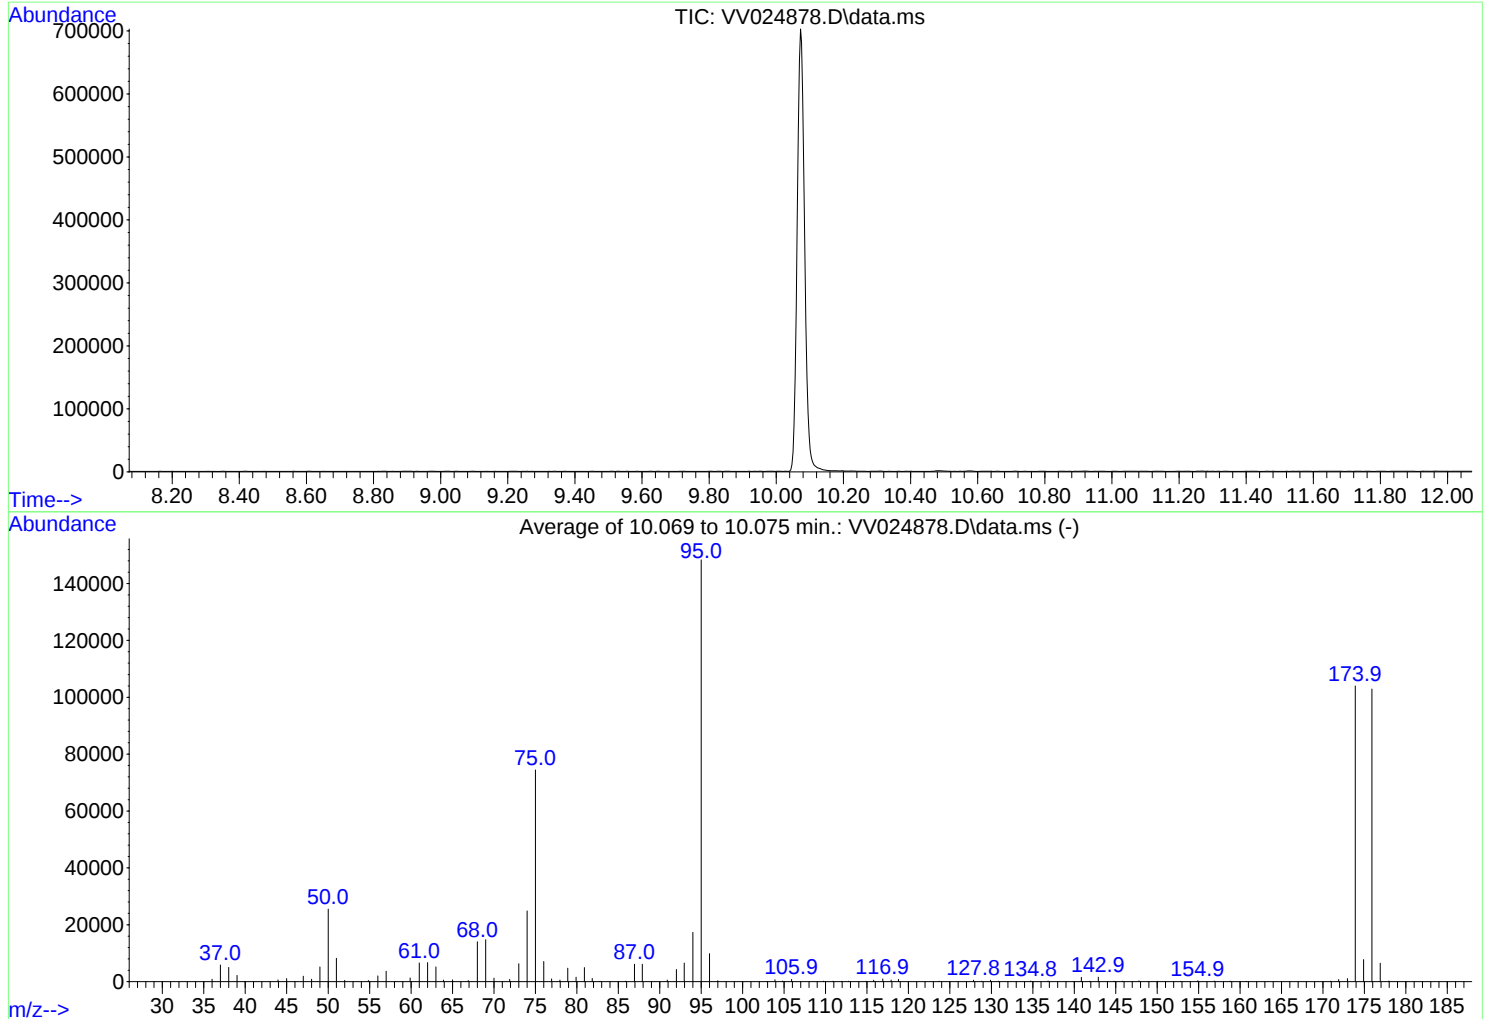

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	25517	PASS
75	95	30	80	50.2	74469	PASS
95	95	100	100	100.0	148331	PASS
96	95	5	9	6.6	9856	PASS
173	174	0.00	2	1.0	1082	PASS
174	95	50	120	70.1	104011	PASS
175	174	5	9	7.5	7773	PASS
176	174	95	105	99.0	102936	PASS
177	176	5	10	6.3	6457	PASS

Scan 2796 (10.030 min): VV024878.D\data.ms
BFB278

m/z	Abundance
39.90	644.0
43.80	300.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	882.0
37.00	5635.0
38.00	5037.0
39.00	2106.0
39.90	621.0
44.00	971.0
45.00	983.0
45.90	141.0
47.00	2012.0
48.00	764.0
49.00	5104.0
50.00	24856.0
51.00	8013.0
52.00	435.0
54.80	426.0
56.00	1939.0
57.00	3660.0
58.00	102.0
59.90	1263.0
61.00	6576.0
62.00	6458.0
63.00	5051.0
63.90	572.0
65.00	657.0
66.90	386.0
68.00	13892.0
69.00	14308.0
70.00	1199.0
71.90	764.0
73.00	6073.0
74.00	24056.0
75.00	72448.0
76.00	6792.0
76.90	1019.0
77.90	559.0
78.90	4546.0
79.90	1648.0
80.90	4700.0
81.80	1103.0
82.80	120.0
85.90	189.0
87.00	6118.0
87.90	6141.0
90.90	550.0
92.00	4126.0
93.00	6358.0
94.00	16688.0
95.00	143232.0
96.00	9454.0
97.00	347.0
103.90	587.0
104.80	210.0
105.90	770.0
109.70	133.0
110.90	164.0
112.80	163.0
114.90	169.0
115.80	518.0
116.90	897.0
117.90	627.0
118.80	779.0
123.70	149.0
127.80	496.0
128.90	170.0
129.90	502.0
130.90	163.0
134.70	209.0
136.90	177.0
140.90	1451.0
141.90	148.0
142.90	1525.0
144.80	178.0
145.80	154.0
147.80	281.0
150.00	174.0
154.90	288.0
156.90	226.0
158.80	139.0
160.70	135.0
171.00	144.0
171.90	715.0
172.90	1070.0
173.90	98296.0
174.90	7552.0
175.90	95888.0
176.90	6149.0
178.00	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	877.0
37.00	6081.0
38.00	5231.0
39.00	2277.0
39.90	670.0
44.00	982.0
45.00	1080.0
46.00	120.0
47.00	2027.0
48.00	839.0
49.00	5350.0
50.00	26344.0
51.00	8470.0
52.00	452.0
54.90	431.0
56.00	2108.0
57.00	3763.0
59.90	1381.0
61.00	6824.0
62.00	6882.0
63.00	5381.0
63.90	604.0
65.00	669.0
66.90	392.0
68.00	14546.0
69.00	15274.0
70.00	1304.0
71.90	846.0
73.00	6491.0
74.00	25824.0
75.00	77168.0
76.00	7330.0
77.00	993.0
77.90	595.0
78.90	4897.0
79.90	1606.0
80.90	5149.0
81.90	1128.0
82.80	145.0
85.80	175.0
87.00	6257.0
87.90	6343.0
90.90	579.0
92.00	4430.0
93.00	6770.0
94.00	17824.0
95.00	153536.0
96.00	10211.0
97.00	339.0
102.90	105.0
103.90	685.0
104.80	236.0
105.90	833.0
109.70	155.0
110.90	203.0
111.90	117.0
112.80	152.0
114.90	184.0
115.80	507.0
116.90	969.0
117.90	573.0
118.80	812.0
123.70	177.0
127.80	528.0
128.90	198.0
129.90	532.0
130.80	186.0
134.70	219.0
136.90	221.0
140.80	1557.0
141.90	142.0
142.90	1632.0
144.80	185.0
145.80	164.0
147.80	309.0
148.90	103.0
150.00	182.0
152.80	134.0
154.90	356.0
156.90	252.0
158.80	172.0
160.70	124.0
170.90	156.0
171.90	796.0
172.90	1099.0
173.90	107552.0
174.90	8031.0
175.90	106640.0
176.90	6729.0
178.00	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278

m/z	Abundance
36.00	837.0
37.00	5861.0
38.00	4842.0
39.00	2188.0
39.90	715.0
44.00	910.0
45.00	1126.0
46.00	118.0
47.00	1785.0
48.00	870.0
49.00	5157.0
50.00	25352.0
51.00	8120.0
52.00	400.0
54.90	357.0
56.00	2003.0
57.00	3552.0
58.10	116.0
59.90	1297.0
61.00	6443.0
62.00	6719.0
63.00	5088.0
63.90	545.0
65.00	608.0
66.90	350.0
68.00	13686.0
69.00	14736.0
70.00	1260.0
71.90	773.0
73.00	6323.0
74.00	24776.0
75.00	73792.0
76.00	7086.0
77.00	941.0
78.00	609.0
78.90	4737.0
79.90	1403.0
80.90	5017.0
81.90	1083.0
82.80	143.0
85.80	177.0
86.90	6081.0
87.90	5910.0
90.90	537.0
92.00	4284.0
92.90	6455.0
94.00	17448.0
95.00	148224.0
96.00	9903.0
97.00	340.0
103.90	704.0
104.80	246.0
105.90	772.0
109.80	145.0
110.90	210.0
111.90	150.0
112.80	127.0
114.90	173.0
115.80	462.0
116.90	957.0
117.90	491.0
118.80	820.0
123.70	136.0
127.90	533.0
128.80	214.0
129.90	469.0
130.80	195.0
134.80	198.0
136.80	243.0
139.90	110.0
140.80	1497.0
141.90	151.0
142.90	1614.0
144.80	182.0
145.80	174.0
147.80	304.0
148.90	106.0
150.00	152.0
152.80	149.0
154.90	400.0
156.90	231.0
158.80	181.0
160.80	128.0
170.80	131.0
171.90	774.0
173.00	1076.0
173.90	106184.0
174.90	7737.0
175.90	106280.0
176.90	6494.0
177.90	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB278