

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031022\
 Data File : VW024940.D
 Acq On : 11 Mar 2022 01:40
 Operator : SY/MD
 Sample : N1879-09
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CODA0

Quant Time: Mar 11 05:28:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 05:21:24 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	282567	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	274486	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	121924	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	113424	39.477	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	78.960%	
7) Chloroethane-d5	1.568	69	90413	40.109	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	80.220%	
11) 1,1-Dichloroethene-d2	2.108	63	148602	30.815	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	61.620%	
21) 2-Butanone-d5	3.895	46	147169	90.005	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	90.000%	
24) Chloroform-d	4.349	84	203469	40.568	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	81.140%	
26) 1,2-Dichloroethane-d4	5.030	65	124144	41.951	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.900%	
32) Benzene-d6	5.050	84	429937	42.259	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	84.520%	
36) 1,2-Dichloropropane-d6	6.069	67	135469	42.737	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	85.480%	
41) Toluene-d8	7.313	98	372769	41.358	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.720%	
43) trans-1,3-Dichloroprop...	7.622	79	55081	39.991	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.980%	
47) 2-Hexanone-d5	8.088	63	96372	80.098	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	80.100%	
56) 1,1,2,2-Tetrachloroeth...	10.213	84	165941	44.137	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.280%	
66) 1,2-Dichlorobenzene-d4	11.622	152	124526	44.338	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.680%	
Target Compounds						
37) 1,2-Dichloropropane	6.069	63	13627	5.862	ug/L #	86
39) cis-1,3-Dichloropropene	6.982	75	3466	0.991	ug/L #	75
61) 1,2,3-Trichloropropane	11.246	75	15346	6.290	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024940.D
Acq On : 11 Mar 2022 01:40
Operator : SY/MD
Sample : N1879-09
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA0

Quant Time: Mar 11 05:28:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 05:21:24 2022
Response via : Initial Calibration

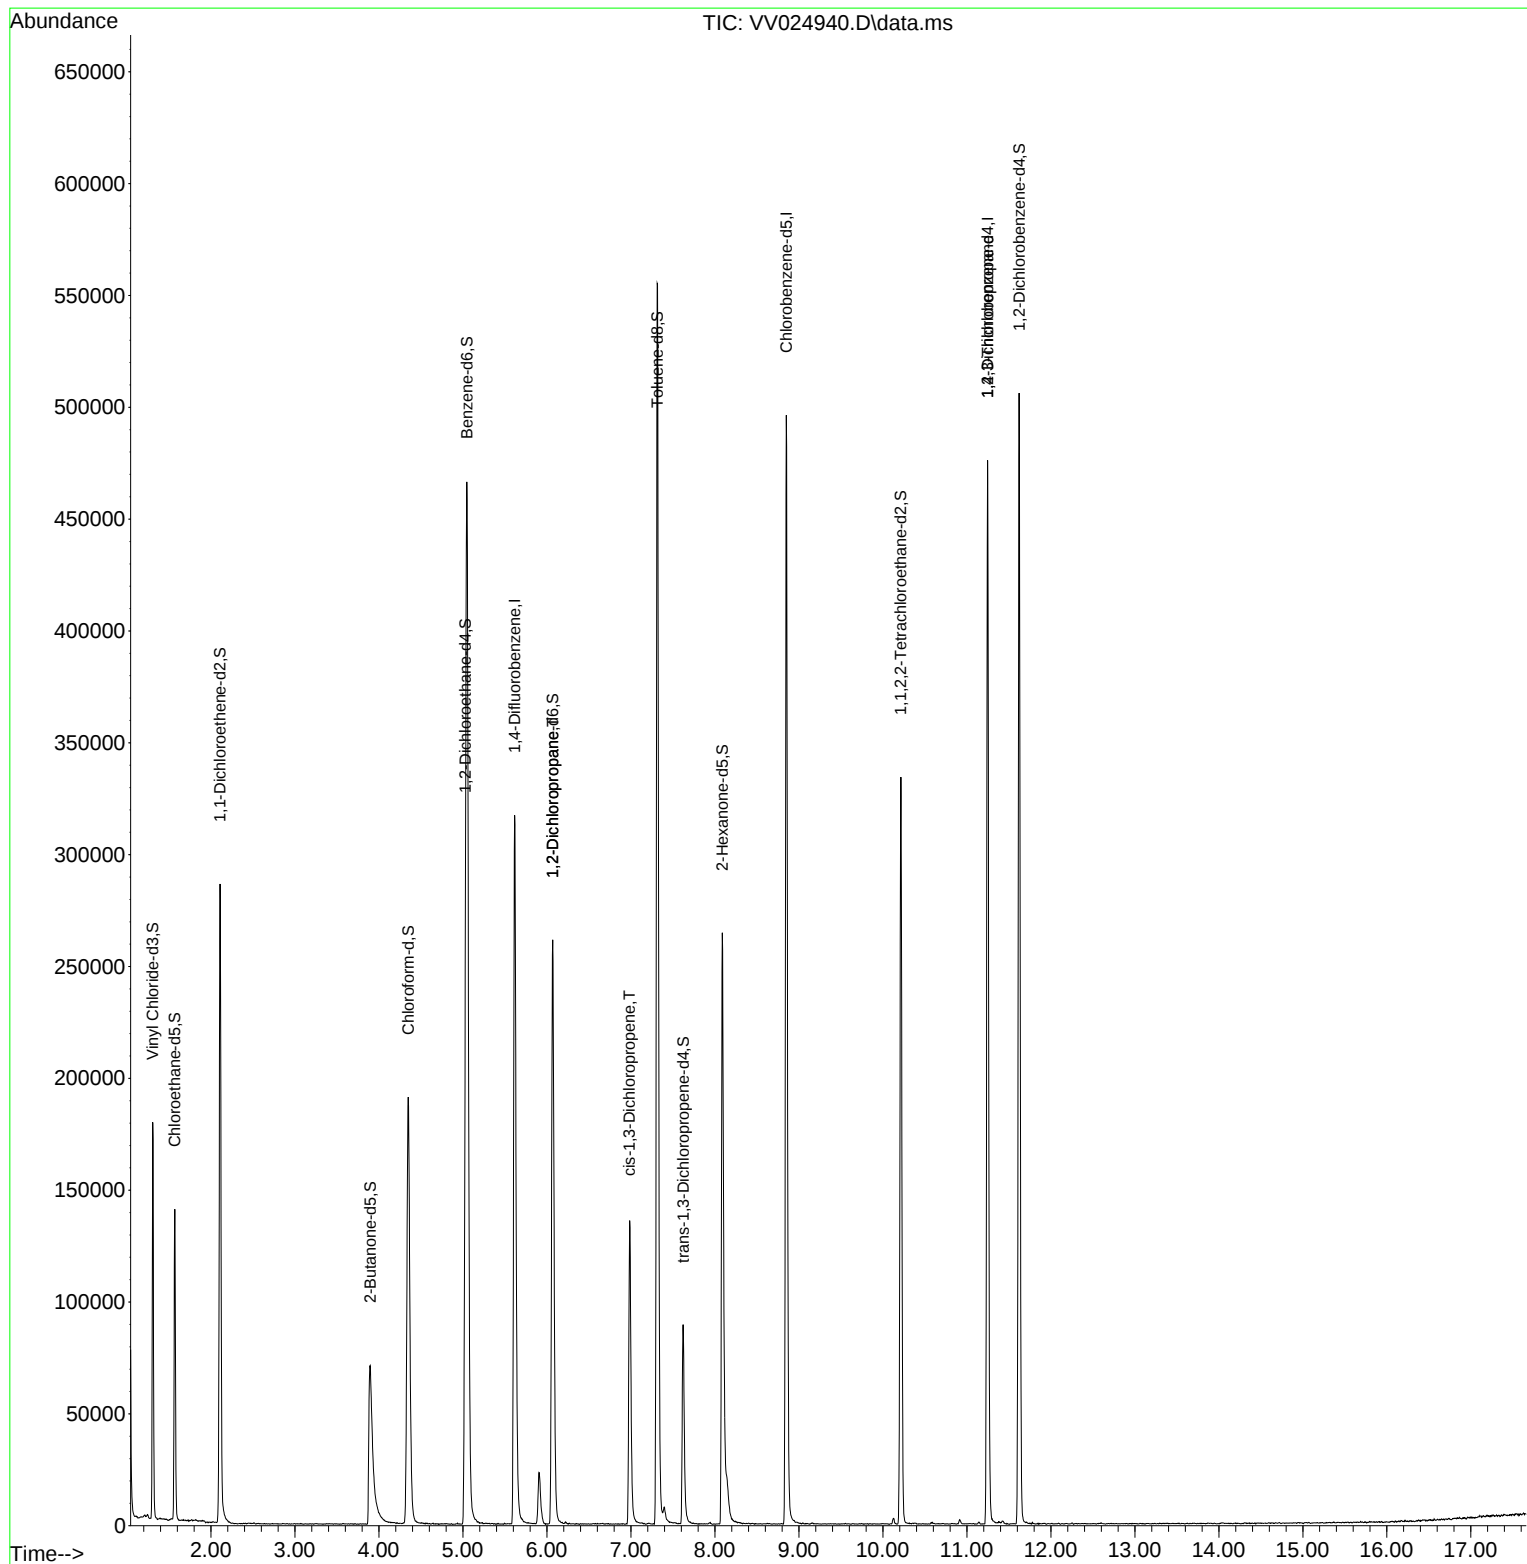

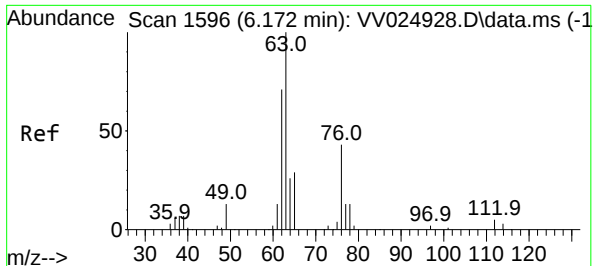

#37

1,2-Dichloropropane

Concen: 5.862 ug/L

RT: 6.069 min Scan# 11

Delta R.T. -0.103 min

Lab File: VV024940.D

Acq: 11 Mar 2022 01:40

Instrument :

MSVOA_V

ClientSampleId :





C0DA0

Tgt Ion: 63 Resp: 13627

Ion Ratio Lower Upper

63 100

112 0.0 3.6 5.4#

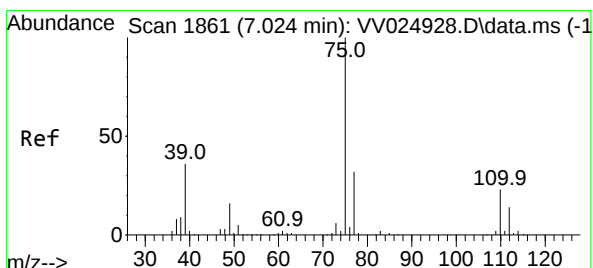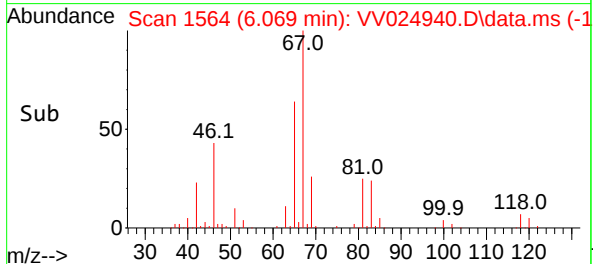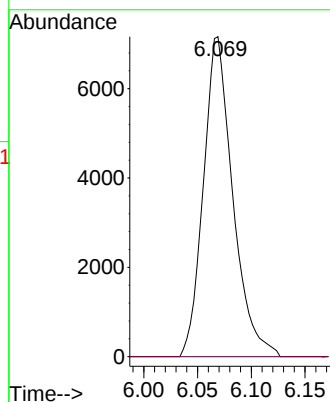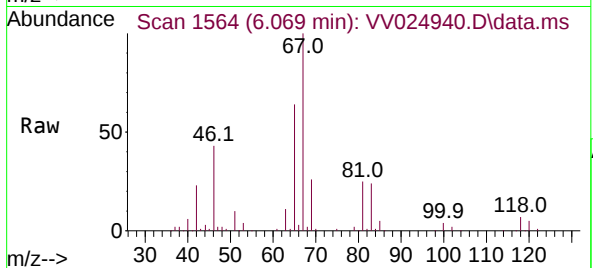

#39

cis-1,3-Dichloropropene

Concen: 0.991 ug/L

RT: 6.982 min Scan# 1848

Delta R.T. -0.042 min

Lab File: VV024940.D




Acq: 11 Mar 2022 01:40


Tgt Ion: 75 Resp: 3466

Ion Ratio Lower Upper

75 100


77 47.0 22.9 42.5#

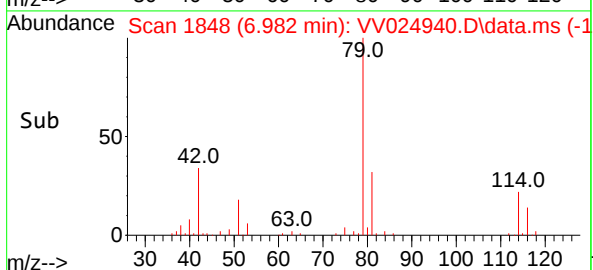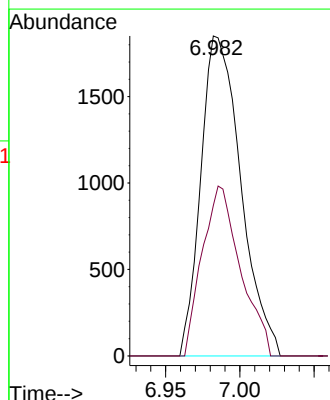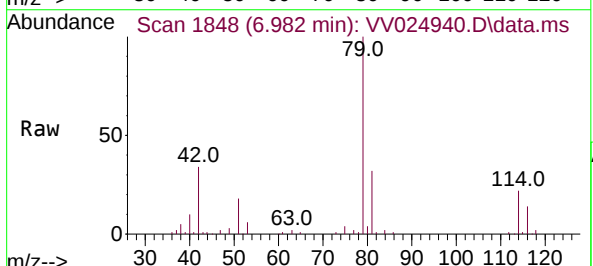

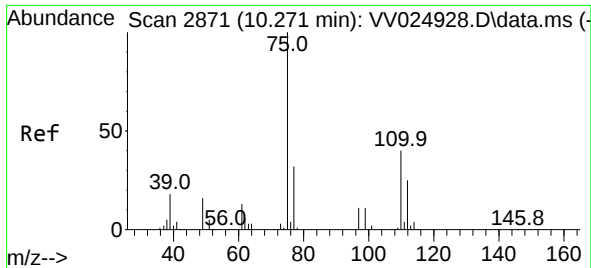

#61
 1,2,3-Trichloropropane
 Concen: 6.290 ug/L
 RT: 11.246 min Scan# 31
 Delta R.T. 0.974 min
 Lab File: VV024940.D
 Acq: 11 Mar 2022 01:40

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA0

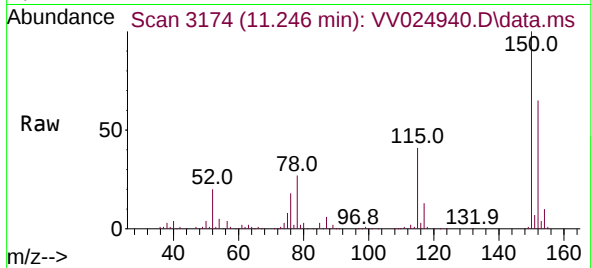

Tgt Ion: 75	Resp:	15346
Ion	Ratio	Lower Upper
75	100	
77	32.0	25.4 38.0
110	2.0	31.4 47.2#

