

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031022\
 Data File : VW024907.D
 Acq On : 10 Mar 2022 11:48
 Operator : SY/MD
 Sample : N1855-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D32

Quant Time: Mar 11 02:46:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 02:45:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	298509	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	290815	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	130092	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	99967	32.935	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	65.880%		
7) Chloroethane-d5	1.568	69	90952	38.193	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	76.380%		
11) 1,1-Dichloroethene-d2	2.108	63	143220	28.113	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	56.220%#		
21) 2-Butanone-d5	3.896	46	166413	96.339	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.340%		
24) Chloroform-d	4.349	84	214928	40.564	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	81.120%		
26) 1,2-Dichloroethane-d4	5.031	65	132534	42.394	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.780%		
32) Benzene-d6	5.050	84	444321	41.220	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.440%		
36) 1,2-Dichloropropane-d6	6.069	67	143428	42.708	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.420%		
41) Toluene-d8	7.317	98	381162	39.914	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	79.820%#		
43) trans-1,3-Dichloroprop...	7.622	79	54430	37.299	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.600%		
47) 2-Hexanone-d5	8.088	63	119036	93.380	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.380%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	180033	45.196	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	134434	44.861	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.720%		
Target Compounds					Qvalue	
13) Acetone	2.192	43	12784	9.692	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024907.D
Acq On : 10 Mar 2022 11:48
Operator : SY/MD
Sample : N1855-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COD32

Quant Time: Mar 11 02:46:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 02:45:24 2022
Response via : Initial Calibration

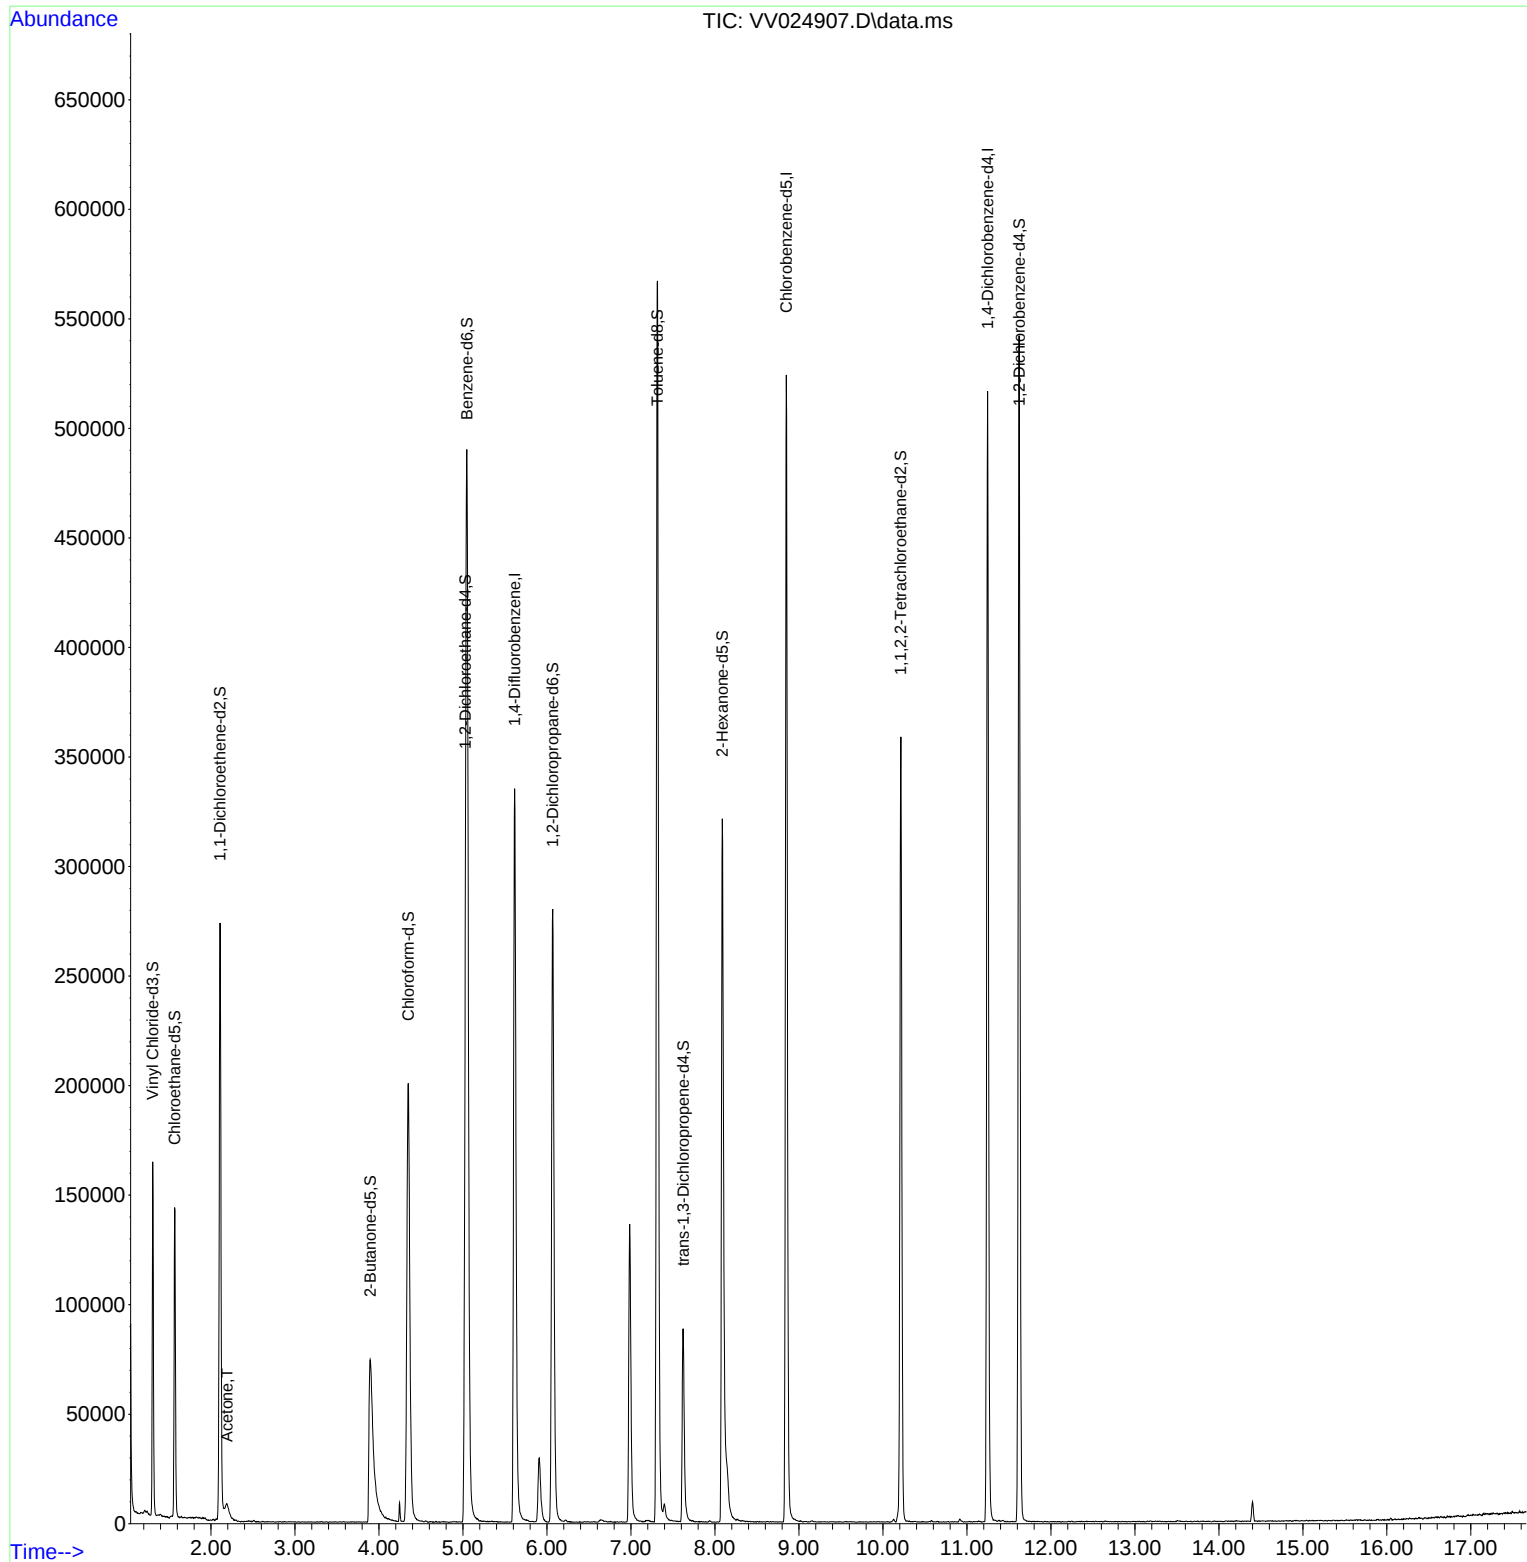

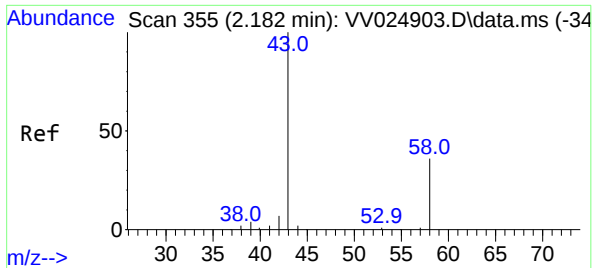

#13
 Acetone
 Concen: 9.692 ug/L
 RT: 2.192 min Scan# 31
 Delta R.T. 0.010 min
 Lab File: VV024907.D
 Acq: 10 Mar 2022 11:48

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D32

Tgt Ion: 43 Resp: 12784
 Ion Ratio Lower Upper
 43 100
 58 31.0 0.0 70.0

