

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031022\
 Data File : VW024921.D
 Acq On : 10 Mar 2022 17:19
 Operator : SY/MD
 Sample : N1856-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D50

Quant Time: Mar 11 02:49:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 02:45:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	288075	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	280811	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	124229	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	127741	43.610	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.220%		
7) Chloroethane-d5	1.568	69	97270	42.326	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	84.660%		
11) 1,1-Dichloroethene-d2	2.108	63	162554	33.064	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.120%		
21) 2-Butanone-d5	3.892	46	132083	79.234	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.230%		
24) Chloroform-d	4.349	84	209988	41.067	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.140%		
26) 1,2-Dichloroethane-d4	5.030	65	128321	42.533	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.060%		
32) Benzene-d6	5.050	84	446921	42.938	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.880%		
36) 1,2-Dichloropropane-d6	6.069	67	139463	43.006	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.020%		
41) Toluene-d8	7.313	98	389466	42.237	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.480%		
43) trans-1,3-Dichloroprop...	7.619	79	57370	40.715	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	81.420%		
47) 2-Hexanone-d5	8.088	63	91140	74.043	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	74.040%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	163146	42.416	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.840%		
66) 1,2-Dichlorobenzene-d4	11.622	152	128906	45.046	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.100%		
Target Compounds					Qvalue	
13) Acetone	2.188	43	4795	3.767	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024921.D
Acq On : 10 Mar 2022 17:19
Operator : SY/MD
Sample : N1856-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D50


Quant Time: Mar 11 02:49:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 02:45:24 2022
Response via : Initial Calibration

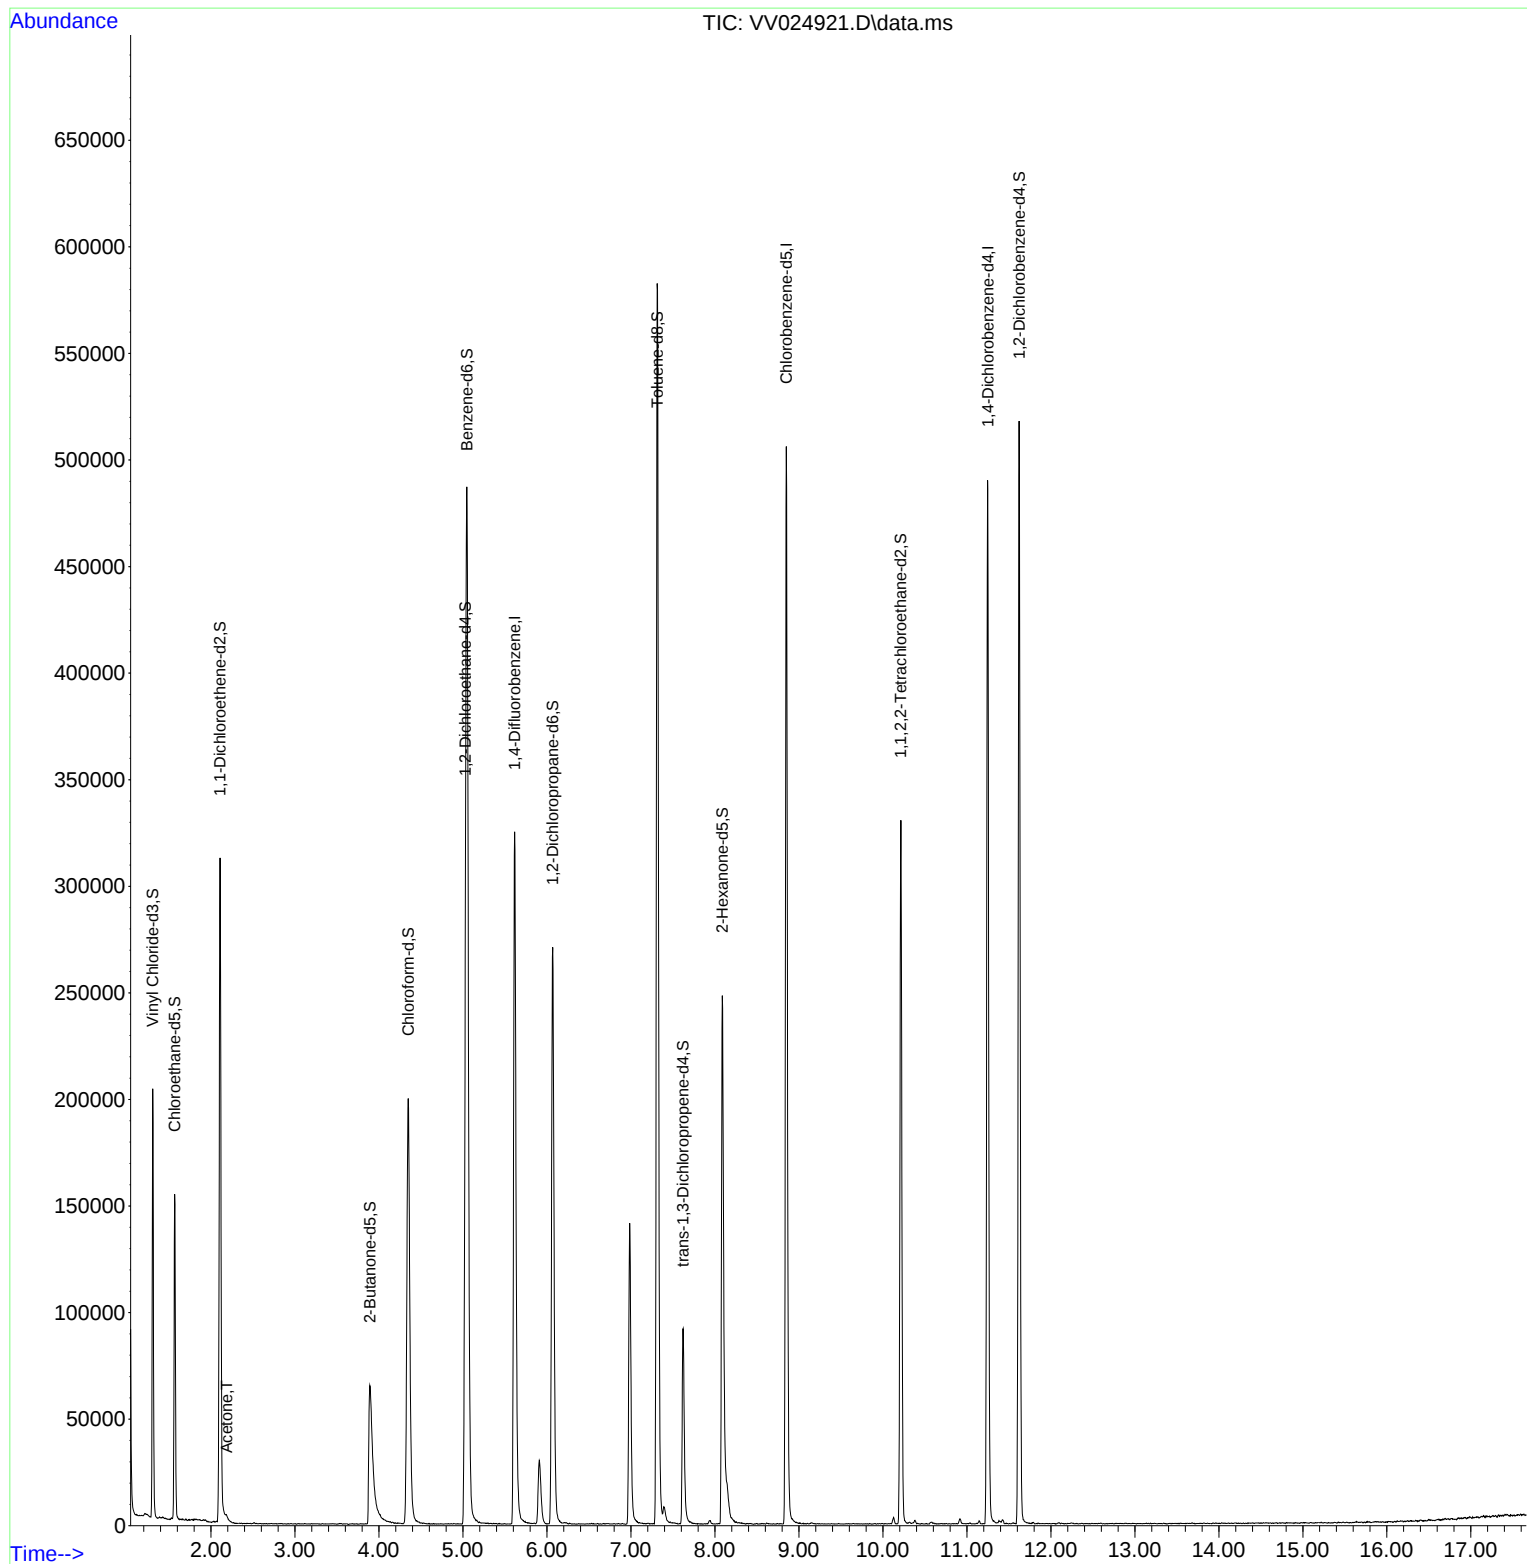

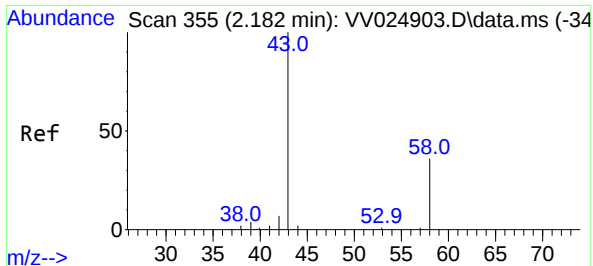

#13
 Acetone
 Concen: 3.767 ug/L
 RT: 2.188 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV024921.D
 Acq: 10 Mar 2022 17:19

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D50

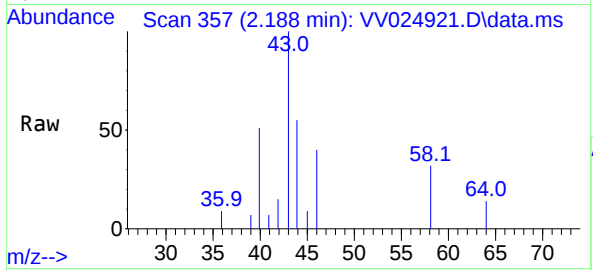

Tgt Ion: 43 Resp: 4795
 Ion Ratio Lower Upper
 43 100
 58 21.6 0.0 70.0

