

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024930.D
 Acq On : 10 Mar 2022 21:44
 Operator : SY/MD
 Sample : N1879-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA1

Quant Time: Mar 11 05:25:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 05:21:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	282452	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	276810	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	122234	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	120440	41.936	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	83.880%	
7) Chloroethane-d5	1.568	69	95079	42.196	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	84.400%	
11) 1,1-Dichloroethene-d2	2.108	63	154619	32.076	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	64.160%	
21) 2-Butanone-d5	3.892	46	139933	85.614	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	85.610%	
24) Chloroform-d	4.349	84	207202	41.329	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.660%	
26) 1,2-Dichloroethane-d4	5.031	65	126200	42.663	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	85.320%	
32) Benzene-d6	5.050	84	441184	43.000	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	86.000%	
36) 1,2-Dichloropropane-d6	6.069	67	139187	43.542	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	87.080%	
41) Toluene-d8	7.313	98	383692	42.212	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	84.420%	
43) trans-1,3-Dichloroprop...	7.619	79	57630	41.490	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.980%	
47) 2-Hexanone-d5	8.088	63	95136	78.407	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	78.410%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	167417	44.155	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.320%	
66) 1,2-Dichlorobenzene-d4	11.622	152	128232	45.542	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.080%	
Target Compounds						Qvalue
34) Trichloroethene	5.918	95	7554	2.950	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024930.D
Acq On : 10 Mar 2022 21:44
Operator : SY/MD
Sample : N1879-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA1


Quant Time: Mar 11 05:25:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 05:21:24 2022
Response via : Initial Calibration

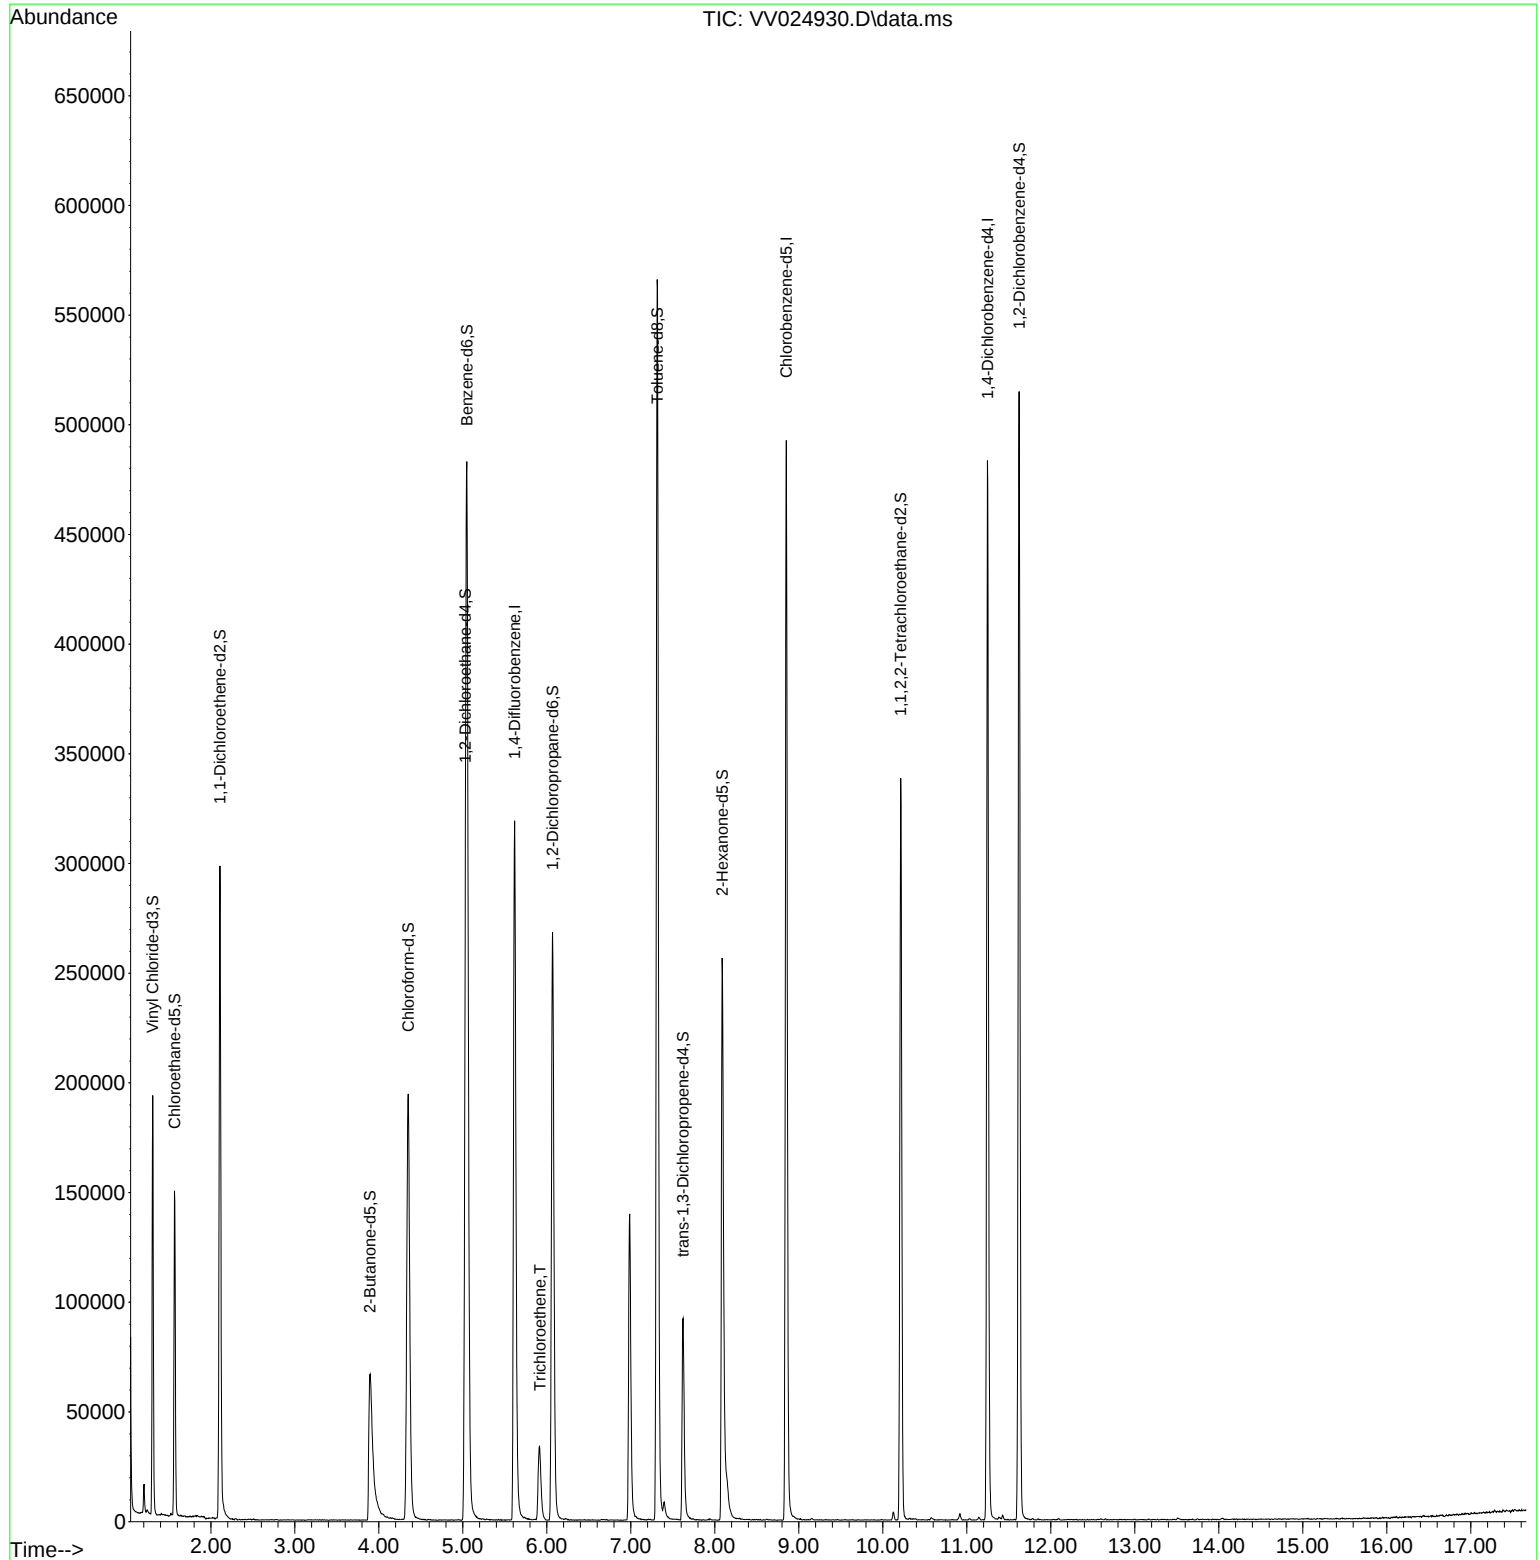

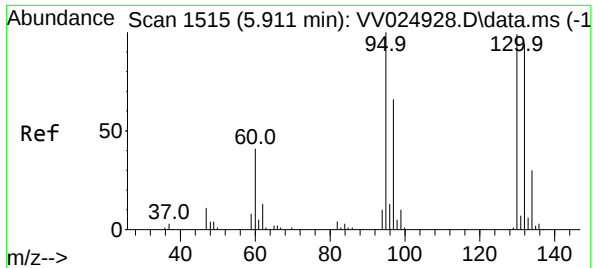

#34
 Trichloroethene
 Concen: 2.950 ug/L
 RT: 5.918 min Scan# 11
 Delta R.T. 0.007 min
 Lab File: VV024930.D
 Acq: 10 Mar 2022 21:44

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA1

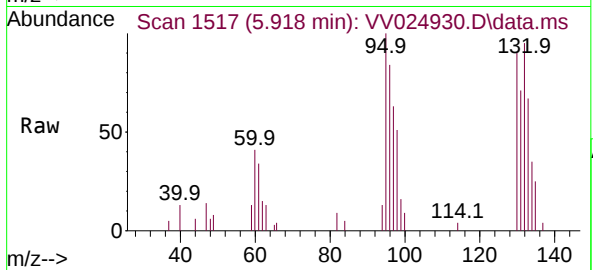

Tgt Ion:	95	Resp:	7554
Ion	Ratio	Lower	Upper
95	100		
97	63.2	45.3	84.1
132	95.0	65.0	120.6
130	90.4	69.3	128.7

