

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024931.D
 Acq On : 10 Mar 2022 22:07
 Operator : SY/MD
 Sample : N1856-21
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D81

Quant Time: Mar 11 05:26:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 05:21:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	287133	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	279797	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	126219	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	116914	40.044	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	80.080%	
7) Chloroethane-d5	1.568	69	90936	39.699	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.400%	
11) 1,1-Dichloroethene-d2	2.108	63	153131	31.249	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	62.500%	
21) 2-Butanone-d5	3.896	46	140959	84.836	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	84.840%	
24) Chloroform-d	4.349	84	210599	41.321	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.640%	
26) 1,2-Dichloroethane-d4	5.031	65	125361	41.688	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.380%	
32) Benzene-d6	5.050	84	438527	42.285	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	84.560%	
36) 1,2-Dichloropropane-d6	6.069	67	137898	42.678	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	85.360%	
41) Toluene-d8	7.313	98	383554	41.746	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	83.500%	
43) trans-1,3-Dichloroprop...	7.619	79	56571	40.293	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	80.580%	
47) 2-Hexanone-d5	8.088	63	97329	79.358	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	79.360%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	167223	43.633	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.260%	
66) 1,2-Dichlorobenzene-d4	11.622	152	129159	44.423	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.840%	
Target Compounds						
20) cis-1,2-Dichloroethene	3.918	96	2507	1.008	ug/L	Qvalue 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024931.D
Acq On : 10 Mar 2022 22:07
Operator : SY/MD
Sample : N1856-21
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D81

Quant Time: Mar 11 05:26:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 05:21:24 2022
Response via : Initial Calibration

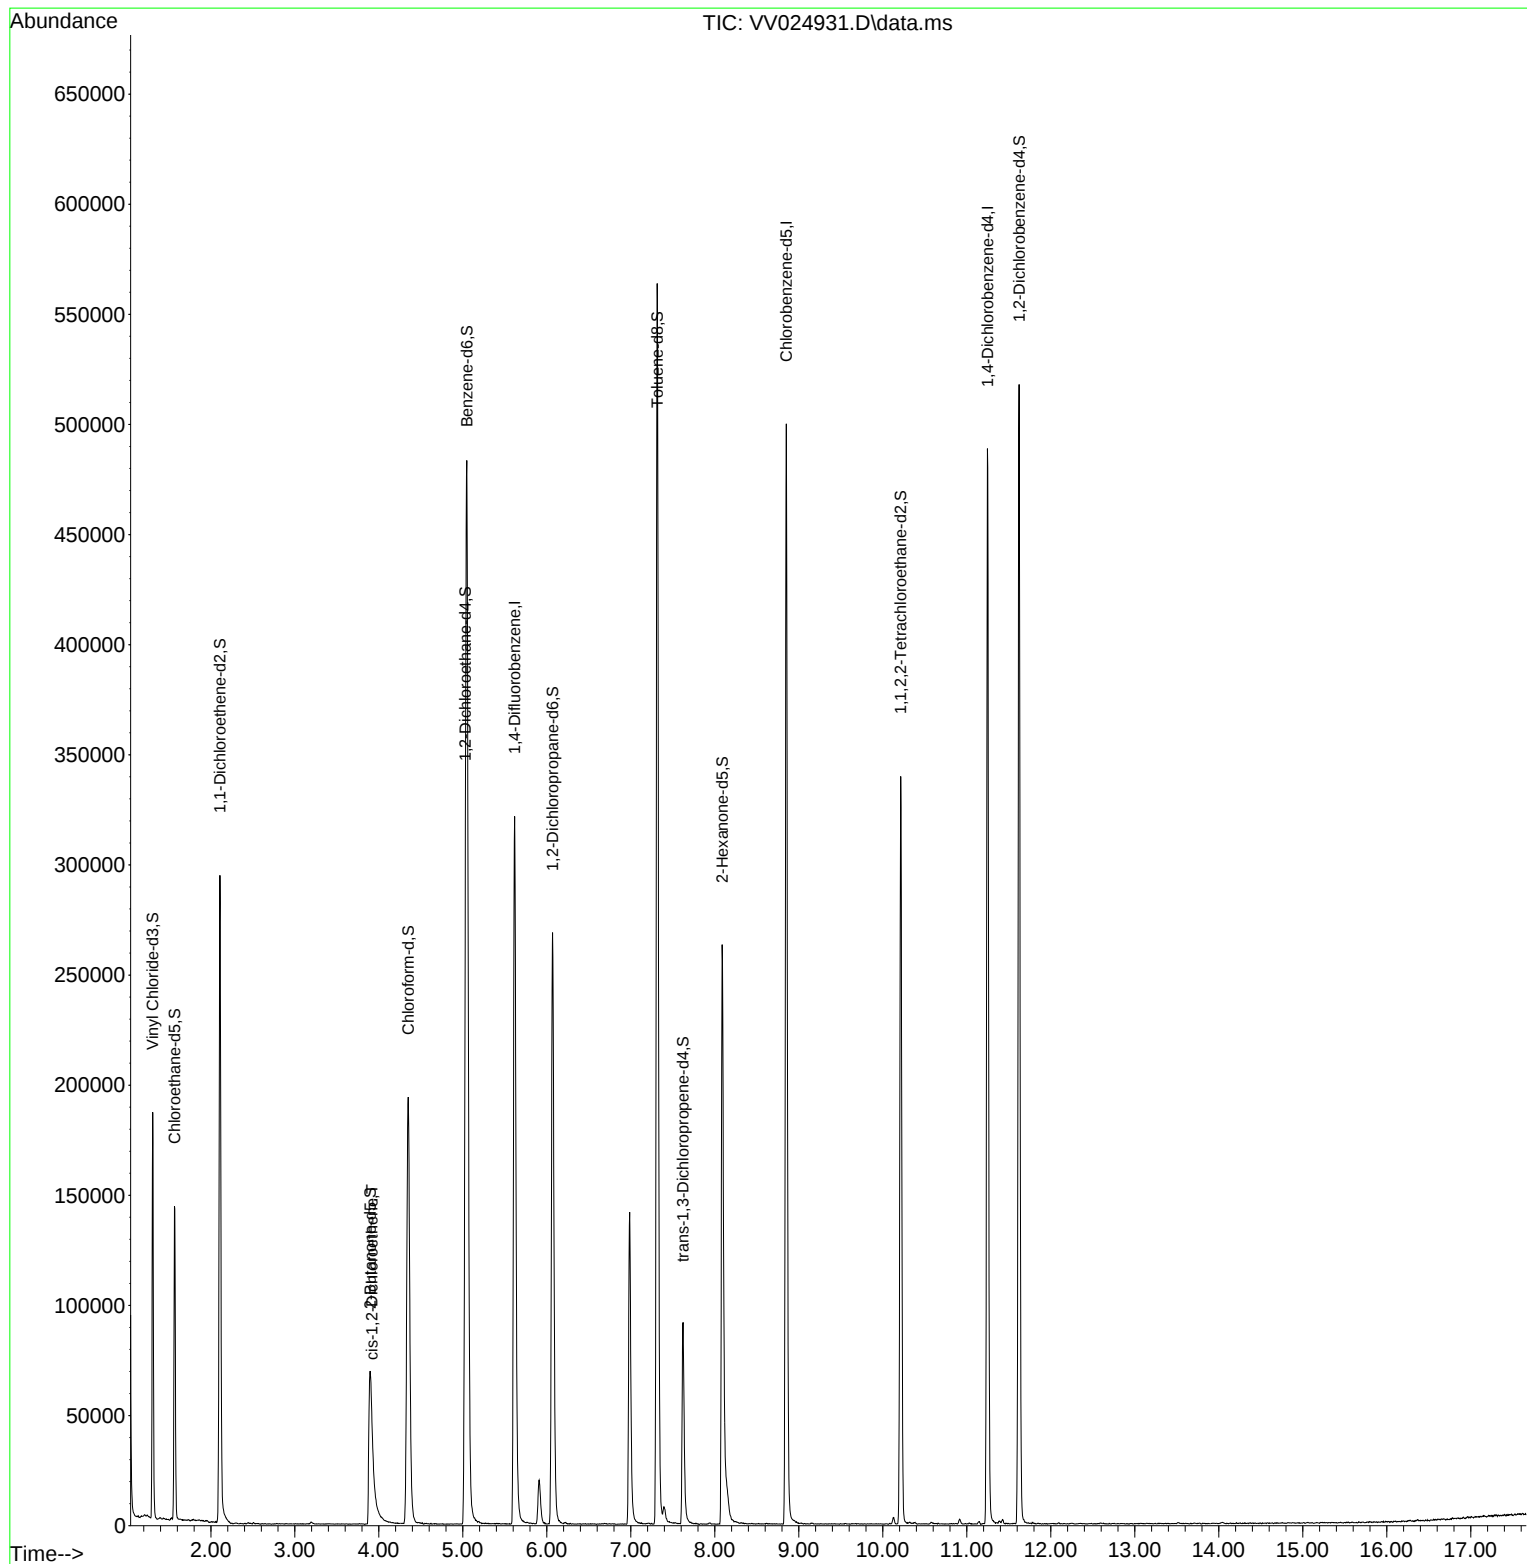

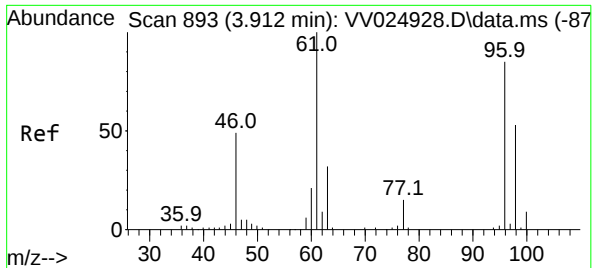

#20
 cis-1,2-Dichloroethene
 Concen: 1.008 ug/L
 RT: 3.918 min Scan# 89
 Delta R.T. 0.007 min
 Lab File: VV024931.D
 Acq: 10 Mar 2022 22:07

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D81

Tgt Ion: 96 Resp: 2507

Ion	Ratio	Lower	Upper
96	100		
61	106.7	86.1	159.9
68	0.0	0.0	0.0

