

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024934.D
 Acq On : 10 Mar 2022 23:18
 Operator : SY/MD
 Sample : N1879-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D86

Quant Time: Mar 11 05:26:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 05:21:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	270957	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	260522	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	115093	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	108537	39.395	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	78.780%	
7) Chloroethane-d5	1.568	69	85678	39.637	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.280%	
11) 1,1-Dichloroethene-d2	2.108	63	139212	30.105	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	60.200%	
21) 2-Butanone-d5	3.896	46	132326	84.395	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	84.390%	
24) Chloroform-d	4.349	84	193820	40.300	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	80.600%	
26) 1,2-Dichloroethane-d4	5.031	65	116515	41.060	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.120%	
32) Benzene-d6	5.050	84	399977	41.421	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.840%	
36) 1,2-Dichloropropane-d6	6.069	67	127798	42.478	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	84.960%	
41) Toluene-d8	7.313	98	346047	40.451	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	80.900%	
43) trans-1,3-Dichloroprop...	7.622	79	50673	38.763	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	77.520%	
47) 2-Hexanone-d5	8.088	63	89343	78.236	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	78.240%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	156025	43.724	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	87.440%	
66) 1,2-Dichlorobenzene-d4	11.622	152	117046	44.148	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.300%	
Target Compounds						Qvalue
34) Trichloroethene	5.918	95	18349	7.613	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024934.D
Acq On : 10 Mar 2022 23:18
Operator : SY/MD
Sample : N1879-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D86


Quant Time: Mar 11 05:26:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 05:21:24 2022
Response via : Initial Calibration

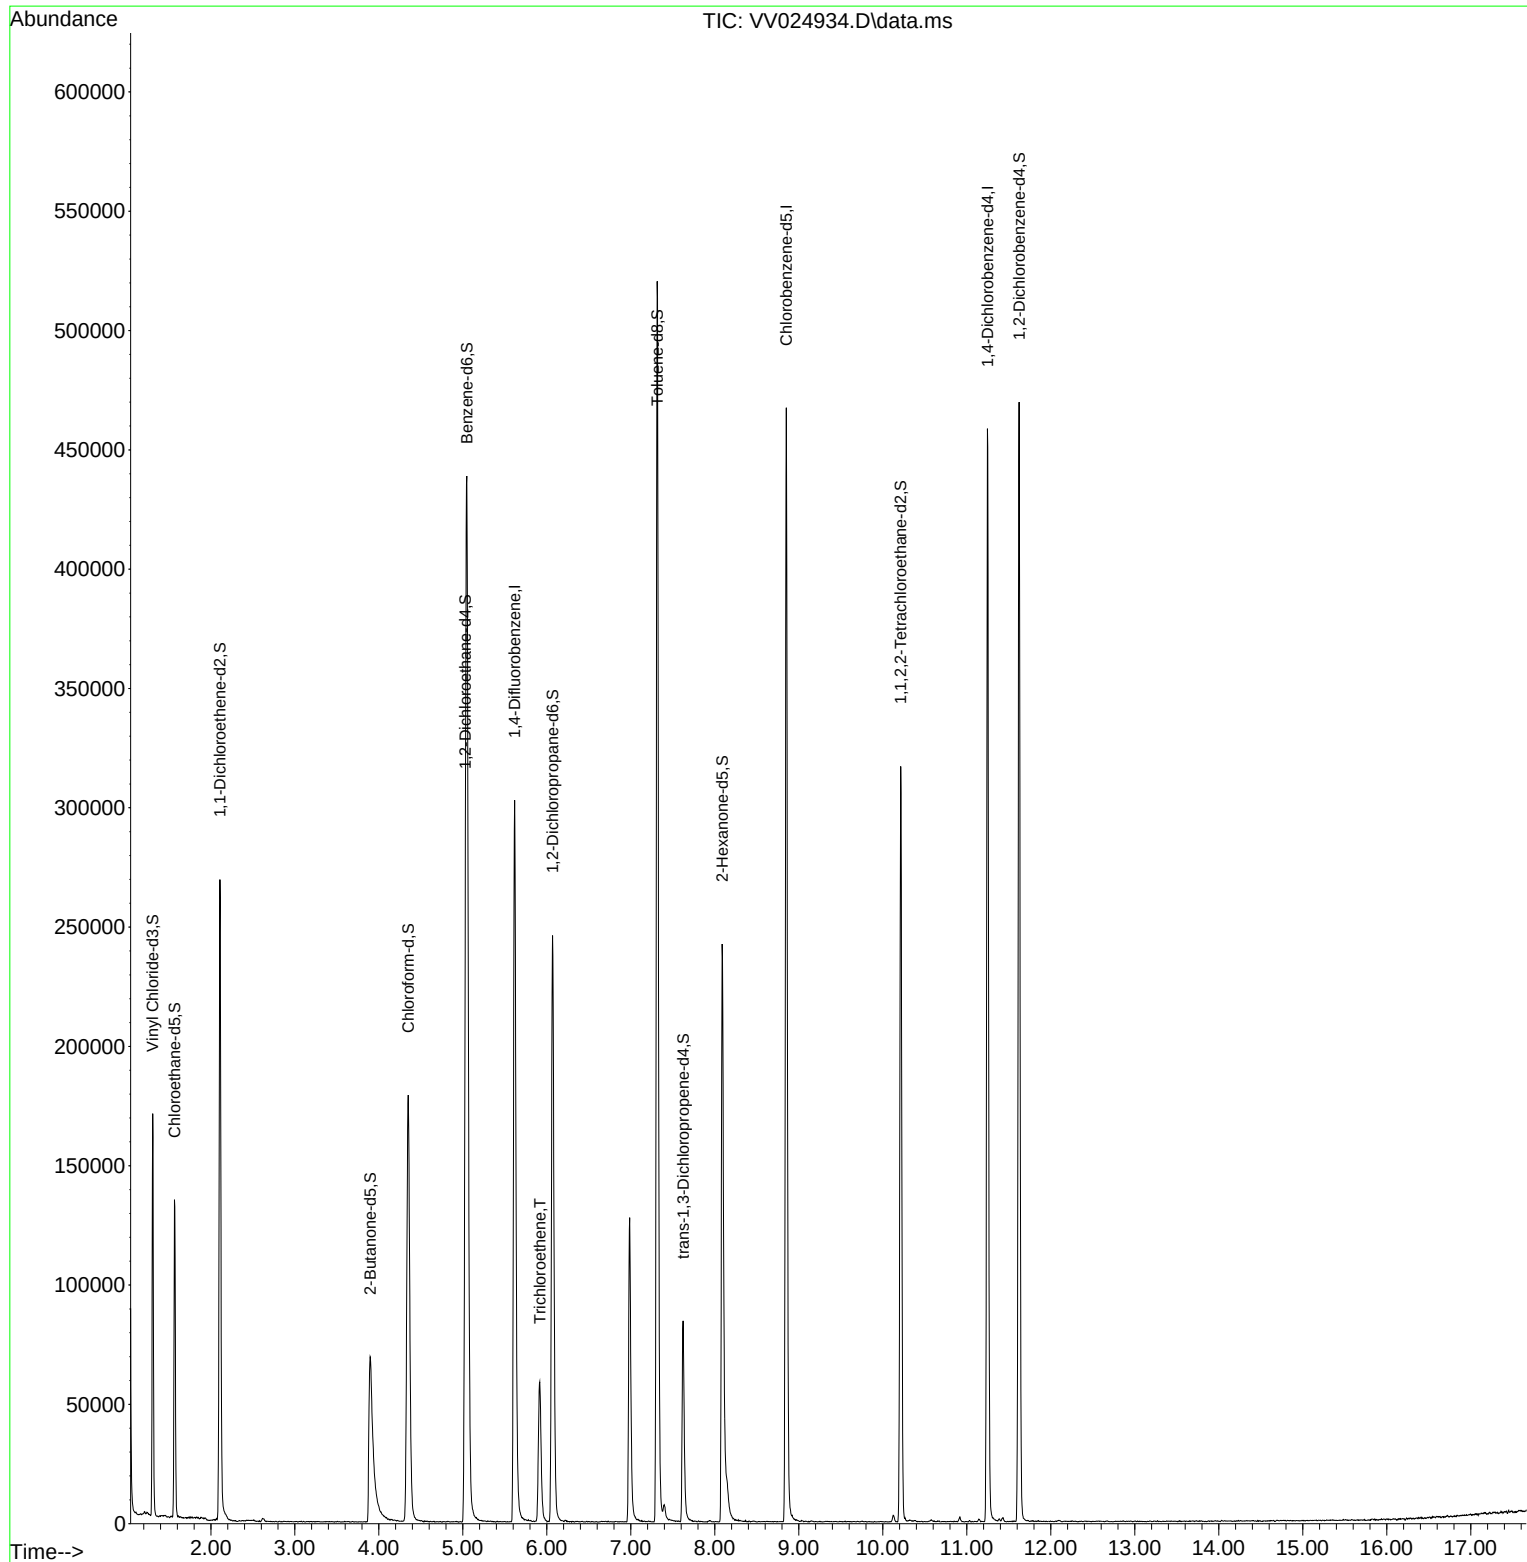

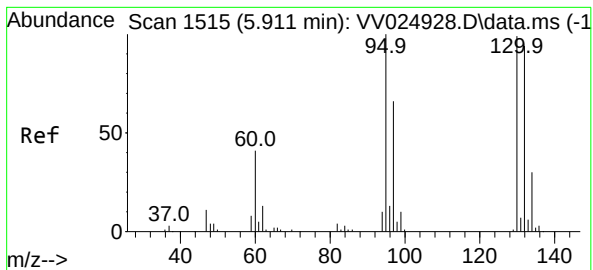

#34
 Trichloroethene
 Concen: 7.613 ug/L
 RT: 5.918 min Scan# 11
 Delta R.T. 0.007 min
 Lab File: VV024934.D
 Acq: 10 Mar 2022 23:18

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D86

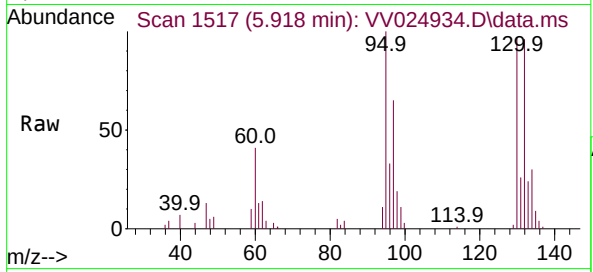

Tgt Ion:	95	Resp:	18349
Ion	Ratio	Lower	Upper
95	100		
97	64.7	45.3	84.1
132	95.8	65.0	120.6
130	96.9	69.3	128.7

