

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024942.D
 Acq On : 11 Mar 2022 02:28
 Operator : SY/MD
 Sample : N1856-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D67

Quant Time: Mar 11 05:28:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 05:21:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	280853	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	271726	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	123455	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	110778	38.791	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	77.580%	
7) Chloroethane-d5	1.571	69	89132	39.782	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	79.560%	
11) 1,1-Dichloroethene-d2	2.108	63	145509	30.358	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	60.720%	
21) 2-Butanone-d5	3.892	46	127831	78.655	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	78.660%	
24) Chloroform-d	4.349	84	202585	40.638	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	81.280%	
26) 1,2-Dichloroethane-d4	5.030	65	123232	41.897	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.800%	
32) Benzene-d6	5.050	84	421861	41.886	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	83.780%	
36) 1,2-Dichloropropane-d6	6.069	67	133696	42.607	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	85.220%	
41) Toluene-d8	7.317	98	369180	41.375	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.760%	
43) trans-1,3-Dichloroprop...	7.622	79	53381	39.150	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	78.300%	
47) 2-Hexanone-d5	8.088	63	87637	73.578	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	73.580%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	160115	43.020	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	86.040%	
66) 1,2-Dichlorobenzene-d4	11.622	152	124504	43.781	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	87.560%	
Target Compounds					Qvalue	
34) Trichloroethene	5.918	95	17287	6.876	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024942.D
Acq On : 11 Mar 2022 02:28
Operator : SY/MD
Sample : N1856-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D67


Quant Time: Mar 11 05:28:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 05:21:24 2022
Response via : Initial Calibration

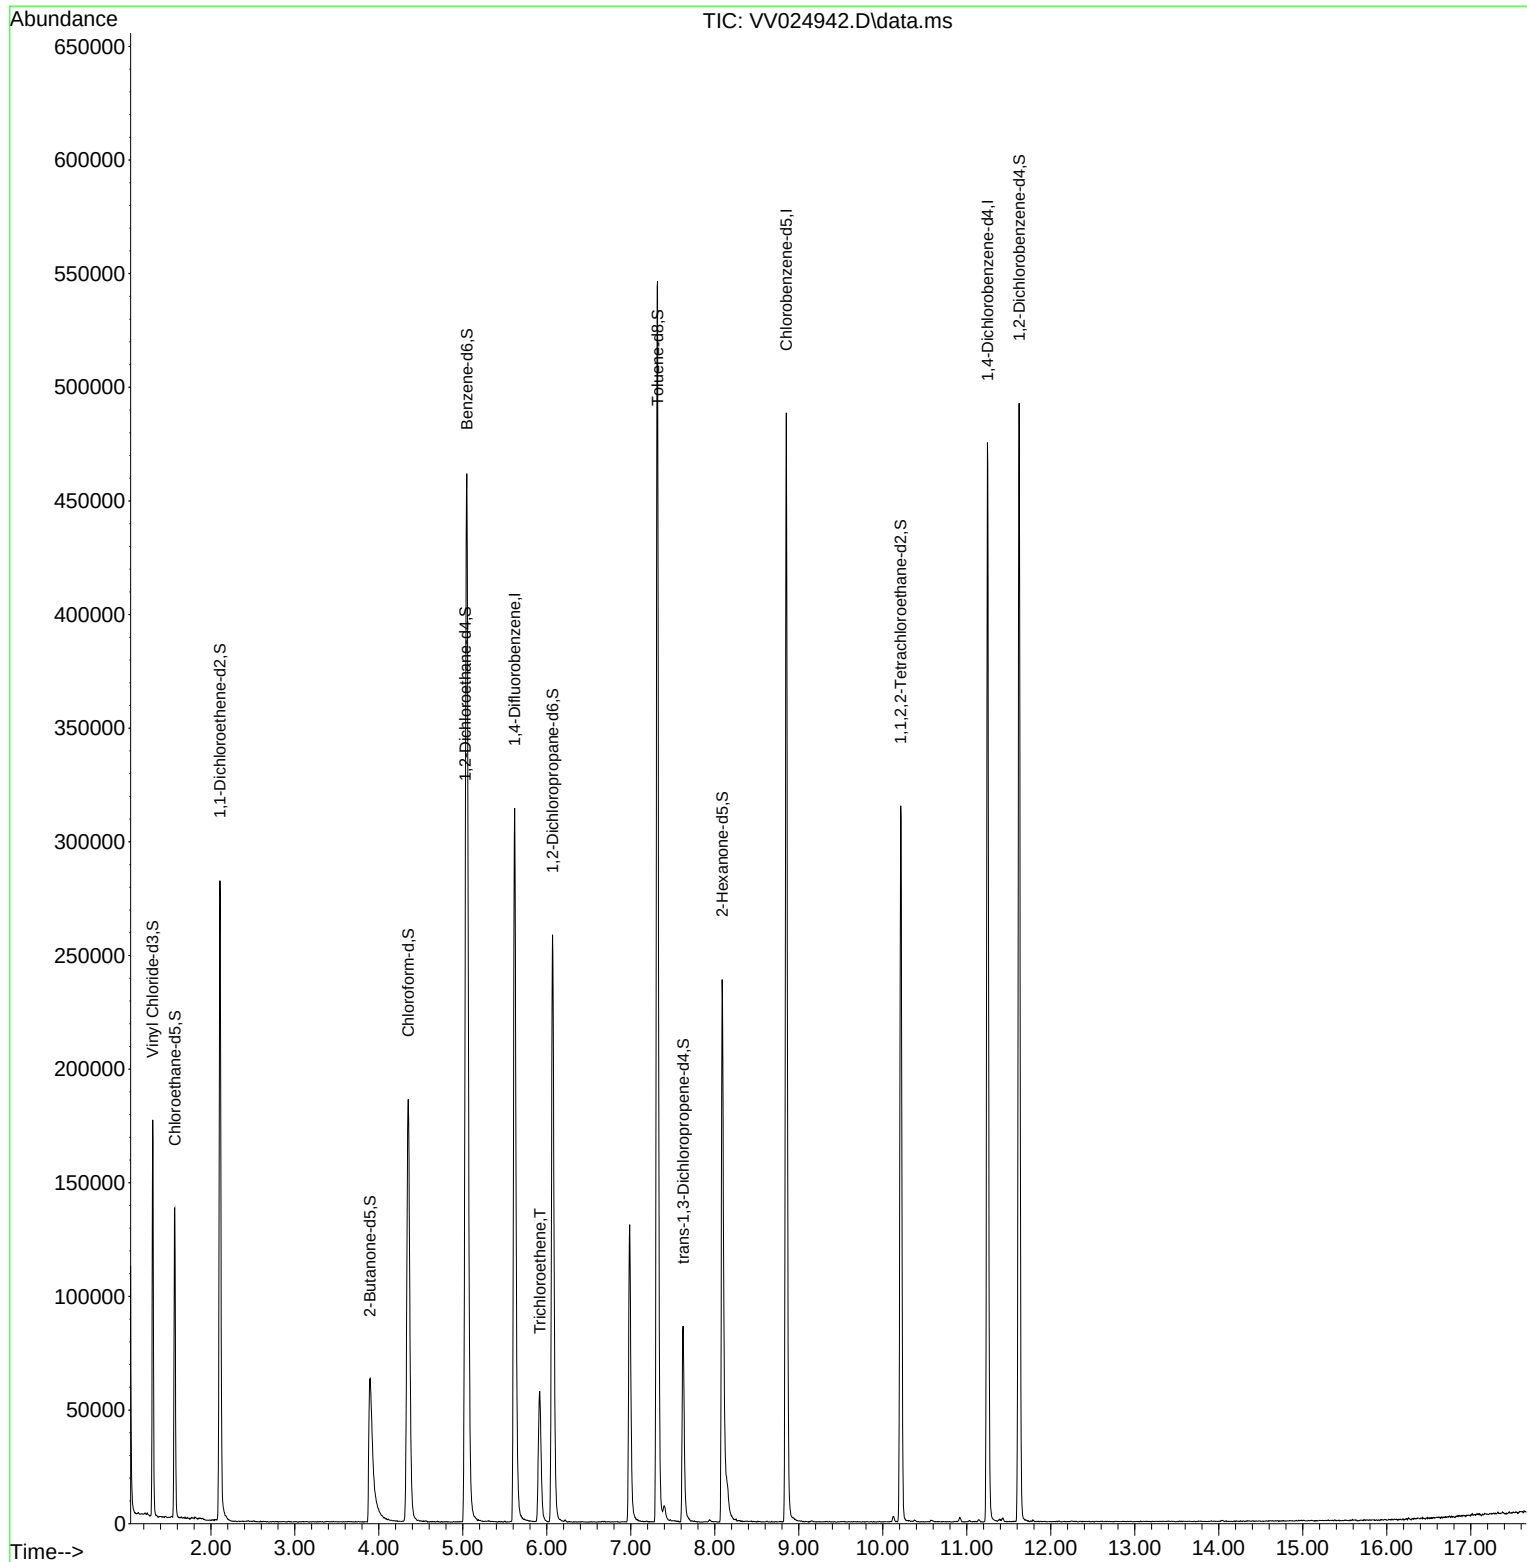

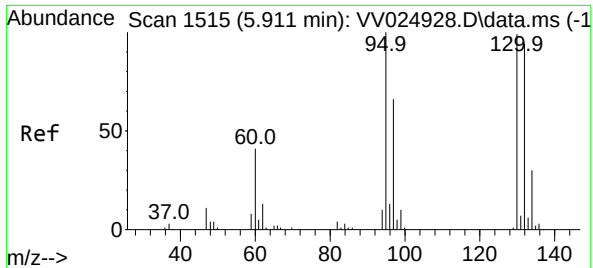

#34
 Trichloroethene
 Concen: 6.876 ug/L
 RT: 5.918 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VV024942.D
 Acq: 11 Mar 2022 02:28

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D67

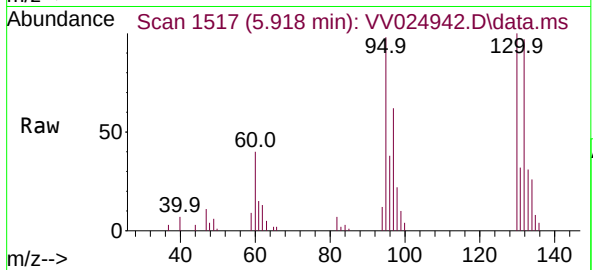

Tgt Ion:	95	Resp:	17287
Ion	Ratio	Lower	Upper
95	100		
97	63.9	45.3	84.1
132	99.9	65.0	120.6
130	102.5	69.3	128.7

