

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024911.D
 Acq On : 10 Mar 2022 13:22
 Operator : SY/MD
 Sample : N1855-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024911.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	46	51	58	rVB	12153	11044	0.21%	0.072%
2	1.307	76	83	102	rVB	158880	161341	3.06%	1.050%
3	1.568	157	164	178	rVB	143019	163912	3.11%	1.066%
4	2.111	322	333	366	rBV2	371603	637097	12.07%	4.145%
5	2.378	412	416	421	rBV2	304	317	0.01%	0.002%
6	2.410	422	426	430	rVV	400	331	0.01%	0.002%
7	2.436	433	434	439	rVV3	470	291	0.01%	0.002%
8	2.462	439	442	448	rVV3	513	521	0.01%	0.003%
9	2.507	452	456	463	rVV3	708	915	0.02%	0.006%
10	2.642	496	498	505	rVB2	543	400	0.01%	0.003%
11	2.674	505	508	510	rBV	357	276	0.01%	0.002%
12	2.693	512	514	518	rVV	444	319	0.01%	0.002%
13	2.719	519	522	526	rVV2	258	247	0.00%	0.002%
14	2.770	528	538	546	rVB5	1601	2520	0.05%	0.016%
15	3.082	631	635	638	rVV	273	239	0.00%	0.002%
16	3.121	644	647	652	rVV2	256	282	0.01%	0.002%
17	3.146	652	655	659	rVV	282	262	0.00%	0.002%
18	3.195	660	670	686	rVB	4255	8996	0.17%	0.059%
19	3.799	854	858	865	rBV2	323	364	0.01%	0.002%
20	3.838	865	870	873	rBV2	333	315	0.01%	0.002%
21	3.908	877	892	945	rBV2	205161	640077	12.13%	4.164%
22	4.198	978	982	986	rVB2	403	313	0.01%	0.002%
23	4.349	1013	1029	1054	rBV	210422	520141	9.86%	3.384%
24	4.609	1093	1110	1140	rVB2	96956	241966	4.59%	1.574%
25	4.970	1216	1222	1228	rBV2	255	334	0.01%	0.002%
26	5.047	1228	1246	1282	rBV2	499804	1283696	24.33%	8.351%
27	5.532	1395	1397	1401	rVB2	316	196	0.00%	0.001%
28	5.616	1411	1423	1453	rBV	340731	682624	12.94%	4.441%
29	5.912	1500	1515	1551	rBV	2744661	5276964	100.00%	34.329%
30	6.069	1551	1564	1594	rVB	287877	584192	11.07%	3.800%
31	6.294	1630	1634	1636	rVB2	342	263	0.00%	0.002%
32	6.458	1682	1685	1691	rVB2	244	201	0.00%	0.001%
33	6.577	1719	1722	1725	rVB2	303	210	0.00%	0.001%
34	6.638	1731	1741	1745	rBV3	1312	2231	0.04%	0.015%
35	6.680	1752	1754	1761	rVB4	502	457	0.01%	0.003%
36	6.738	1770	1772	1776	rVB2	412	259	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024911.D
 Acq On : 10 Mar 2022 13:22
 Operator : SY/MD
 Sample : N1855-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COD38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.892	1817	1820	1827	rBV	230	245	0.00%	0.002%
38	6.986	1838	1849	1873	rBV	143128	258341	4.90%	1.681%
39	7.182	1904	1910	1912	rBV3	724	818	0.02%	0.005%
40	7.252	1930	1932	1936	rVB2	328	218	0.00%	0.001%
41	7.313	1939	1951	1970	rBV	592004	1008499	19.11%	6.561%
42	7.481	2000	2003	2007	rVB2	353	240	0.00%	0.002%
43	7.622	2036	2047	2069	rBV	91943	162570	3.08%	1.058%
44	7.809	2102	2105	2110	rVB3	328	284	0.01%	0.002%
45	7.847	2110	2117	2128	rBV4	2045	3964	0.08%	0.026%
46	7.940	2139	2146	2155	rVB2	1816	2734	0.05%	0.018%
47	8.021	2168	2171	2174	rVB2	305	225	0.00%	0.001%
48	8.047	2174	2179	2182	rBV2	390	425	0.01%	0.003%
49	8.088	2182	2192	2236	rBV	307865	614945	11.65%	4.000%
50	8.394	2284	2287	2298	rVB	517	619	0.01%	0.004%
51	8.551	2332	2336	2340	rBV2	298	284	0.01%	0.002%
52	8.577	2340	2344	2351	rVB2	314	373	0.01%	0.002%
53	8.612	2351	2355	2358	rBV2	475	381	0.01%	0.002%
54	8.850	2417	2429	2456	rBV	522242	845433	16.02%	5.500%
55	9.018	2477	2481	2482	rBV2	306	202	0.00%	0.001%
56	9.143	2515	2520	2526	rBV3	590	806	0.02%	0.005%
57	9.227	2542	2546	2553	rBV2	284	266	0.01%	0.002%
58	9.317	2571	2574	2577	rVV	348	241	0.00%	0.002%
59	9.368	2581	2590	2595	rBV	337	429	0.01%	0.003%
60	9.465	2615	2620	2623	rBV	308	288	0.01%	0.002%
61	9.686	2687	2689	2696	rVB2	355	260	0.00%	0.002%
62	9.764	2710	2713	2719	rBV2	255	250	0.00%	0.002%
63	9.879	2745	2749	2753	rVB2	287	227	0.00%	0.001%
64	10.030	2791	2796	2801	rVB2	236	259	0.00%	0.002%
65	10.124	2817	2825	2832	rBV4	1115	1605	0.03%	0.010%
66	10.156	2832	2835	2839	rVB	259	221	0.00%	0.001%
67	10.214	2839	2853	2872	rBV	370736	573836	10.87%	3.733%
68	10.384	2899	2906	2913	rBV5	1772	2284	0.04%	0.015%
69	10.445	2922	2925	2932	rVB2	237	217	0.00%	0.001%
70	10.481	2932	2936	2939	rBV2	285	216	0.00%	0.001%
71	10.522	2946	2949	2953	rVB2	310	225	0.00%	0.001%
72	10.580	2962	2967	2972	rVB4	390	448	0.01%	0.003%
73	10.918	3065	3072	3080	rBV6	994	1678	0.03%	0.011%
74	11.014	3097	3102	3106	rBV2	205	225	0.00%	0.001%
75	11.140	3136	3141	3143	rBV2	504	342	0.01%	0.002%
76	11.201	3153	3160	3163	rBV2	270	344	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024911.D
 Acq On : 10 Mar 2022 13:22
 Operator : SY/MD
 Sample : N1855-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.246	3163	3174	3196	rBV	520501	792632	15.02%	5.156%
78	11.423	3224	3229	3235	rVB4	702	735	0.01%	0.005%
79	11.567	3270	3274	3279	rBV2	332	310	0.01%	0.002%
80	11.622	3279	3291	3311	rBV	562556	862660	16.35%	5.612%
81	11.780	3337	3340	3344	rVB2	366	316	0.01%	0.002%
82	11.818	3344	3352	3354	rBV2	186	264	0.01%	0.002%
83	11.969	3397	3399	3406	rVB2	279	247	0.00%	0.002%
84	12.008	3406	3411	3414	rVB	269	244	0.00%	0.002%
85	12.243	3479	3484	3486	rBV2	532	504	0.01%	0.003%
86	12.583	3587	3590	3594	rBV2	292	233	0.00%	0.002%
87	12.686	3619	3622	3625	rVB	367	238	0.00%	0.002%
88	13.117	3751	3756	3759	rBV2	241	243	0.00%	0.002%
89	13.696	3933	3936	3941	rVB2	332	261	0.00%	0.002%
90	13.995	4027	4029	4038	rVB	382	317	0.01%	0.002%
91	14.217	4095	4098	4100	rBV2	341	194	0.00%	0.001%
92	14.416	4157	4160	4163	rVB2	423	251	0.00%	0.002%
93	14.435	4163	4166	4170	rBV	288	230	0.00%	0.001%
94	14.513	4186	4190	4193	rBV3	269	283	0.01%	0.002%
95	14.567	4205	4207	4213	rBV3	225	201	0.00%	0.001%
96	14.734	4253	4259	4261	rBV3	460	462	0.01%	0.003%
97	14.786	4272	4275	4278	rBV	237	206	0.00%	0.001%
98	15.599	4525	4528	4531	rBV	450	300	0.01%	0.002%
99	16.184	4707	4710	4714	rVB2	748	463	0.01%	0.003%
100	16.316	4748	4751	4754	rBV2	678	535	0.01%	0.003%




Sum of corrected areas: 15371909

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024911.D
Acq On : 10 Mar 2022 13:22
Operator : SY/MD
Sample : N1855-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

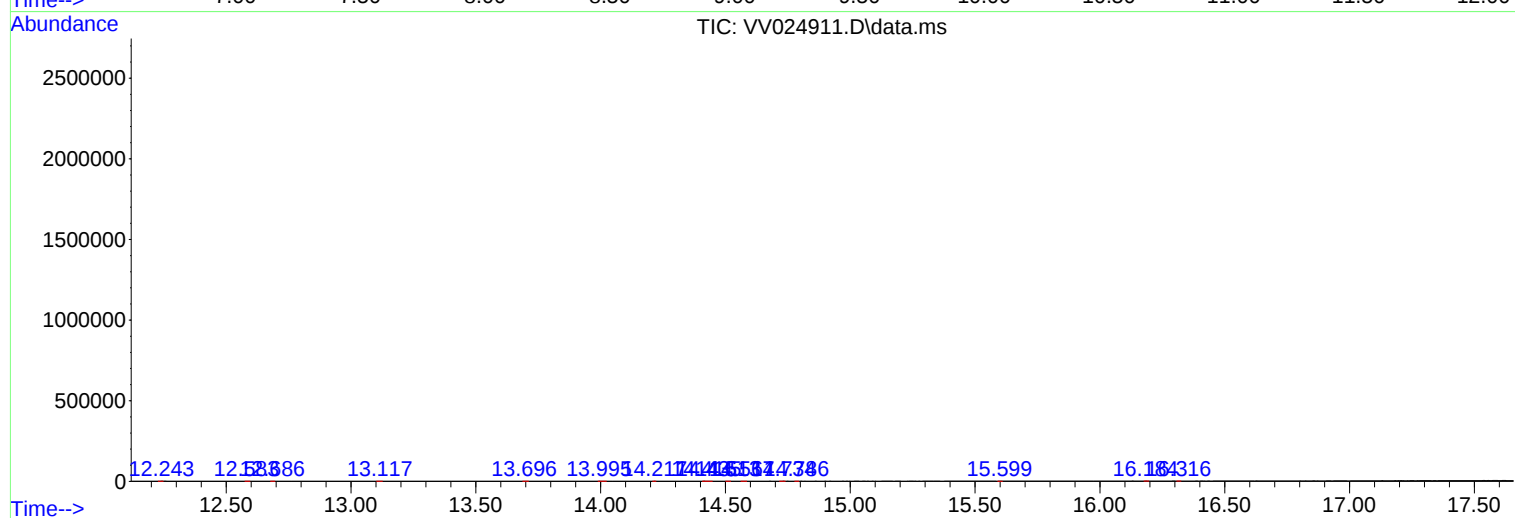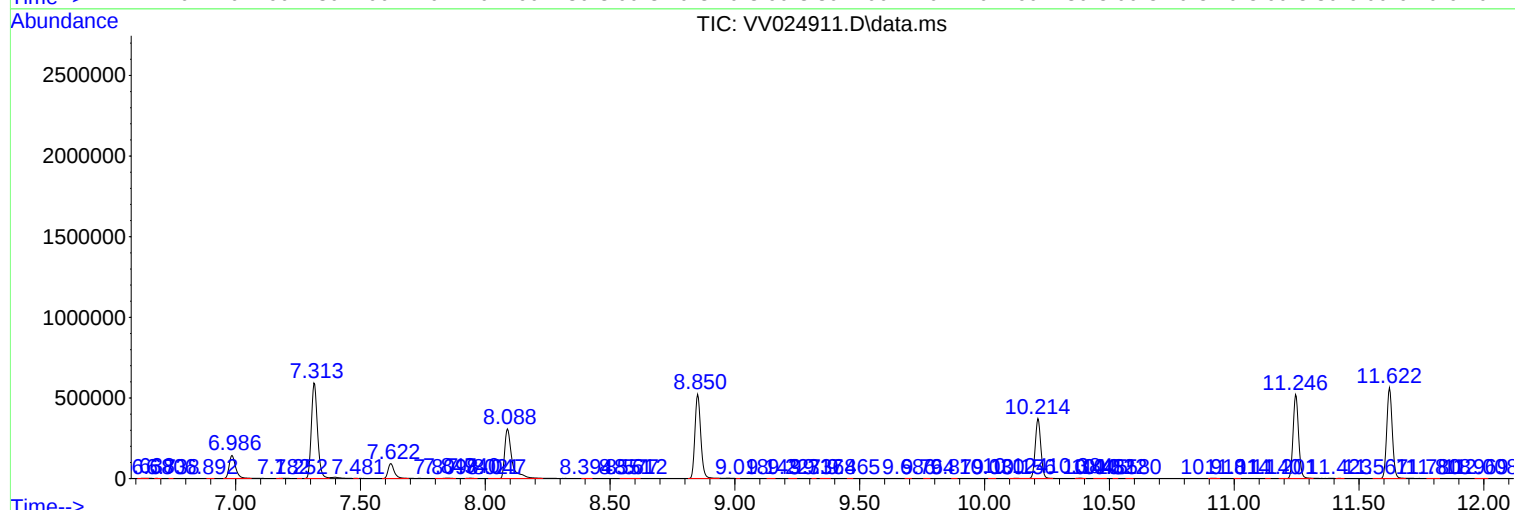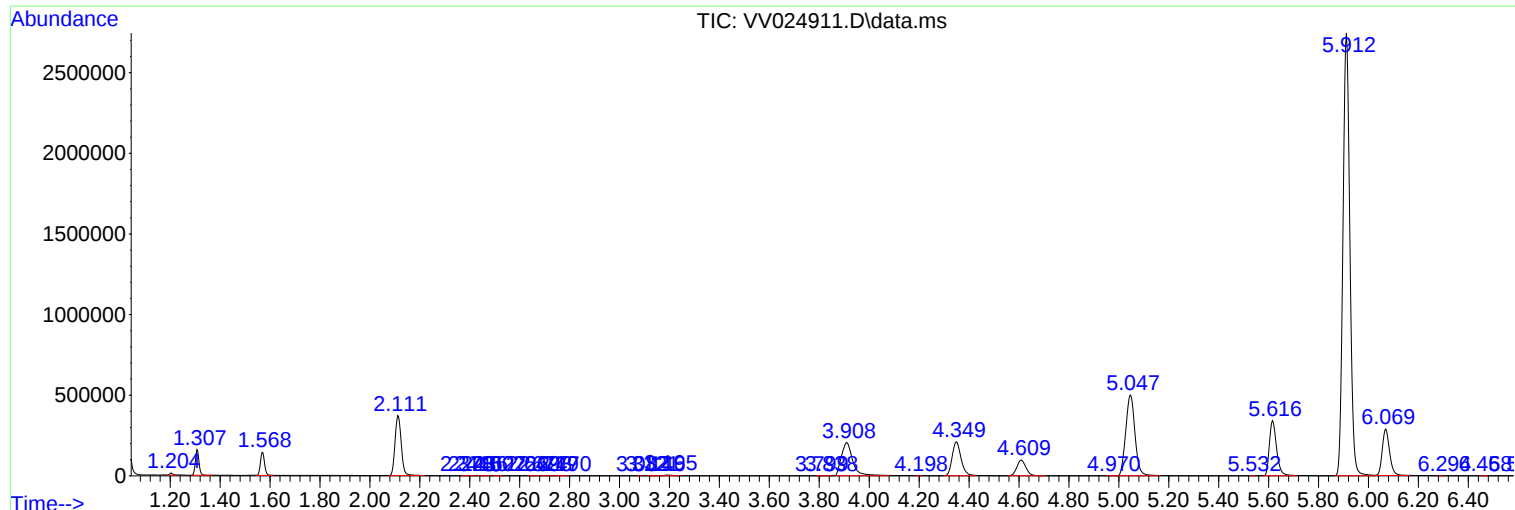

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024911.D
Acq On : 10 Mar 2022 13:22
Operator : SY/MD
Sample : N1855-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024911.D
Acq On : 10 Mar 2022 13:22
Operator : SY/MD
Sample : N1855-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------