

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024912.D
 Acq On : 10 Mar 2022 13:46
 Operator : SY/MD
 Sample : N1855-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024912.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB	201089	200828	16.52%	2.283%
2	1.568	157	164	182	rVB	151546	172371	14.18%	1.959%
3	2.108	322	332	350	rBV	312413	457754	37.65%	5.203%
4	2.925	582	586	590	rBV2	265	271	0.02%	0.003%
5	3.140	650	653	657	rBV2	231	150	0.01%	0.002%
6	3.204	670	673	674	rBV	198	92	0.01%	0.001%
7	3.378	723	727	730	rBV2	235	185	0.02%	0.002%
8	3.436	742	745	749	rBV	164	125	0.01%	0.001%
9	3.474	754	757	759	rBV2	136	90	0.01%	0.001%
10	3.552	773	781	785	rBV2	207	301	0.02%	0.003%
11	3.593	785	794	799	rBV2	263	436	0.04%	0.005%
12	3.648	808	811	816	rBV2	205	181	0.01%	0.002%
13	3.674	816	819	823	rVB2	301	203	0.02%	0.002%
14	3.696	823	826	829	rBV2	180	118	0.01%	0.001%
15	3.809	858	861	862	rBV	165	106	0.01%	0.001%
16	3.896	878	888	940	rBV	64804	234086	19.25%	2.661%
17	4.349	1014	1029	1054	rBV	191006	473867	38.98%	5.387%
18	4.728	1144	1147	1149	rBV2	220	138	0.01%	0.002%
19	4.905	1199	1202	1204	rBV	162	107	0.01%	0.001%
20	4.928	1207	1209	1213	rVB	285	142	0.01%	0.002%
21	5.047	1229	1246	1286	rBV2	477928	1215786	100.00%	13.820%
22	5.416	1359	1361	1367	rVB2	603	422	0.03%	0.005%
23	5.449	1367	1371	1375	rBV	405	391	0.03%	0.004%
24	5.506	1386	1389	1392	rBV2	216	165	0.01%	0.002%
25	5.532	1395	1397	1399	rBV	110	65	0.01%	0.001%
26	5.616	1411	1423	1451	rBV	323584	649949	53.46%	7.388%
27	5.912	1503	1515	1542	rVB5	42631	100267	8.25%	1.140%
28	6.024	1547	1550	1551	rBV	211	117	0.01%	0.001%
29	6.069	1551	1564	1589	rBV	266242	534713	43.98%	6.078%
30	6.211	1606	1608	1611	rBV2	542	393	0.03%	0.004%
31	6.262	1621	1624	1627	rBV2	266	180	0.01%	0.002%
32	6.294	1632	1634	1640	rVV2	228	213	0.02%	0.002%
33	6.359	1653	1654	1655	rBV	115	30	0.00%	0.000%
34	6.449	1679	1682	1685	rBV2	279	188	0.02%	0.002%
35	6.522	1702	1705	1707	rBV	167	101	0.01%	0.001%
36	6.558	1714	1716	1719	rBV	124	78	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024912.D
 Acq On : 10 Mar 2022 13:46
 Operator : SY/MD
 Sample : N1855-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.574	1719	1721	1724	rBV2	220	157	0.01%	0.002%
38	6.706	1760	1762	1763	rBV	205	87	0.01%	0.001%
39	6.738	1769	1772	1777	rVB	133	91	0.01%	0.001%
40	6.857	1806	1809	1813	rBV2	187	170	0.01%	0.002%
41	6.986	1838	1849	1871	rBV	139541	250844	20.63%	2.851%
42	7.211	1915	1919	1921	rBV4	457	422	0.03%	0.005%
43	7.252	1931	1932	1936	rBV2	219	142	0.01%	0.002%
44	7.313	1940	1951	1970	rBV	581207	987403	81.22%	11.224%
45	7.622	2036	2047	2069	rBV	90665	159526	13.12%	1.813%
46	7.805	2102	2104	2107	rBV2	201	115	0.01%	0.001%
47	7.825	2107	2110	2113	rBV	215	152	0.01%	0.002%
48	7.873	2121	2125	2128	rBV2	378	390	0.03%	0.004%
49	7.937	2140	2145	2152	rVB3	733	908	0.07%	0.010%
50	7.992	2158	2162	2164	rBV2	206	152	0.01%	0.002%
51	8.088	2182	2192	2235	rBV	237900	474351	39.02%	5.392%
52	8.420	2292	2295	2296	rBV2	215	122	0.01%	0.001%
53	8.516	2322	2325	2329	rBV2	175	138	0.01%	0.002%
54	8.542	2330	2333	2335	rBV2	155	107	0.01%	0.001%
55	8.587	2345	2347	2349	rBV	121	61	0.01%	0.001%
56	8.616	2353	2356	2364	rVB3	479	430	0.04%	0.005%
57	8.731	2385	2392	2395	rBV2	203	282	0.02%	0.003%
58	8.789	2405	2410	2413	rBV2	246	282	0.02%	0.003%
59	8.850	2418	2429	2453	rBV	504578	813183	66.89%	9.244%
60	9.056	2491	2493	2497	rBV2	381	274	0.02%	0.003%
61	9.111	2505	2510	2513	rBV2	480	441	0.04%	0.005%
62	9.137	2515	2518	2520	rBV2	204	149	0.01%	0.002%
63	9.198	2532	2537	2542	rVB2	279	275	0.02%	0.003%
64	9.233	2542	2548	2554	rBV2	262	315	0.03%	0.004%
65	9.265	2555	2558	2560	rBV2	108	69	0.01%	0.001%
66	9.310	2566	2572	2578	rBV2	379	502	0.04%	0.006%
67	9.336	2578	2580	2582	rBV2	111	64	0.01%	0.001%
68	9.503	2629	2632	2634	rBV	251	185	0.02%	0.002%
69	9.580	2652	2656	2661	rBV2	292	308	0.03%	0.004%
70	9.683	2686	2688	2690	rBV2	116	67	0.01%	0.001%
71	9.719	2696	2699	2702	rBV	239	178	0.01%	0.002%
72	9.757	2708	2711	2716	rVB2	188	104	0.01%	0.001%
73	9.876	2744	2748	2754	rBV2	286	354	0.03%	0.004%
74	10.127	2819	2826	2836	rVB2	3280	4644	0.38%	0.053%
75	10.214	2841	2853	2870	rBV	317919	490121	40.31%	5.571%
76	10.455	2925	2928	2932	rBV2	183	189	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024912.D
 Acq On : 10 Mar 2022 13:46
 Operator : SY/MD
 Sample : N1855-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M

Title : VOC Analysis

77	10.799	3032	3035	3040	rBV2	221	238	0.02%	0.003%
78	10.915	3064	3071	3081	rVB4	2368	3537	0.29%	0.040%
79	11.246	3163	3174	3193	rBV	506753	766169	63.02%	8.709%
80	11.622	3279	3291	3314	rBV	510717	792773	65.21%	9.012%
81	11.837	3355	3358	3359	rBV	245	143	0.01%	0.002%
82	11.979	3398	3402	3406	rBV2	450	427	0.04%	0.005%
83	12.053	3423	3425	3427	rBV2	285	135	0.01%	0.002%
84	12.136	3447	3451	3454	rBV2	391	267	0.02%	0.003%
85	12.252	3481	3487	3494	rBV3	501	842	0.07%	0.010%
86	13.538	3885	3887	3889	rBV	234	141	0.01%	0.002%
87	14.500	4183	4186	4187	rBV	343	221	0.02%	0.003%




Sum of corrected areas: 8797256

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024912.D
Acq On : 10 Mar 2022 13:46
Operator : SY/MD
Sample : N1855-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

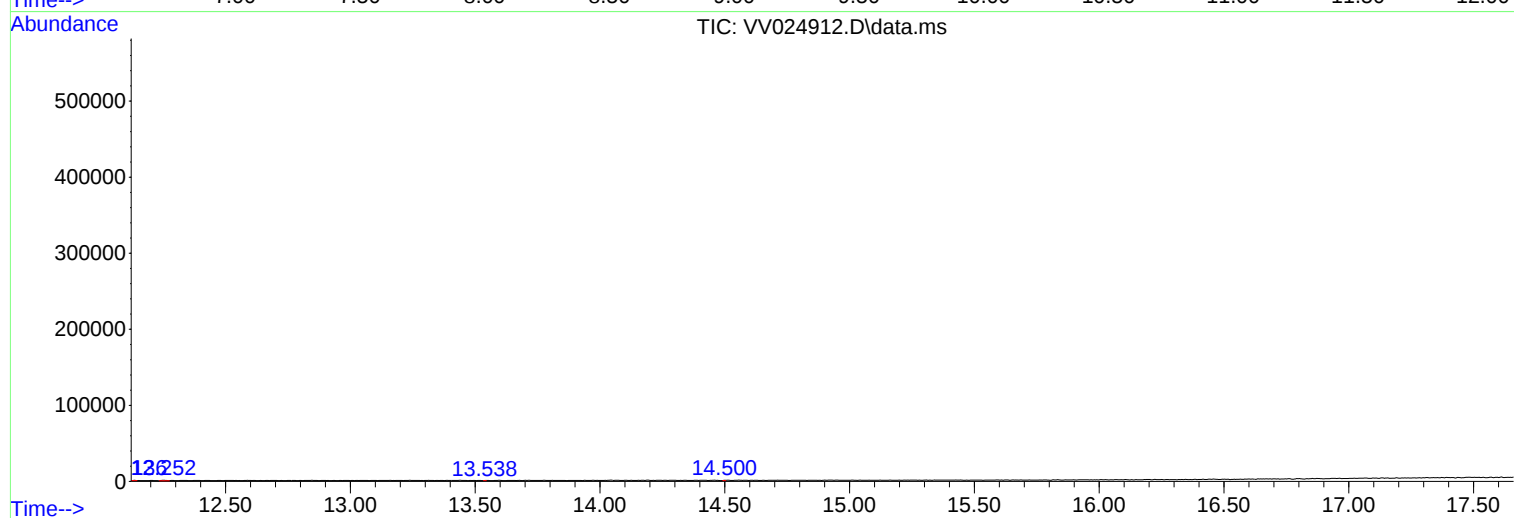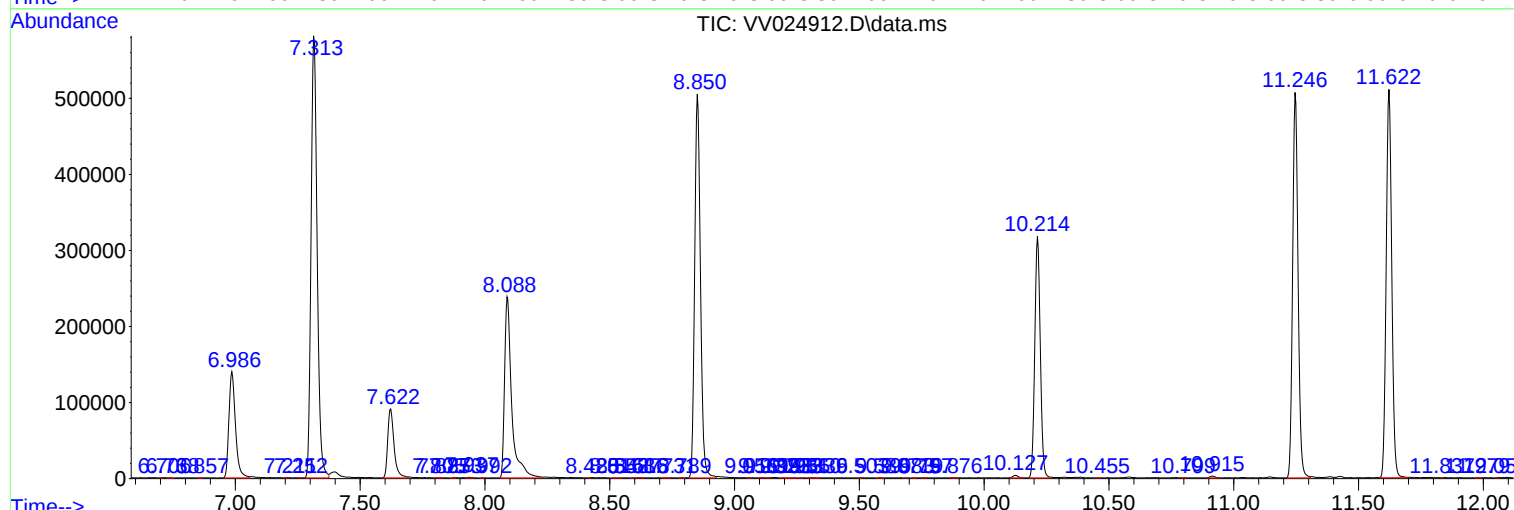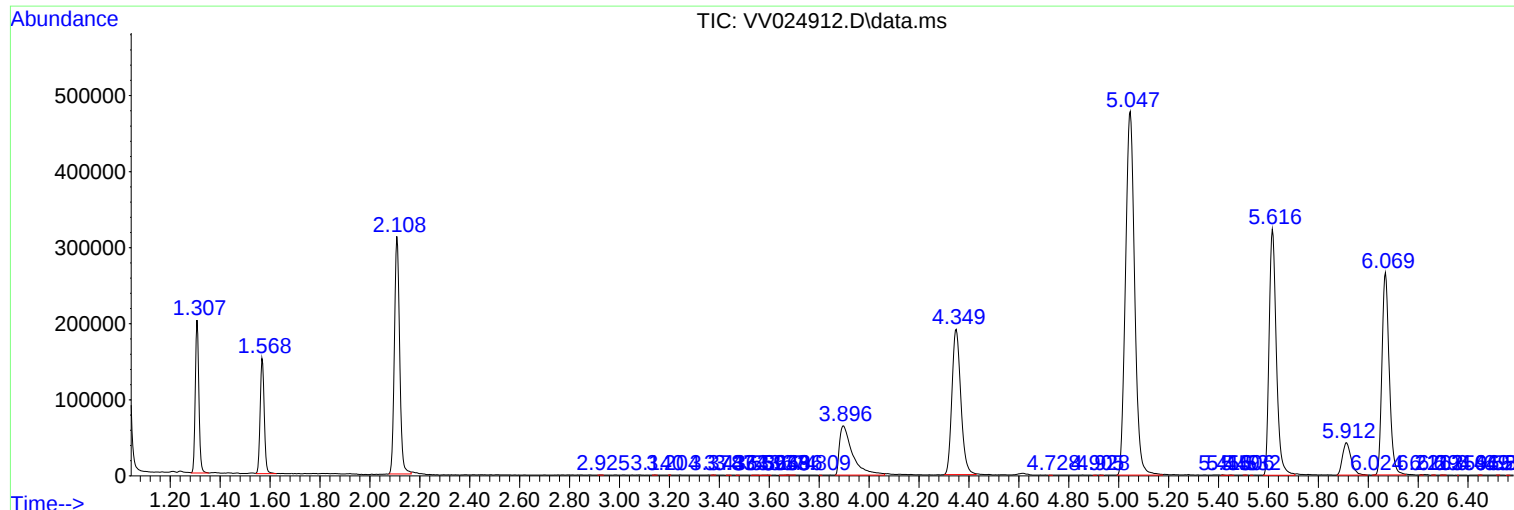

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024912.D
Acq On : 10 Mar 2022 13:46
Operator : SY/MD
Sample : N1855-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024912.D
Acq On : 10 Mar 2022 13:46
Operator : SY/MD
Sample : N1855-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------