

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024913.D
 Acq On : 10 Mar 2022 14:10
 Operator : SY/MD
 Sample : N1855-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024913.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	205408	207110	16.54%	2.291%
2	1.568	157	164	178	rVB	156452	176528	14.10%	1.953%
3	2.024	303	306	308	rBV2	445	287	0.02%	0.003%
4	2.108	321	332	364	rBV	316732	467860	37.36%	5.176%
5	2.275	381	384	387	rVB	403	254	0.02%	0.003%
6	2.294	387	390	394	rVB3	375	250	0.02%	0.003%
7	2.407	421	425	431	rVB2	439	403	0.03%	0.004%
8	2.468	439	444	447	rBV2	465	494	0.04%	0.005%
9	2.516	453	459	462	rVB3	474	511	0.04%	0.006%
10	2.603	481	486	488	rBV2	304	265	0.02%	0.003%
11	2.674	505	508	514	rVV2	261	221	0.02%	0.002%
12	2.828	545	556	560	rBV2	428	685	0.05%	0.008%
13	3.076	629	633	637	rBV	257	219	0.02%	0.002%
14	3.127	643	649	652	rBV2	336	396	0.03%	0.004%
15	3.227	673	680	683	rBV2	215	267	0.02%	0.003%
16	3.249	683	687	692	rBV2	204	244	0.02%	0.003%
17	3.317	698	708	711	rBV2	190	303	0.02%	0.003%
18	3.362	716	722	725	rBV	316	300	0.02%	0.003%
19	3.526	763	773	776	rBV2	376	627	0.05%	0.007%
20	3.895	878	888	943	rBV2	64378	233138	18.62%	2.579%
21	4.230	988	992	994	rBV3	295	219	0.02%	0.002%
22	4.349	1013	1029	1057	rBV	198505	489861	39.12%	5.419%
23	4.680	1130	1132	1140	rVB	440	232	0.02%	0.003%
24	4.783	1161	1164	1170	rBV2	254	233	0.02%	0.003%
25	4.963	1215	1220	1223	rBV2	332	257	0.02%	0.003%
26	5.047	1229	1246	1277	rBV2	498808	1252352	100.00%	13.855%
27	5.368	1343	1346	1350	rBV2	227	209	0.02%	0.002%
28	5.407	1355	1358	1363	rBV2	380	371	0.03%	0.004%
29	5.458	1371	1374	1378	rVB2	302	253	0.02%	0.003%
30	5.616	1411	1423	1457	rBV	331259	662539	52.90%	7.330%
31	5.796	1475	1479	1484	rBV2	330	301	0.02%	0.003%
32	5.911	1503	1515	1538	rVB5	34732	83873	6.70%	0.928%
33	6.069	1550	1564	1593	rBV	275593	552910	44.15%	6.117%
34	6.243	1617	1618	1622	rVB3	473	228	0.02%	0.003%
35	6.503	1695	1699	1704	rVB2	248	210	0.02%	0.002%
36	6.641	1736	1742	1745	rBV2	338	274	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024913.D
 Acq On : 10 Mar 2022 14:10
 Operator : SY/MD
 Sample : N1855-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.664	1745	1749	1758	rVB3	322	501	0.04%	0.006%
38	6.783	1784	1786	1791	rBV2	233	212	0.02%	0.002%
39	6.985	1838	1849	1875	rBV	144842	260548	20.80%	2.882%
40	7.313	1940	1951	1970	rBV	584583	1019273	81.39%	11.276%
41	7.622	2037	2047	2070	rBV	95562	163752	13.08%	1.812%
42	7.760	2088	2090	2094	rVB2	516	348	0.03%	0.004%
43	7.792	2094	2100	2103	rBV3	328	369	0.03%	0.004%
44	7.934	2139	2144	2147	rBV2	597	615	0.05%	0.007%
45	8.088	2182	2192	2229	rBV	250160	491868	39.28%	5.442%
46	8.471	2308	2311	2315	rBV	343	276	0.02%	0.003%
47	8.500	2315	2320	2325	rVB2	438	562	0.04%	0.006%
48	8.535	2325	2331	2337	rBV2	336	508	0.04%	0.006%
49	8.850	2418	2429	2463	rBV	509828	829050	66.20%	9.172%
50	9.156	2519	2524	2527	rVV3	303	363	0.03%	0.004%
51	9.291	2561	2566	2569	rVB2	253	221	0.02%	0.002%
52	9.387	2593	2596	2602	rVB2	246	271	0.02%	0.003%
53	9.471	2618	2622	2624	rBV	283	255	0.02%	0.003%
54	9.487	2624	2627	2632	rVV2	302	352	0.03%	0.004%
55	9.564	2643	2651	2653	rBV2	350	383	0.03%	0.004%
56	9.670	2682	2684	2692	rVB2	375	378	0.03%	0.004%
57	9.818	2726	2730	2734	rBV2	224	223	0.02%	0.002%
58	9.841	2734	2737	2744	rVB2	179	208	0.02%	0.002%
59	10.127	2817	2826	2835	rVB2	3454	5160	0.41%	0.057%
60	10.214	2842	2853	2872	rBV	324363	508795	40.63%	5.629%
61	10.316	2880	2885	2889	rBV4	487	670	0.05%	0.007%
62	10.352	2893	2896	2899	rVV4	613	439	0.04%	0.005%
63	10.381	2903	2905	2910	rVB4	975	770	0.06%	0.009%
64	10.461	2923	2930	2934	rBV3	295	366	0.03%	0.004%
65	10.574	2960	2965	2966	rBV3	731	687	0.05%	0.008%
66	10.664	2990	2993	2996	rVB2	419	276	0.02%	0.003%
67	10.837	3040	3047	3051	rBV3	378	477	0.04%	0.005%
68	10.915	3064	3071	3080	rVB4	2847	3920	0.31%	0.043%
69	11.024	3099	3105	3106	rBV	209	221	0.02%	0.002%
70	11.037	3107	3109	3115	rVV2	491	391	0.03%	0.004%
71	11.114	3129	3133	3136	rBV2	319	310	0.02%	0.003%
72	11.149	3136	3144	3148	rVB4	1344	1916	0.15%	0.021%
73	11.246	3163	3174	3192	rBV	513561	775028	61.89%	8.574%
74	11.387	3212	3218	3225	rBV6	1606	2159	0.17%	0.024%
75	11.426	3225	3230	3244	rVB5	2324	3768	0.30%	0.042%
76	11.484	3244	3248	3254	rBV2	304	316	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024913.D
 Acq On : 10 Mar 2022 14:10
 Operator : SY/MD
 Sample : N1855-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.622	3279	3291	3313	rBV	539480	820617	65.53%	9.078%
78	11.776	3332	3339	3340	rBV3	632	607	0.05%	0.007%
79	11.844	3357	3360	3362	rBV	335	262	0.02%	0.003%
80	11.972	3395	3400	3406	rBV2	278	375	0.03%	0.004%
81	12.046	3419	3423	3426	rVB2	375	252	0.02%	0.003%
82	12.085	3431	3435	3436	rBV	442	275	0.02%	0.003%
83	12.252	3482	3487	3494	rBV3	373	476	0.04%	0.005%
84	12.541	3572	3577	3579	rBV2	389	314	0.03%	0.003%
85	12.593	3587	3593	3598	rBV3	476	482	0.04%	0.005%
86	12.734	3635	3637	3646	rVB2	388	392	0.03%	0.004%
87	12.776	3646	3650	3652	rBV2	289	226	0.02%	0.003%
88	12.808	3657	3660	3665	rVB2	332	322	0.03%	0.004%
89	13.152	3760	3767	3769	rBV	352	456	0.04%	0.005%
90	13.207	3780	3784	3789	rBV2	220	269	0.02%	0.003%
91	13.233	3789	3792	3795	rVB2	425	233	0.02%	0.003%
92	13.310	3813	3816	3821	rBV2	207	226	0.02%	0.003%
93	13.696	3932	3936	3941	rVB2	308	334	0.03%	0.004%
94	13.889	3993	3996	3999	rVB	337	215	0.02%	0.002%
95	14.156	4075	4079	4082	rBV2	289	228	0.02%	0.003%
96	14.393	4149	4153	4155	rBV2	419	339	0.03%	0.004%
97	15.406	4466	4468	4471	rBV	308	219	0.02%	0.002%
98	15.959	4637	4640	4642	rBV	530	294	0.02%	0.003%
99	16.139	4693	4696	4699	rVB4	560	365	0.03%	0.004%
100	16.326	4752	4754	4759	rBV4	555	473	0.04%	0.005%


Sum of corrected areas: 9039140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024913.D
Acq On : 10 Mar 2022 14:10
Operator : SY/MD
Sample : N1855-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

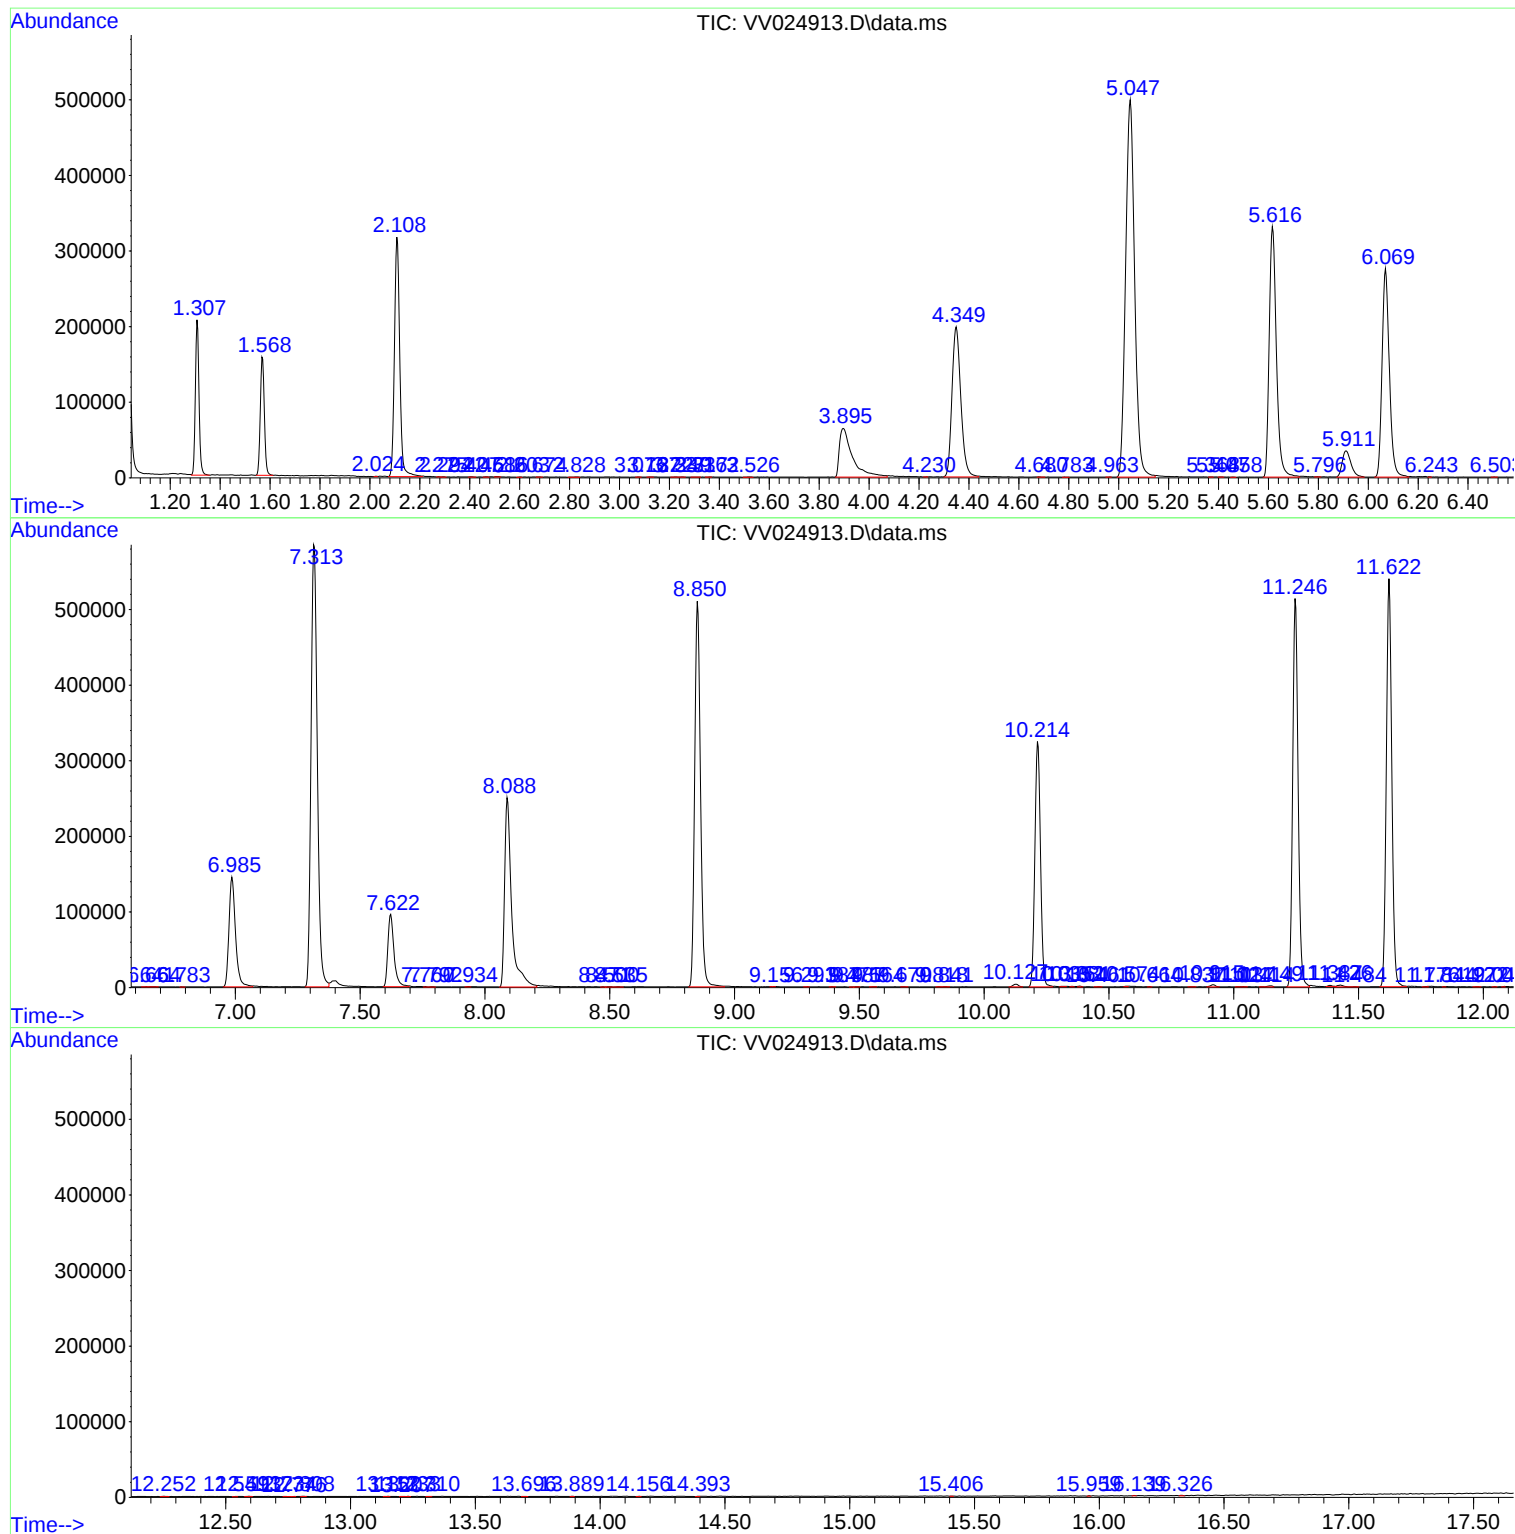

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024913.D
Acq On : 10 Mar 2022 14:10
Operator : SY/MD
Sample : N1855-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024913.D
Acq On : 10 Mar 2022 14:10
Operator : SY/MD
Sample : N1855-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------