

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024918.D
 Acq On : 10 Mar 2022 16:08
 Operator : SY/MD
 Sample : N1855-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024918.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	200075	201599	8.58%	1.771%
2	1.568	157	164	179	rVB	150662	170672	7.26%	1.499%
3	2.111	322	333	354	rBV3	348347	556270	23.66%	4.886%
4	2.510	452	457	465	rBV2	763	938	0.04%	0.008%
5	2.767	533	537	542	rVB4	795	817	0.03%	0.007%
6	2.883	571	573	576	rBV2	169	103	0.00%	0.001%
7	3.005	606	611	614	rBV2	223	254	0.01%	0.002%
8	3.198	664	671	683	rVB3	1685	3089	0.13%	0.027%
9	3.375	722	726	727	rBV2	174	131	0.01%	0.001%
10	3.442	745	747	750	rBV2	128	68	0.00%	0.001%
11	3.461	750	753	758	rBV2	195	203	0.01%	0.002%
12	3.551	778	781	785	rBV2	244	179	0.01%	0.002%
13	3.722	826	834	839	rBV2	268	414	0.02%	0.004%
14	3.908	878	892	928	rBV3	105406	354684	15.09%	3.115%
15	4.349	1013	1029	1058	rBV	192116	473850	20.16%	4.162%
16	4.532	1085	1086	1087	rBV	267	95	0.00%	0.001%
17	4.609	1094	1110	1134	rBV3	36203	91425	3.89%	0.803%
18	4.908	1201	1203	1205	rBV	163	75	0.00%	0.001%
19	4.924	1206	1208	1209	rVB	186	53	0.00%	0.000%
20	5.047	1228	1246	1278	rBV2	477817	1216199	51.74%	10.682%
21	5.539	1398	1399	1400	rVB	126	24	0.00%	0.000%
22	5.555	1400	1404	1405	rBV2	139	100	0.00%	0.001%
23	5.616	1410	1423	1450	rBV	326965	658668	28.02%	5.785%
24	5.912	1500	1515	1551	rBV	1199955	2350820	100.00%	20.648%
25	6.069	1551	1564	1594	rVB	265746	543861	23.13%	4.777%
26	6.275	1626	1628	1633	rVB3	396	272	0.01%	0.002%
27	6.468	1685	1688	1692	rBV	206	147	0.01%	0.001%
28	6.503	1698	1699	1701	rBV	40	19	0.00%	0.000%
29	6.522	1701	1705	1707	rBV	190	160	0.01%	0.001%
30	6.567	1716	1719	1720	rBV	222	144	0.01%	0.001%
31	6.632	1736	1739	1740	rBV	104	57	0.00%	0.001%
32	6.686	1753	1756	1758	rBV2	275	185	0.01%	0.002%
33	6.715	1762	1765	1767	rVV	237	101	0.00%	0.001%
34	6.741	1772	1773	1774	rBV	178	45	0.00%	0.000%
35	6.796	1787	1790	1793	rBV	170	101	0.00%	0.001%
36	6.847	1803	1806	1811	rBV	153	177	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024918.D
 Acq On : 10 Mar 2022 16:08
 Operator : SY/MD
 Sample : N1855-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.876	1811	1815	1822	rVV2	248	333	0.01%	0.003%
38	6.985	1838	1849	1870	rBV	138943	250750	10.67%	2.202%
39	7.217	1916	1921	1925	rBV4	662	680	0.03%	0.006%
40	7.265	1934	1936	1938	rBV	176	65	0.00%	0.001%
41	7.313	1940	1951	1971	rBV	565672	983634	41.84%	8.640%
42	7.622	2037	2047	2071	rBV	92363	160057	6.81%	1.406%
43	7.780	2094	2096	2098	rBV2	203	113	0.00%	0.001%
44	7.809	2102	2105	2107	rBV	206	122	0.01%	0.001%
45	7.854	2112	2119	2125	rVV3	1247	1544	0.07%	0.014%
46	7.879	2125	2127	2130	rVB	251	132	0.01%	0.001%
47	7.937	2138	2145	2155	rVB3	486	958	0.04%	0.008%
48	8.088	2183	2192	2228	rBV	243594	476531	20.27%	4.186%
49	8.413	2289	2293	2294	rBV	234	157	0.01%	0.001%
50	8.445	2301	2303	2307	rVB2	255	131	0.01%	0.001%
51	8.519	2317	2326	2330	rBV2	410	517	0.02%	0.005%
52	8.577	2341	2344	2345	rBV	343	158	0.01%	0.001%
53	8.850	2417	2429	2461	rBV	511033	823328	35.02%	7.232%
54	9.072	2496	2498	2500	rBV	353	185	0.01%	0.002%
55	9.146	2516	2521	2523	rBV3	527	494	0.02%	0.004%
56	9.342	2579	2582	2584	rBV2	217	122	0.01%	0.001%
57	9.513	2632	2635	2638	rBV2	134	100	0.00%	0.001%
58	9.554	2643	2648	2650	rBV2	239	140	0.01%	0.001%
59	9.567	2650	2652	2654	rBV2	133	66	0.00%	0.001%
60	9.599	2659	2662	2665	rBV2	205	147	0.01%	0.001%
61	9.786	2716	2720	2726	rBV2	262	252	0.01%	0.002%
62	9.831	2731	2734	2738	rBV2	152	113	0.00%	0.001%
63	9.853	2739	2741	2743	rBV2	156	98	0.00%	0.001%
64	9.911	2756	2759	2765	rBV2	237	224	0.01%	0.002%
65	10.124	2818	2825	2834	rBV4	3344	4406	0.19%	0.039%
66	10.214	2841	2853	2875	rBV	316096	495776	21.09%	4.355%
67	10.352	2893	2896	2897	rBV	393	265	0.01%	0.002%
68	10.423	2915	2918	2923	rBV2	235	233	0.01%	0.002%
69	10.696	3000	3003	3006	rBV2	203	152	0.01%	0.001%
70	10.821	3038	3042	3045	rBV2	289	274	0.01%	0.002%
71	10.911	3064	3070	3080	rVB5	2229	3526	0.15%	0.031%
72	10.966	3084	3087	3089	rBV	199	121	0.01%	0.001%
73	10.985	3089	3093	3095	rBV2	314	218	0.01%	0.002%
74	11.056	3112	3115	3118	rBV2	281	226	0.01%	0.002%
75	11.149	3136	3144	3150	rVB3	1242	1829	0.08%	0.016%
76	11.246	3163	3174	3197	rBV	502517	761438	32.39%	6.688%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024918.D
 Acq On : 10 Mar 2022 16:08
 Operator : SY/MD
 Sample : N1855-18
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M

Title : VOC Analysis

77	11.474	3243	3245	3246	rBV	179	61	0.00%	0.001%
78	11.622	3279	3291	3311	rBV	511169	788767	33.55%	6.928%
79	11.763	3332	3335	3337	rBV2	241	150	0.01%	0.001%
80	11.779	3337	3340	3341	rBV2	568	342	0.01%	0.003%
81	11.837	3357	3358	3360	rBV	277	114	0.00%	0.001%
82	11.988	3402	3405	3406	rBV	154	98	0.00%	0.001%
83	12.947	3702	3703	3704	rBV	155	50	0.00%	0.000%




Sum of corrected areas: 11385196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024918.D
Acq On : 10 Mar 2022 16:08
Operator : SY/MD
Sample : N1855-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

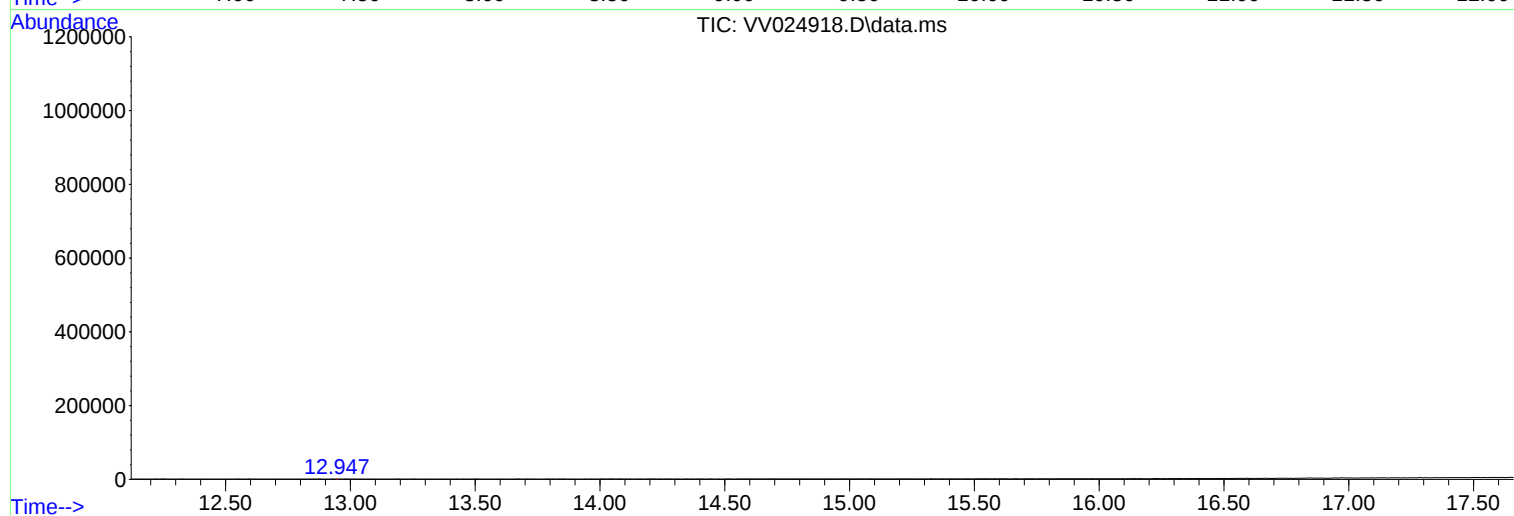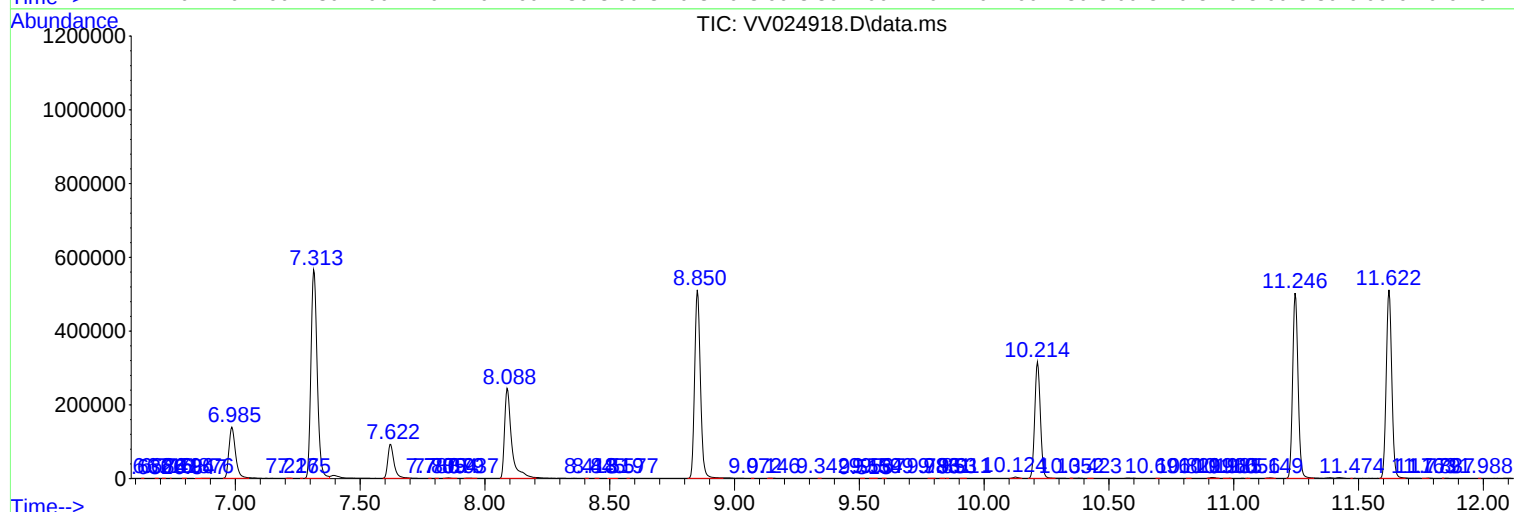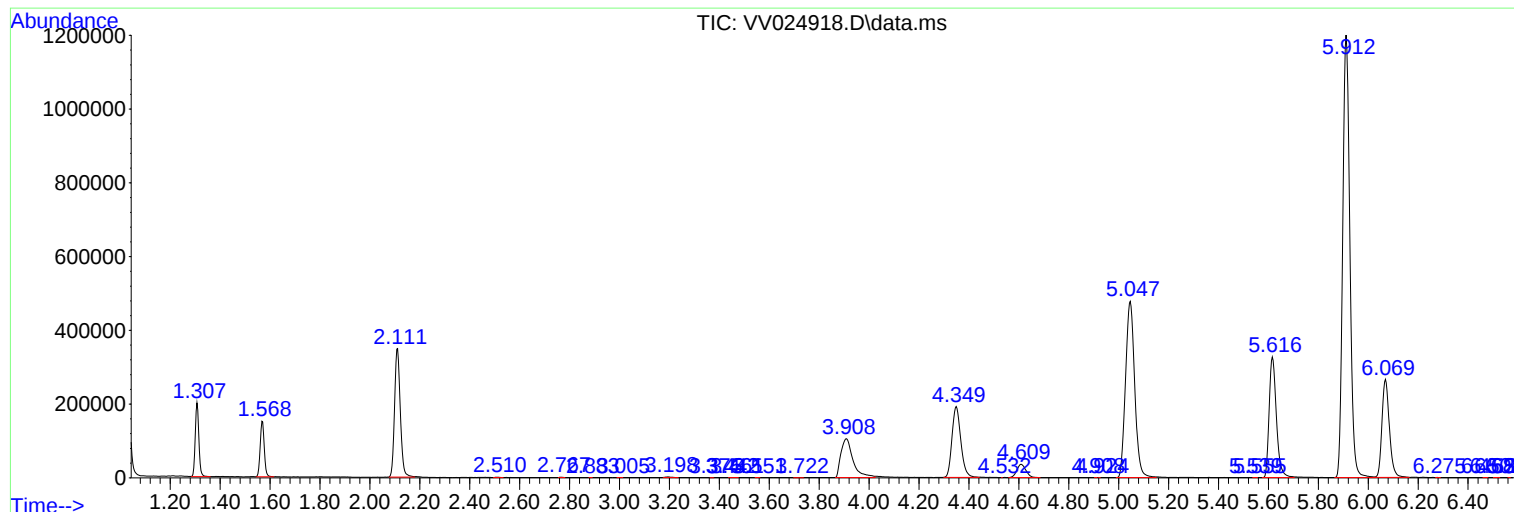

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024918.D
Acq On : 10 Mar 2022 16:08
Operator : SY/MD
Sample : N1855-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024918.D
Acq On : 10 Mar 2022 16:08
Operator : SY/MD
Sample : N1855-18
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------