

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024919.D
 Acq On : 10 Mar 2022 16:32
 Operator : SY/MD
 Sample : N1855-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024919.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	197774	200229	7.44%	1.694%
2	1.568	156	164	176	rBV	150913	168971	6.27%	1.429%
3	2.108	321	332	361	rBV2	319651	481757	17.89%	4.076%
4	2.368	410	413	417	rVB3	314	275	0.01%	0.002%
5	2.433	431	433	436	rBV3	493	308	0.01%	0.003%
6	2.764	526	536	554	rVB	11137	19151	0.71%	0.162%
7	2.925	582	586	588	rBV2	209	188	0.01%	0.002%
8	2.986	600	605	608	rBV2	260	292	0.01%	0.002%
9	3.130	647	650	655	rBV2	179	183	0.01%	0.002%
10	3.195	659	670	683	rBV2	2047	4160	0.15%	0.035%
11	3.616	791	801	805	rBV2	289	417	0.02%	0.004%
12	3.651	809	812	815	rVV	263	189	0.01%	0.002%
13	3.905	877	891	928	rBV3	115344	388550	14.43%	3.287%
14	4.281	1005	1008	1011	rBV3	367	251	0.01%	0.002%
15	4.349	1012	1029	1060	rBV	193823	484047	17.97%	4.095%
16	4.497	1073	1075	1076	rBV2	373	192	0.01%	0.002%
17	4.529	1082	1085	1089	rVB2	310	206	0.01%	0.002%
18	4.609	1089	1110	1131	rBV2	44688	113208	4.20%	0.958%
19	4.806	1165	1171	1174	rBV	219	274	0.01%	0.002%
20	4.876	1191	1193	1199	rVB2	305	180	0.01%	0.002%
21	4.931	1205	1210	1218	rBV2	291	478	0.02%	0.004%
22	5.047	1229	1246	1278	rBV2	479176	1219820	45.30%	10.319%
23	5.208	1293	1296	1300	rVB4	553	408	0.02%	0.003%
24	5.236	1303	1305	1310	rVB2	273	219	0.01%	0.002%
25	5.262	1311	1313	1318	rVB3	222	182	0.01%	0.002%
26	5.416	1357	1361	1367	rVB4	401	434	0.02%	0.004%
27	5.616	1411	1423	1448	rBV	331444	660744	24.54%	5.590%
28	5.857	1494	1498	1501	rBV2	235	183	0.01%	0.002%
29	5.912	1501	1515	1546	rBV	1388171	2693009	100.00%	22.782%
30	6.069	1551	1564	1590	rVB	262112	535212	19.87%	4.528%
31	6.217	1607	1610	1612	rVB4	353	198	0.01%	0.002%
32	6.256	1618	1622	1624	rVB3	369	259	0.01%	0.002%
33	6.304	1632	1637	1639	rBV	253	222	0.01%	0.002%
34	6.339	1645	1648	1655	rVB2	326	359	0.01%	0.003%
35	6.526	1700	1706	1708	rBV	212	202	0.01%	0.002%
36	6.593	1723	1727	1730	rBV2	220	217	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031022\
 Data File : VW024919.D
 Acq On : 10 Mar 2022 16:32
 Operator : SY/MD
 Sample : N1855-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.986	1838	1849	1876	rBV	141564	255661	9.49%	2.163%
38	7.140	1893	1897	1900	rBV2	275	303	0.01%	0.003%
39	7.195	1910	1914	1915	rBV2	366	224	0.01%	0.002%
40	7.314	1939	1951	1970	rBV	575736	990726	36.79%	8.381%
41	7.622	2035	2047	2078	rBV	89948	159870	5.94%	1.352%
42	7.850	2112	2118	2127	rVB3	1179	1534	0.06%	0.013%
43	7.892	2127	2131	2133	rVB2	328	189	0.01%	0.002%
44	7.931	2139	2143	2145	rBV2	484	362	0.01%	0.003%
45	8.088	2182	2192	2231	rBV	263779	504542	18.74%	4.268%
46	8.481	2311	2314	2320	rBV2	352	336	0.01%	0.003%
47	8.567	2335	2341	2344	rBV2	259	278	0.01%	0.002%
48	8.619	2353	2357	2363	rBV3	422	443	0.02%	0.004%
49	8.725	2383	2390	2399	rVB2	253	431	0.02%	0.004%
50	8.767	2399	2403	2409	rVB2	159	197	0.01%	0.002%
51	8.799	2409	2413	2417	rBV	256	264	0.01%	0.002%
52	8.850	2417	2429	2456	rBV	509704	826619	30.69%	6.993%
53	9.027	2481	2484	2489	rVB2	416	260	0.01%	0.002%
54	9.146	2517	2521	2522	rBV2	377	283	0.01%	0.002%
55	9.172	2526	2529	2532	rVV3	335	193	0.01%	0.002%
56	9.259	2549	2556	2560	rBV2	218	250	0.01%	0.002%
57	9.304	2566	2570	2573	rBV2	238	225	0.01%	0.002%
58	9.352	2579	2585	2591	rBV2	310	402	0.01%	0.003%
59	9.625	2665	2670	2678	rVB2	250	355	0.01%	0.003%
60	9.664	2678	2682	2685	rBV	208	189	0.01%	0.002%
61	9.699	2689	2693	2696	rBV	233	217	0.01%	0.002%
62	9.908	2754	2758	2761	rVV	277	187	0.01%	0.002%
63	9.953	2769	2772	2778	rVB	229	180	0.01%	0.002%
64	9.982	2778	2781	2784	rBV	212	195	0.01%	0.002%
65	10.047	2798	2801	2806	rVB	277	204	0.01%	0.002%
66	10.127	2816	2826	2834	rBV2	3064	4021	0.15%	0.034%
67	10.214	2840	2853	2876	rBV	331310	515071	19.13%	4.357%
68	10.371	2900	2902	2905	rVV2	360	228	0.01%	0.002%
69	10.387	2905	2907	2910	rVB	522	291	0.01%	0.002%
70	10.580	2961	2967	2969	rBV3	778	860	0.03%	0.007%
71	10.776	3025	3028	3032	rVB2	375	276	0.01%	0.002%
72	10.911	3066	3070	3072	rBV2	1576	1412	0.05%	0.012%
73	10.976	3087	3090	3093	rBV	234	189	0.01%	0.002%
74	11.030	3103	3107	3112	rVB3	429	453	0.02%	0.004%
75	11.063	3112	3117	3119	rBV2	246	221	0.01%	0.002%
76	11.140	3138	3141	3142	rBV2	743	420	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024919.D
 Acq On : 10 Mar 2022 16:32
 Operator : SY/MD
 Sample : N1855-19
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.246	3163	3174	3195	rBV	508780	773491	28.72%	6.544%
78	11.387	3214	3218	3223	rVB5	1114	1051	0.04%	0.009%
79	11.423	3223	3229	3230	rBV3	1323	1021	0.04%	0.009%
80	11.535	3260	3264	3266	rBV	254	223	0.01%	0.002%
81	11.622	3279	3291	3311	rVV	517624	794755	29.51%	6.723%
82	11.693	3311	3313	3320	rVB4	1186	1066	0.04%	0.009%
83	11.780	3336	3340	3350	rVB5	712	900	0.03%	0.008%
84	11.831	3350	3356	3357	rBV2	284	192	0.01%	0.002%
85	12.088	3432	3436	3443	rBV3	446	546	0.02%	0.005%
86	12.587	3587	3591	3592	rBV	340	190	0.01%	0.002%
87	12.690	3619	3623	3626	rBV	295	251	0.01%	0.002%
88	12.776	3644	3650	3653	rBV2	248	272	0.01%	0.002%
89	13.181	3772	3776	3779	rBV2	225	222	0.01%	0.002%
90	13.284	3805	3808	3812	rVB	283	206	0.01%	0.002%
91	13.516	3877	3880	3883	rBV	327	241	0.01%	0.002%
92	13.532	3883	3885	3889	rVB2	299	199	0.01%	0.002%
93	13.577	3895	3899	3905	rVB	299	281	0.01%	0.002%
94	13.876	3989	3992	3995	rVB	345	208	0.01%	0.002%
95	14.021	4034	4037	4040	rBV2	330	253	0.01%	0.002%
96	14.079	4053	4055	4059	rBV2	237	176	0.01%	0.001%
97	14.194	4085	4091	4095	rVB2	295	340	0.01%	0.003%
98	14.220	4095	4099	4104	rBV2	347	391	0.01%	0.003%
99	14.712	4249	4252	4254	rBV3	401	260	0.01%	0.002%
100	15.599	4526	4528	4532	rBV	370	229	0.01%	0.002%




Sum of corrected areas: 11820699

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024919.D
Acq On : 10 Mar 2022 16:32
Operator : SY/MD
Sample : N1855-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

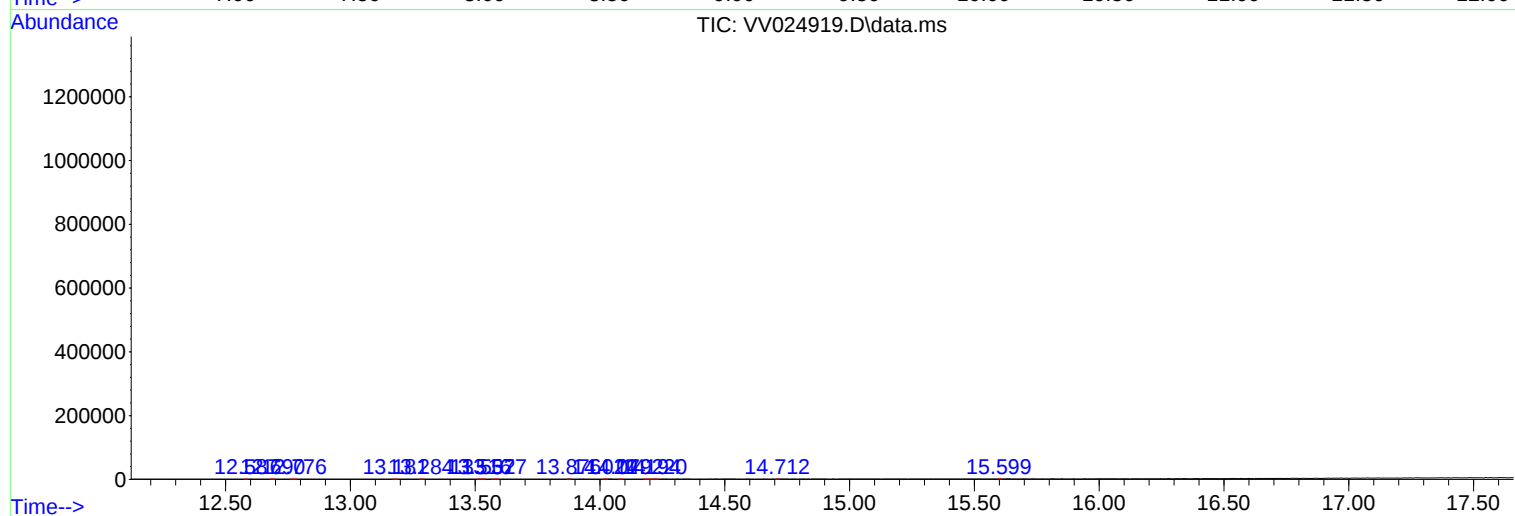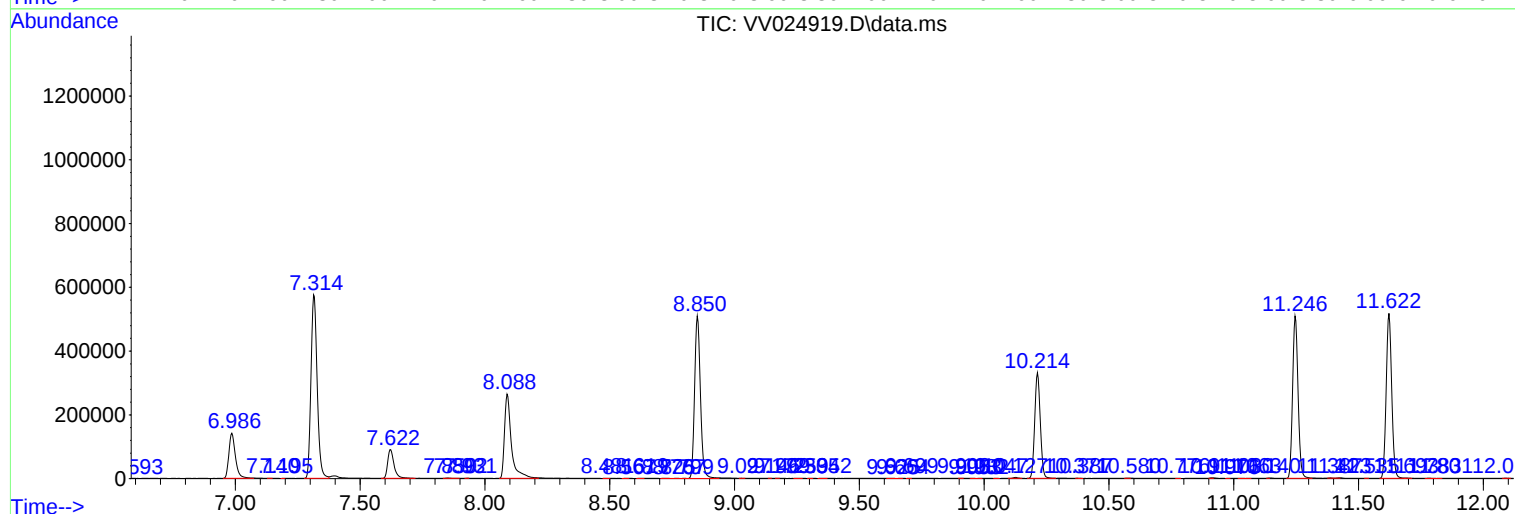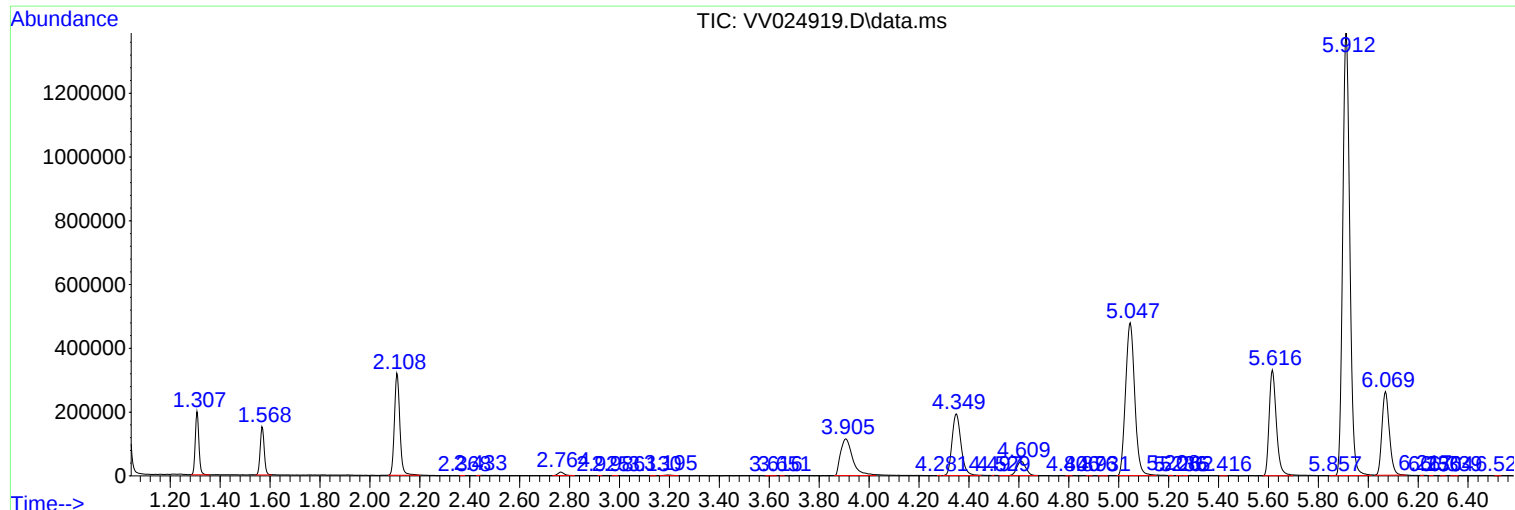

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024919.D
Acq On : 10 Mar 2022 16:32
Operator : SY/MD
Sample : N1855-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024919.D
Acq On : 10 Mar 2022 16:32
Operator : SY/MD
Sample : N1855-19
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D62

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------