

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024924.D
 Acq On : 10 Mar 2022 18:30
 Operator : SY/MD
 Sample : N1775-24ME
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSC7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.503	447	455	463	rBV5	1989	3177	0.42%	0.144%
2	2.699	513	516	518	rBV	247	156	0.02%	0.007%
3	2.815	549	552	557	rBV2	232	268	0.04%	0.012%
4	2.928	584	587	590	rBV2	152	126	0.02%	0.006%
5	3.021	610	616	618	rBV3	1301	1452	0.19%	0.066%
6	3.230	678	681	682	rBV	152	99	0.01%	0.004%
7	3.252	686	688	690	rBV	151	74	0.01%	0.003%
8	3.619	794	802	807	rBV2	226	334	0.04%	0.015%
9	3.677	815	820	825	rBV2	209	287	0.04%	0.013%
10	3.876	878	882	883	rBV	300	200	0.03%	0.009%
11	4.474	1065	1068	1070	rBV	242	194	0.03%	0.009%
12	4.564	1094	1096	1098	rBV	169	72	0.01%	0.003%
13	4.622	1110	1114	1119	rBV	252	277	0.04%	0.013%
14	4.664	1124	1127	1131	rVV4	253	221	0.03%	0.010%
15	4.789	1164	1166	1170	rVB	156	90	0.01%	0.004%
16	4.854	1183	1186	1189	rBV2	172	120	0.02%	0.005%
17	4.892	1196	1198	1201	rBV2	468	332	0.04%	0.015%
18	5.053	1234	1248	1268	rBV4	13431	32586	4.34%	1.473%
19	5.172	1283	1285	1288	rBV	164	83	0.01%	0.004%
20	5.188	1288	1290	1292	rBV	169	56	0.01%	0.003%
21	5.249	1307	1309	1313	rVB	161	103	0.01%	0.005%
22	5.275	1313	1317	1319	rBV	95	80	0.01%	0.004%
23	5.339	1328	1337	1353	rBV4	4197	12157	1.62%	0.549%
24	5.612	1410	1422	1452	rBV	284331	597399	79.50%	27.000%
25	6.075	1558	1566	1579	rVB5	5606	10876	1.45%	0.492%
26	6.191	1600	1602	1604	rVB2	130	56	0.01%	0.003%
27	6.217	1604	1610	1615	rBV2	261	364	0.05%	0.016%
28	6.391	1662	1664	1667	rBV	175	124	0.02%	0.006%
29	6.439	1675	1679	1684	rVB2	250	226	0.03%	0.010%
30	6.497	1694	1697	1700	rVB	227	148	0.02%	0.007%
31	6.564	1716	1718	1723	rBV2	173	116	0.02%	0.005%
32	6.648	1736	1744	1754	rBV5	1536	3003	0.40%	0.136%
33	6.757	1776	1778	1782	rVB2	414	216	0.03%	0.010%
34	6.915	1822	1827	1829	rBV2	317	256	0.03%	0.012%
35	6.973	1842	1845	1846	rBV	182	102	0.01%	0.005%
36	7.001	1849	1854	1865	rVB5	2089	4263	0.57%	0.193%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024924.D
 Acq On : 10 Mar 2022 18:30
 Operator : SY/MD
 Sample : N1775-24ME
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBSC7ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	7.169	1903	1906	1909	rBV2	177	126	0.02%	0.006%
38	7.249	1927	1931	1936	rVB2	285	250	0.03%	0.011%
39	7.278	1936	1940	1941	rBV	197	142	0.02%	0.006%
40	7.323	1945	1954	1973	rVV2	12618	25254	3.36%	1.141%
41	7.612	2041	2044	2046	rBV	198	140	0.02%	0.006%
42	7.645	2046	2054	2058	rBV5	1424	1997	0.27%	0.090%
43	7.802	2096	2103	2110	rBV4	595	878	0.12%	0.040%
44	7.834	2110	2113	2115	rBV2	320	175	0.02%	0.008%
45	7.873	2122	2125	2128	rBV2	238	145	0.02%	0.007%
46	7.899	2128	2133	2134	rBV	191	147	0.02%	0.007%
47	8.140	2200	2208	2210	rBV2	1350	1607	0.21%	0.073%
48	8.320	2261	2264	2267	rVB	225	124	0.02%	0.006%
49	8.342	2267	2271	2273	rBV2	251	194	0.03%	0.009%
50	8.419	2291	2295	2296	rBV	157	102	0.01%	0.005%
51	8.509	2321	2323	2326	rBV2	133	91	0.01%	0.004%
52	8.709	2382	2385	2388	rBV	145	85	0.01%	0.004%
53	8.728	2388	2391	2397	rBV2	209	220	0.03%	0.010%
54	8.857	2418	2431	2462	rBV	380137	751435	100.00%	33.962%
55	9.133	2514	2517	2519	rVB2	255	160	0.02%	0.007%
56	9.149	2519	2522	2529	rVB2	332	312	0.04%	0.014%
57	9.181	2529	2532	2535	rBV2	224	158	0.02%	0.007%
58	9.217	2539	2543	2548	rBV2	156	175	0.02%	0.008%
59	9.345	2579	2583	2586	rBV2	228	228	0.03%	0.010%
60	9.516	2625	2636	2638	rBV2	270	526	0.07%	0.024%
61	9.786	2716	2720	2726	rBV2	195	275	0.04%	0.012%
62	9.998	2783	2786	2788	rBV2	157	103	0.01%	0.005%
63	10.088	2811	2814	2818	rVB2	230	153	0.02%	0.007%
64	10.226	2847	2857	2869	rBV3	7123	13083	1.74%	0.591%
65	10.548	2954	2957	2959	rBV3	328	227	0.03%	0.010%
66	10.824	3040	3043	3046	rBV2	324	245	0.03%	0.011%
67	10.895	3062	3065	3068	rBV	255	189	0.03%	0.009%
68	11.088	3122	3125	3127	rVB	174	82	0.01%	0.004%
69	11.252	3165	3176	3204	rBV	451344	709794	94.46%	32.080%
70	11.423	3226	3229	3231	rBV	349	240	0.03%	0.011%
71	11.580	3275	3278	3280	rBV	184	123	0.02%	0.006%
72	11.632	3285	3294	3306	rVV	20939	32283	4.30%	1.459%
73	11.718	3318	3321	3324	rBV	198	126	0.02%	0.006%
74	12.316	3505	3507	3508	rBV	294	68	0.01%	0.003%
75	12.352	3513	3518	3520	rBV4	861	762	0.10%	0.034%
76	12.892	3683	3686	3688	rBV	253	186	0.02%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024924.D
Acq On : 10 Mar 2022 18:30
Operator : SY/MD
Sample : N1775-24ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSC7ME

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Title : VOC Analysis

77	13.686	3930	3933	3938	rBV	454	292	0.04%	0.013%
----	--------	------	------	------	-----	-----	-----	-------	--------




Sum of corrected areas: 2212595

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024924.D
Acq On : 10 Mar 2022 18:30
Operator : SY/MD
Sample : N1775-24ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSC7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

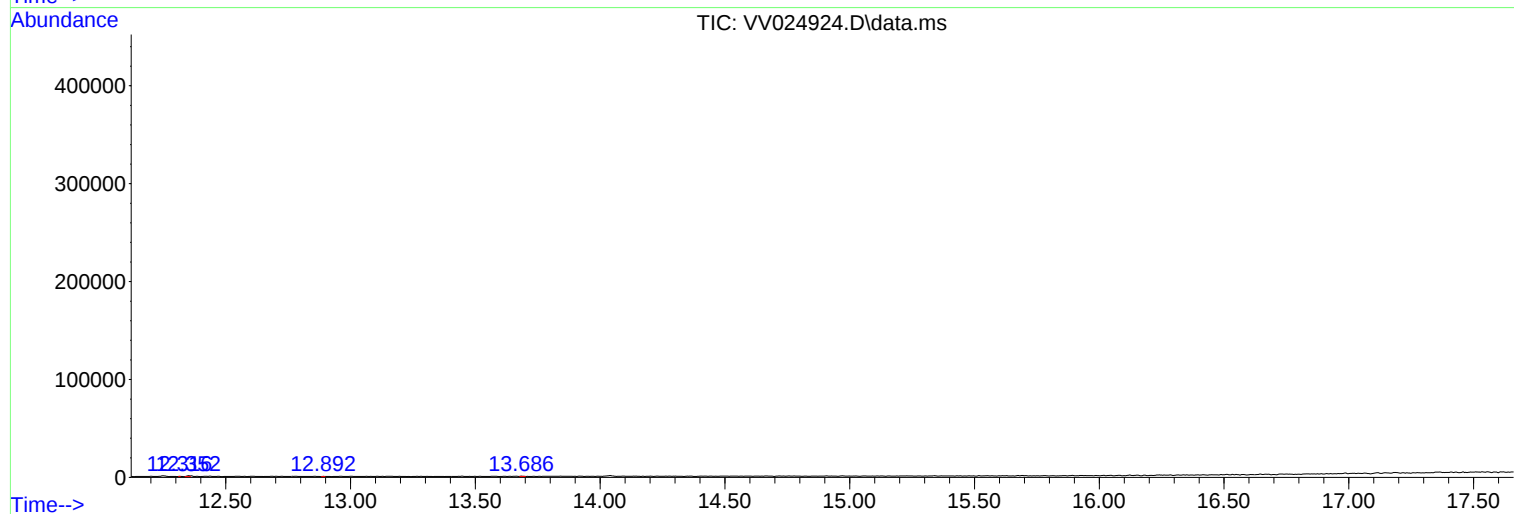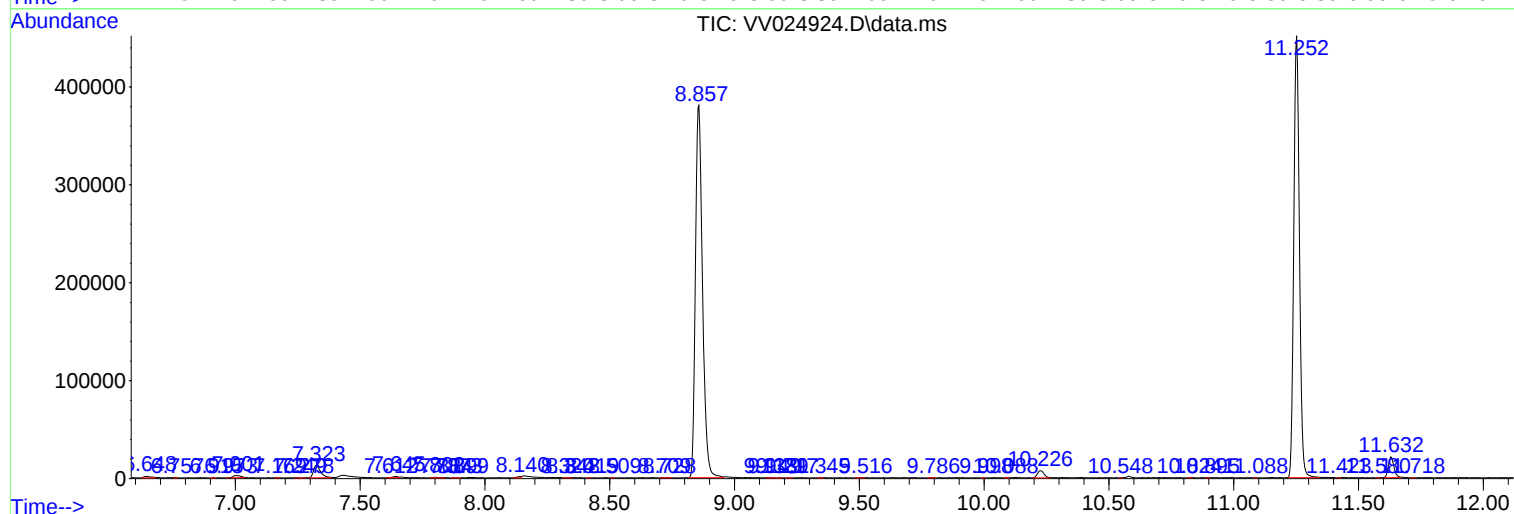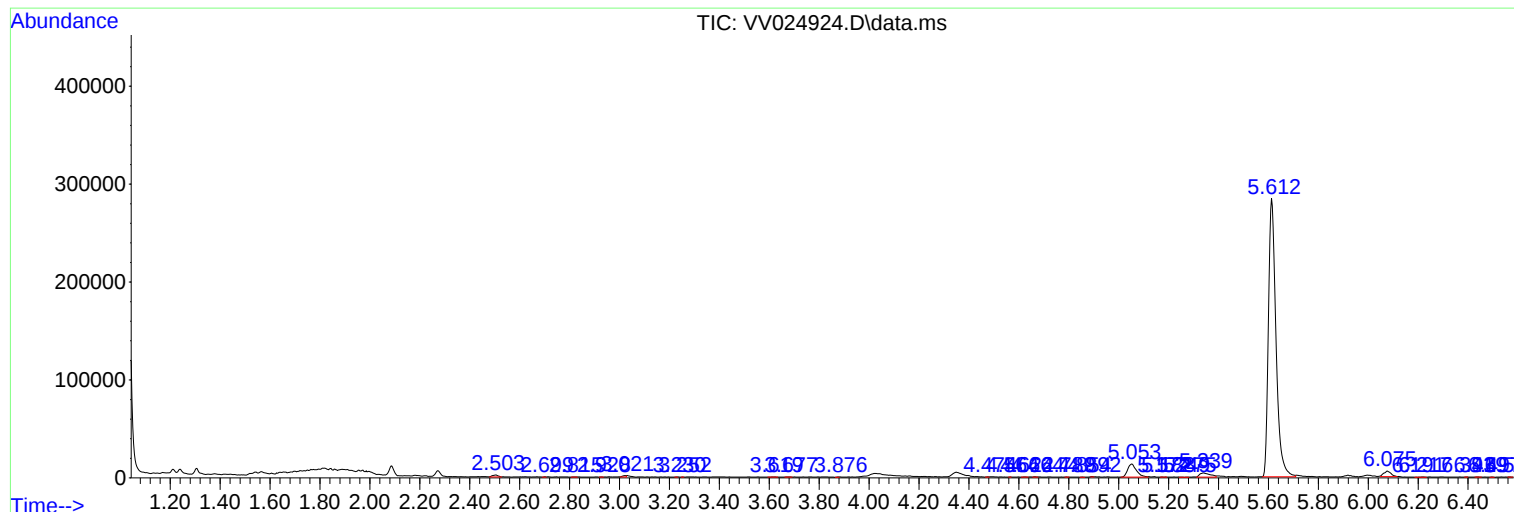

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024924.D
Acq On : 10 Mar 2022 18:30
Operator : SY/MD
Sample : N1775-24ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSC7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024924.D
Acq On : 10 Mar 2022 18:30
Operator : SY/MD
Sample : N1775-24ME
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBSC7ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------