

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024925.D
 Acq On : 10 Mar 2022 18:54
 Operator : SY/MD
 Sample : N1879-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024925.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	195091	195187	15.84%	2.200%
2	1.568	157	164	183	rVB	151497	167733	13.61%	1.891%
3	2.108	321	332	362	rVB	299408	440789	35.78%	4.969%
4	2.539	462	466	471	rBV	267	245	0.02%	0.003%
5	2.564	471	474	478	rVB3	359	257	0.02%	0.003%
6	2.590	478	482	486	rBV2	224	248	0.02%	0.003%
7	2.773	532	539	549	rVB4	609	948	0.08%	0.011%
8	2.815	549	552	558	rBV2	274	247	0.02%	0.003%
9	2.899	575	578	580	rBV	219	134	0.01%	0.002%
10	3.117	643	646	647	rBV2	162	99	0.01%	0.001%
11	3.175	661	664	666	rBV	174	111	0.01%	0.001%
12	3.359	718	721	723	rBV	186	119	0.01%	0.001%
13	3.503	760	766	769	rBV2	233	269	0.02%	0.003%
14	3.892	877	887	927	rBV	71318	239009	19.40%	2.694%
15	4.349	1013	1029	1057	rBV2	194114	487038	39.53%	5.490%
16	4.596	1102	1106	1107	rBV	295	213	0.02%	0.002%
17	4.619	1111	1113	1118	rVB2	398	277	0.02%	0.003%
18	4.680	1130	1132	1136	rBV2	169	116	0.01%	0.001%
19	4.825	1174	1177	1180	rBV2	270	223	0.02%	0.003%
20	4.886	1193	1196	1201	rBV2	246	155	0.01%	0.002%
21	4.912	1201	1204	1206	rVB	245	107	0.01%	0.001%
22	4.931	1206	1210	1212	rBV2	168	121	0.01%	0.001%
23	4.950	1212	1216	1221	rVB2	289	286	0.02%	0.003%
24	5.047	1228	1246	1281	rBV2	479931	1232022	100.00%	13.888%
25	5.362	1342	1344	1347	rBV	190	69	0.01%	0.001%
26	5.384	1349	1351	1353	rVB	336	127	0.01%	0.001%
27	5.407	1353	1358	1363	rBV3	413	515	0.04%	0.006%
28	5.436	1364	1367	1370	rVB2	324	197	0.02%	0.002%
29	5.548	1397	1402	1403	rBV2	139	110	0.01%	0.001%
30	5.558	1403	1405	1410	rVV	204	146	0.01%	0.002%
31	5.616	1411	1423	1463	rBV	321870	655173	53.18%	7.385%
32	5.908	1503	1514	1533	rBV5	25633	57791	4.69%	0.651%
33	6.014	1545	1547	1550	rVB	230	100	0.01%	0.001%
34	6.069	1550	1564	1590	rBV	269678	549691	44.62%	6.196%
35	6.326	1640	1644	1645	rBV	122	93	0.01%	0.001%
36	6.371	1655	1658	1661	rBV	127	100	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024925.D
 Acq On : 10 Mar 2022 18:54
 Operator : SY/MD
 Sample : N1879-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.465	1685	1687	1688	rBV	75	33	0.00%	0.000%
38	6.651	1743	1745	1749	rBV	283	204	0.02%	0.002%
39	6.728	1765	1769	1773	rBV	407	313	0.03%	0.004%
40	6.847	1803	1806	1808	rBV	127	84	0.01%	0.001%
41	6.947	1834	1837	1838	rBV	177	99	0.01%	0.001%
42	6.985	1838	1849	1872	rVV	137582	249941	20.29%	2.817%
43	7.313	1940	1951	1971	rBV	571458	988841	80.26%	11.146%
44	7.622	2036	2047	2065	rBV	90708	158266	12.85%	1.784%
45	7.812	2102	2106	2111	rBV2	385	358	0.03%	0.004%
46	7.834	2111	2113	2115	rBV	181	101	0.01%	0.001%
47	7.886	2126	2129	2133	rBV2	127	107	0.01%	0.001%
48	7.940	2139	2146	2155	rBV2	655	956	0.08%	0.011%
49	8.030	2172	2174	2177	rVB	149	73	0.01%	0.001%
50	8.088	2182	2192	2227	rBV	263307	514025	41.72%	5.794%
51	8.567	2334	2341	2343	rBV	220	289	0.02%	0.003%
52	8.616	2350	2356	2358	rBV	352	382	0.03%	0.004%
53	8.664	2367	2371	2373	rBV2	296	203	0.02%	0.002%
54	8.680	2373	2376	2379	rVB	241	136	0.01%	0.002%
55	8.747	2393	2397	2399	rBV	260	199	0.02%	0.002%
56	8.850	2417	2429	2460	rBV	507218	820358	66.59%	9.247%
57	9.046	2488	2490	2498	rVB3	385	309	0.03%	0.003%
58	9.153	2517	2523	2532	rBV2	533	906	0.07%	0.010%
59	9.227	2543	2546	2549	rVB	172	102	0.01%	0.001%
60	9.252	2549	2554	2560	rBV2	230	328	0.03%	0.004%
61	9.497	2626	2630	2632	rBV	256	190	0.02%	0.002%
62	9.600	2660	2662	2668	rBV	144	119	0.01%	0.001%
63	9.661	2677	2681	2683	rBV2	407	314	0.03%	0.004%
64	9.751	2706	2709	2712	rBV	201	114	0.01%	0.001%
65	9.854	2739	2741	2743	rBV2	80	34	0.00%	0.000%
66	9.870	2743	2746	2748	rBV	125	74	0.01%	0.001%
67	10.098	2814	2817	2818	rBV	186	101	0.01%	0.001%
68	10.124	2818	2825	2835	rVB2	3610	5238	0.43%	0.059%
69	10.214	2841	2853	2875	rBV	330144	521026	42.29%	5.873%
70	10.471	2930	2933	2937	rBV	244	210	0.02%	0.002%
71	10.709	3001	3007	3010	rBV2	339	359	0.03%	0.004%
72	10.886	3059	3062	3064	rBV	182	89	0.01%	0.001%
73	10.918	3064	3072	3081	rVV5	2129	3377	0.27%	0.038%
74	11.008	3094	3100	3103	rBV	332	343	0.03%	0.004%
75	11.030	3103	3107	3109	rBV2	354	301	0.02%	0.003%
76	11.143	3136	3142	3151	rBV4	1042	1654	0.13%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024925.D
Acq On : 10 Mar 2022 18:54
Operator : SY/MD
Sample : N1879-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Title : VOC Analysis

77	11.246	3162	3174	3201	rBV	491574	764463	62.05%	8.617%
78	11.567	3270	3274	3276	rBV2	329	267	0.02%	0.003%
79	11.622	3279	3291	3309	rBV	518088	806015	65.42%	9.086%
80	11.947	3389	3392	3393	rBV2	184	113	0.01%	0.001%
81	12.046	3419	3423	3428	rBV2	273	293	0.02%	0.003%




Sum of corrected areas: 8871372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024925.D
Acq On : 10 Mar 2022 18:54
Operator : SY/MD
Sample : N1879-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

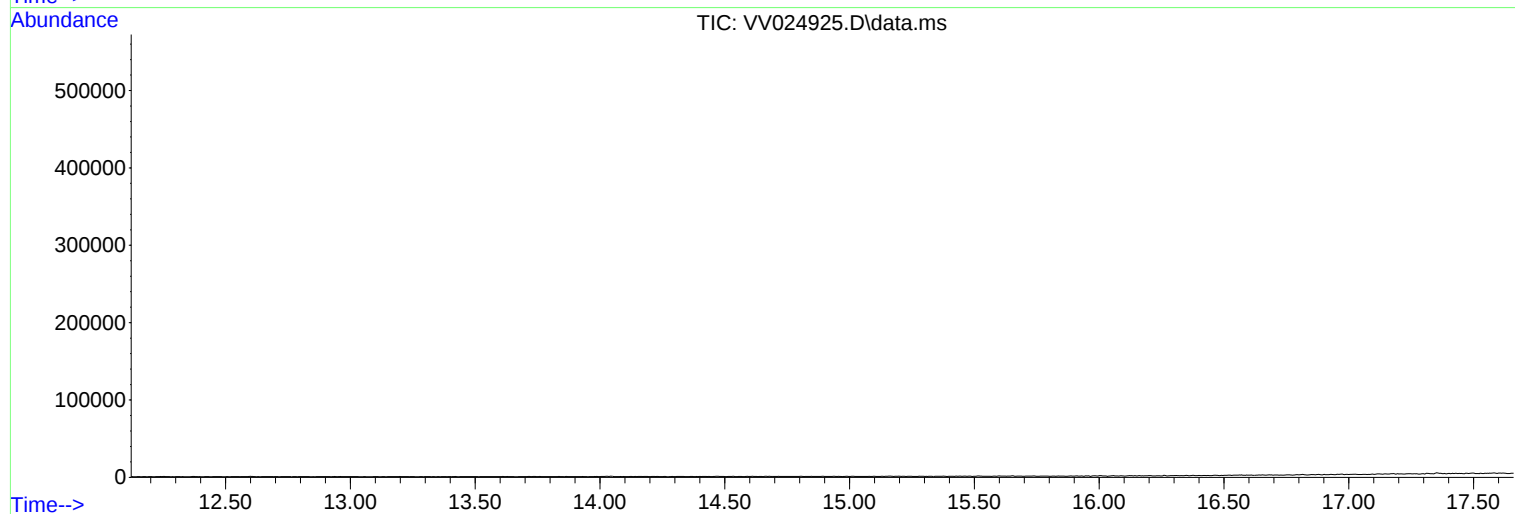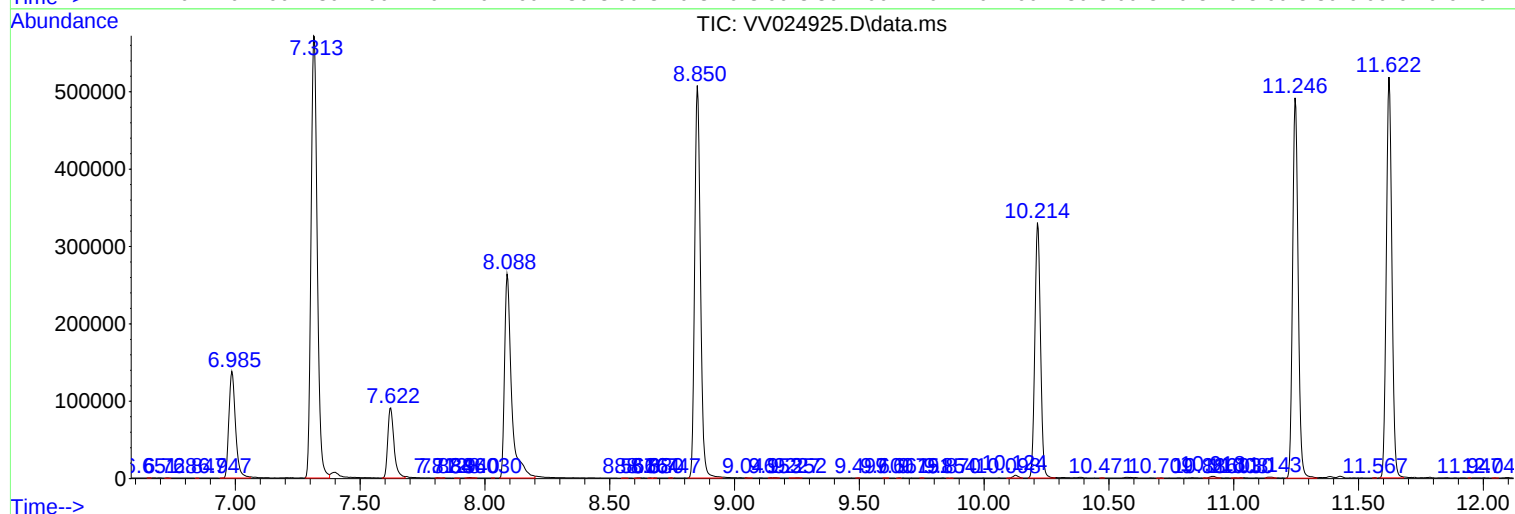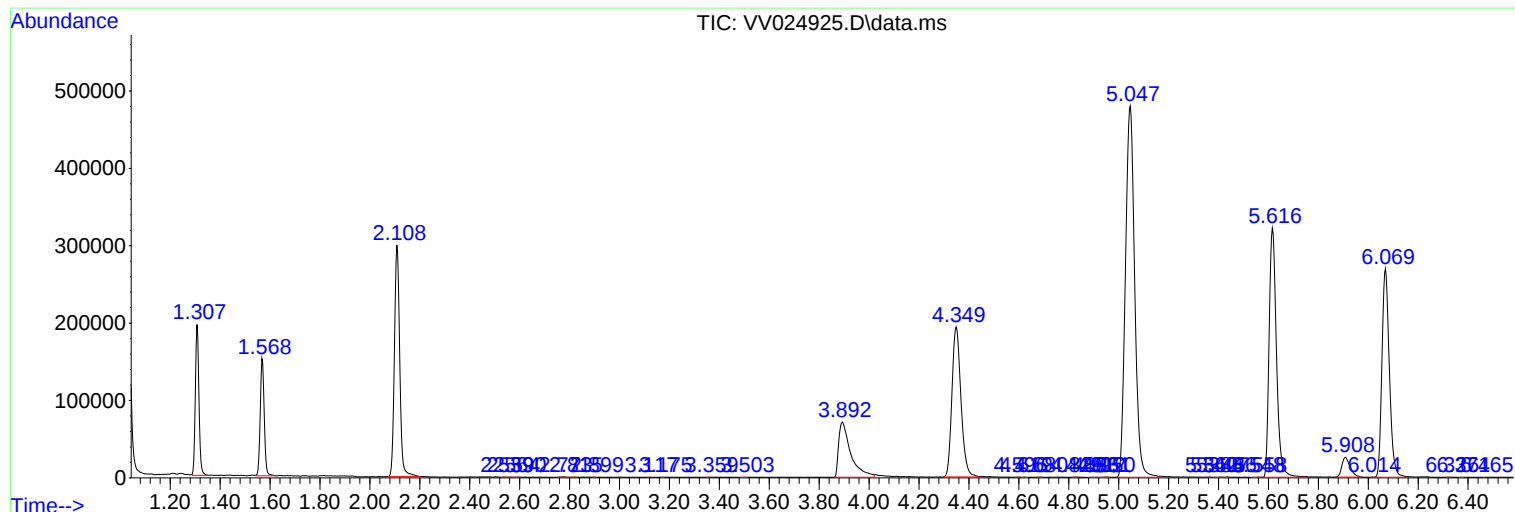

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024925.D
Acq On : 10 Mar 2022 18:54
Operator : SY/MD
Sample : N1879-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.908	4.41 ug/L	57791	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	43
2			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	38
3			Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	32
4			4-Chloro-3-fluoropyridine	131	C5H3ClFN	002546-56-7	25
5			2-Chloro-5-methylthiazole	133	C4H4ClNS	033342-65-3	25

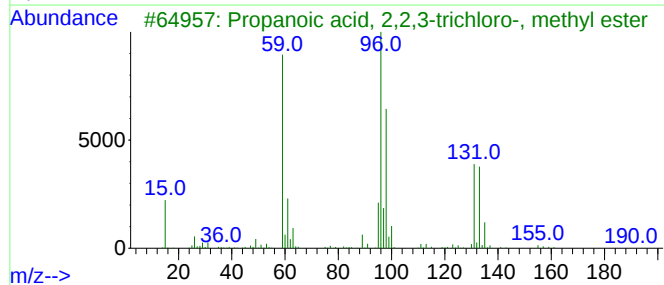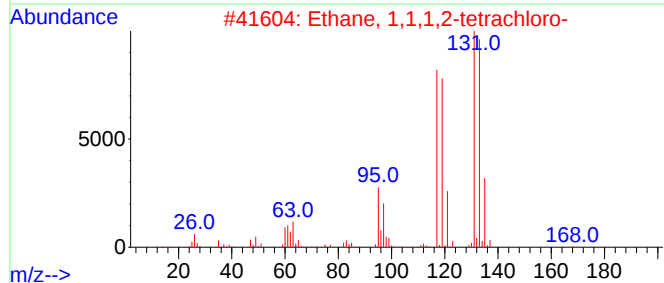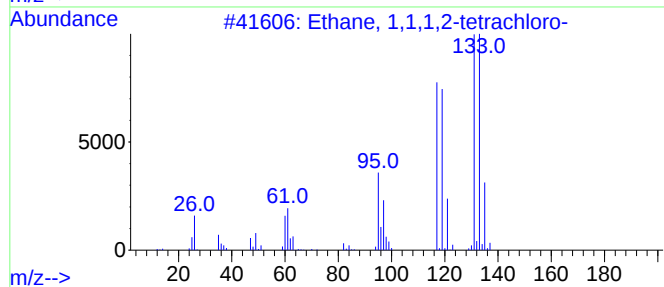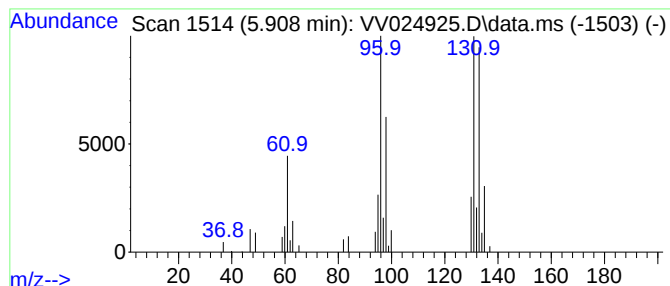

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024925.D
Acq On : 10 Mar 2022 18:54
Operator : SY/MD
Sample : N1879-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	5.908	4.4	ug/L	57791	1	5.616	655173	50.0