

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024934.D
 Acq On : 10 Mar 2022 23:18
 Operator : SY/MD
 Sample : N1879-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	168761	170754	15.26%	2.083%
2	1.568	157	164	176	rVB	132923	149472	13.35%	1.823%
3	2.108	321	332	366	rVB	268273	396492	35.42%	4.836%
4	2.336	398	403	406	rBV2	406	404	0.04%	0.005%
5	2.423	427	430	431	rBV2	305	204	0.02%	0.002%
6	2.577	475	478	481	rVB2	456	265	0.02%	0.003%
7	2.616	481	490	494	rBV3	1454	2134	0.19%	0.026%
8	2.818	547	553	558	rBV2	311	403	0.04%	0.005%
9	3.053	621	626	630	rBV	193	248	0.02%	0.003%
10	3.076	630	633	638	rVB2	283	212	0.02%	0.003%
11	3.105	638	642	649	rVB2	242	222	0.02%	0.003%
12	3.143	649	654	657	rBV2	204	212	0.02%	0.003%
13	3.227	676	680	684	rVB2	226	214	0.02%	0.003%
14	3.249	684	687	691	rBV	246	223	0.02%	0.003%
15	3.507	764	767	772	rBV	243	191	0.02%	0.002%
16	3.593	791	794	798	rVV2	252	209	0.02%	0.003%
17	3.632	803	806	813	rVB2	240	308	0.03%	0.004%
18	3.687	819	823	829	rVB2	244	246	0.02%	0.003%
19	3.896	877	888	927	rBV	69197	247487	22.11%	3.018%
20	4.349	1012	1029	1059	rBV	178451	442511	39.54%	5.397%
21	4.542	1087	1089	1093	rBV3	359	257	0.02%	0.003%
22	4.693	1130	1136	1138	rBV2	181	173	0.02%	0.002%
23	4.822	1172	1176	1180	rVV2	205	177	0.02%	0.002%
24	4.937	1210	1212	1216	rVB	293	208	0.02%	0.003%
25	4.973	1216	1223	1227	rBV2	281	398	0.04%	0.005%
26	5.047	1228	1246	1280	rBV2	438329	1119280	100.00%	13.651%
27	5.297	1321	1324	1327	rBV2	290	190	0.02%	0.002%
28	5.375	1346	1348	1352	rVB	227	176	0.02%	0.002%
29	5.410	1352	1359	1362	rBV4	401	390	0.03%	0.005%
30	5.616	1410	1423	1452	rBV	302397	604421	54.00%	7.372%
31	5.915	1497	1516	1538	rBV4	58538	133871	11.96%	1.633%
32	6.014	1543	1547	1551	rBV2	330	291	0.03%	0.004%
33	6.069	1551	1564	1596	rBV	245628	497149	44.42%	6.063%
34	6.220	1606	1611	1612	rBV5	586	482	0.04%	0.006%
35	6.278	1626	1629	1634	rVB2	268	306	0.03%	0.004%
36	6.301	1634	1636	1638	rBV	323	190	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024934.D
 Acq On : 10 Mar 2022 23:18
 Operator : SY/MD
 Sample : N1879-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.346	1644	1650	1653	rBV2	303	341	0.03%	0.004%
38	6.477	1685	1691	1694	rBV	278	250	0.02%	0.003%
39	6.497	1694	1697	1704	rVB2	236	246	0.02%	0.003%
40	6.651	1741	1745	1748	rVV2	208	180	0.02%	0.002%
41	6.728	1766	1769	1776	rBV2	342	240	0.02%	0.003%
42	6.985	1838	1849	1878	rBV	127530	229210	20.48%	2.795%
43	7.211	1916	1919	1924	rVB2	269	235	0.02%	0.003%
44	7.313	1939	1951	1970	rBV	519888	889557	79.48%	10.849%
45	7.571	2028	2031	2037	rVB3	371	313	0.03%	0.004%
46	7.622	2037	2047	2070	rBV	84212	145743	13.02%	1.777%
47	7.728	2078	2080	2082	rVB2	393	181	0.02%	0.002%
48	7.805	2100	2104	2109	rVB3	353	289	0.03%	0.004%
49	7.921	2137	2140	2142	rBV	339	275	0.02%	0.003%
50	7.944	2143	2147	2153	rVB2	551	638	0.06%	0.008%
51	8.005	2162	2166	2173	rBV2	249	308	0.03%	0.004%
52	8.088	2179	2192	2232	rBV	242173	476696	42.59%	5.814%
53	8.281	2250	2252	2254	rVB	526	175	0.02%	0.002%
54	8.297	2254	2257	2262	rBV2	321	305	0.03%	0.004%
55	8.368	2277	2279	2283	rVB2	550	239	0.02%	0.003%
56	8.407	2288	2291	2297	rVB2	413	393	0.04%	0.005%
57	8.625	2352	2359	2361	rBV2	218	260	0.02%	0.003%
58	8.709	2382	2385	2394	rVB2	208	320	0.03%	0.004%
59	8.850	2417	2429	2449	rBV	466880	749007	66.92%	9.135%
60	9.030	2481	2485	2486	rBV2	415	248	0.02%	0.003%
61	9.075	2494	2499	2502	rBV	266	285	0.03%	0.003%
62	9.146	2514	2521	2523	rBV4	400	399	0.04%	0.005%
63	9.837	2731	2736	2740	rBV2	183	216	0.02%	0.003%
64	9.902	2752	2756	2762	rBV2	200	194	0.02%	0.002%
65	10.124	2817	2825	2836	rBV4	2728	4190	0.37%	0.051%
66	10.214	2841	2853	2867	rBV	316601	489761	43.76%	5.973%
67	10.374	2899	2903	2905	rBV2	257	223	0.02%	0.003%
68	10.458	2927	2929	2934	rVB2	229	191	0.02%	0.002%
69	10.577	2963	2966	2972	rVB4	611	507	0.05%	0.006%
70	10.918	3064	3072	3080	rBV5	2084	2919	0.26%	0.036%
71	10.992	3090	3095	3098	rBV	171	185	0.02%	0.002%
72	11.034	3102	3108	3114	rVB3	577	628	0.06%	0.008%
73	11.063	3114	3117	3121	rBV	252	182	0.02%	0.002%
74	11.143	3136	3142	3149	rVB4	1072	1418	0.13%	0.017%
75	11.246	3163	3174	3193	rBV	458075	694668	62.06%	8.472%
76	11.387	3212	3218	3223	rVV2	836	1017	0.09%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024934.D
 Acq On : 10 Mar 2022 23:18
 Operator : SY/MD
 Sample : N1879-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.429	3224	3231	3244	rVB4	1758	2890	0.26%	0.035%
78	11.622	3279	3291	3320	rBV	469090	726533	64.91%	8.861%
79	11.815	3346	3351	3354	rBV2	248	226	0.02%	0.003%
80	11.837	3354	3358	3360	rVV2	257	184	0.02%	0.002%
81	11.853	3360	3363	3367	rVB2	421	269	0.02%	0.003%
82	12.152	3451	3456	3458	rBV	188	195	0.02%	0.002%
83	12.255	3485	3488	3492	rBV2	277	180	0.02%	0.002%
84	12.497	3559	3563	3565	rBV	206	187	0.02%	0.002%
85	13.271	3801	3804	3808	rBV	365	239	0.02%	0.003%
86	13.529	3879	3884	3886	rBV	422	307	0.03%	0.004%
87	13.612	3906	3910	3918	rBV2	229	300	0.03%	0.004%
88	13.718	3940	3943	3945	rBV	255	181	0.02%	0.002%
89	13.773	3957	3960	3963	rBV3	310	206	0.02%	0.003%
90	14.033	4036	4041	4045	rBV2	495	515	0.05%	0.006%
91	14.214	4094	4097	4100	rBV3	323	235	0.02%	0.003%
92	14.233	4101	4103	4106	rVB2	315	183	0.02%	0.002%
93	14.464	4172	4175	4178	rBB2	469	289	0.03%	0.004%
94	14.487	4178	4182	4185	rBV3	373	339	0.03%	0.004%
95	14.693	4240	4246	4249	rBV2	530	677	0.06%	0.008%
96	15.236	4412	4415	4417	rBV2	277	196	0.02%	0.002%
97	15.824	4593	4598	4600	rBV3	520	522	0.05%	0.006%
98	15.876	4612	4614	4616	rBV2	377	215	0.02%	0.003%
99	16.146	4694	4698	4700	rBV4	460	407	0.04%	0.005%
100	16.236	4722	4726	4730	rBV3	870	864	0.08%	0.011%




Sum of corrected areas: 8199341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024934.D
Acq On : 10 Mar 2022 23:18
Operator : SY/MD
Sample : N1879-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

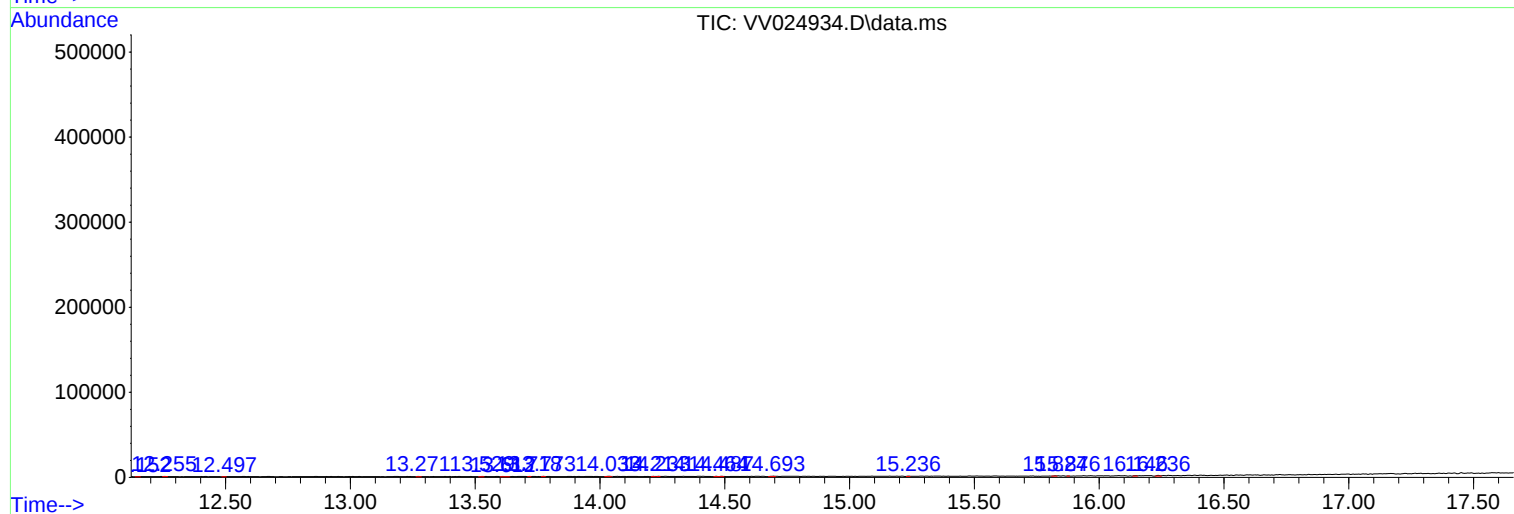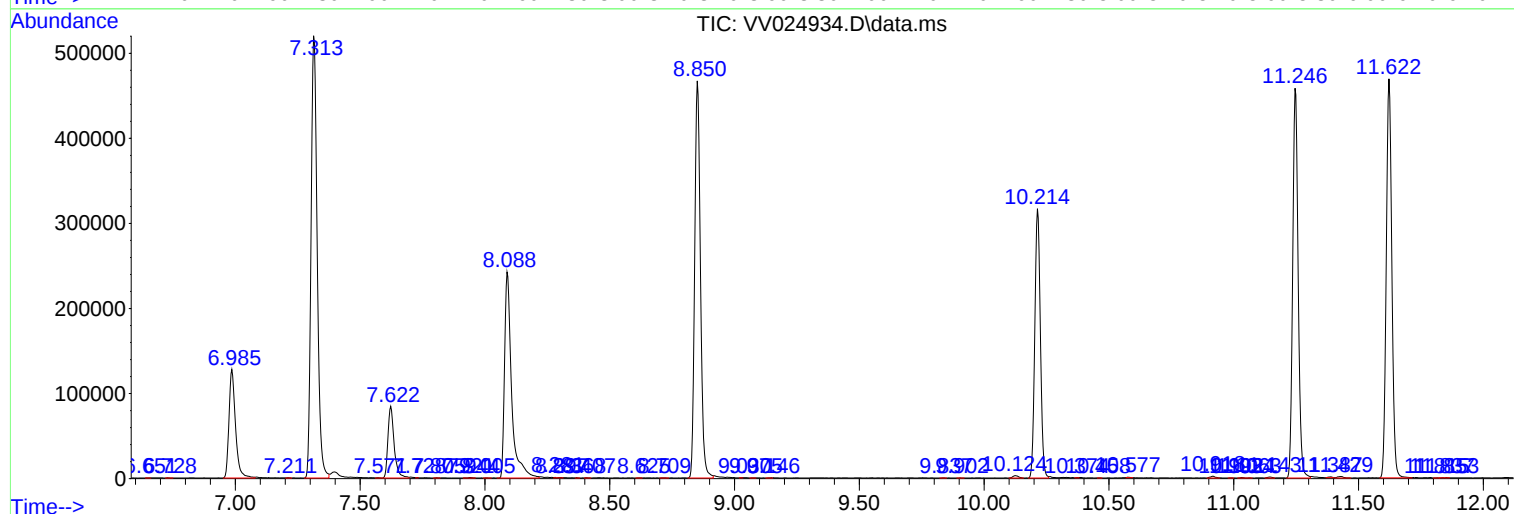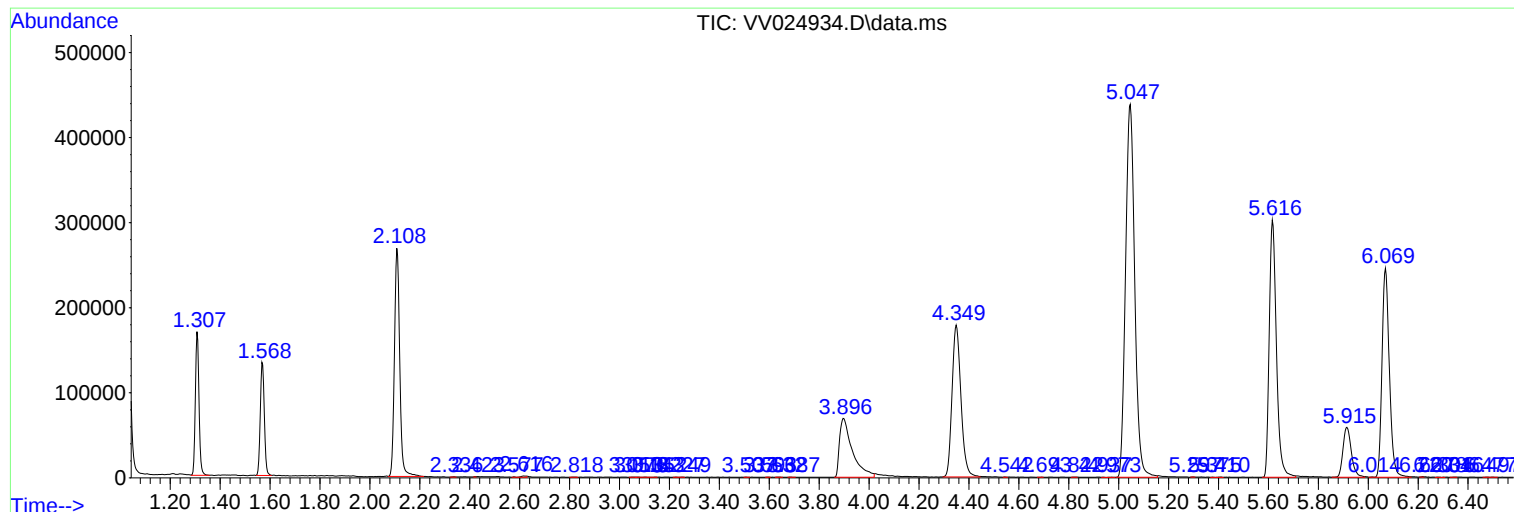

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024934.D
Acq On : 10 Mar 2022 23:18
Operator : SY/MD
Sample : N1879-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024934.D
Acq On : 10 Mar 2022 23:18
Operator : SY/MD
Sample : N1879-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D86

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------