

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024942.D
 Acq On : 11 Mar 2022 02:28
 Operator : SY/MD
 Sample : N1856-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rBV	174111	173334	14.74%	2.035%
2	1.571	157	165	178	rVB	136215	154998	13.18%	1.820%
3	1.809	237	239	240	rBV	691	285	0.02%	0.003%
4	2.108	321	332	354	rBV	281382	413073	35.13%	4.849%
5	2.410	419	426	427	rBV2	171	242	0.02%	0.003%
6	2.593	479	483	485	rBV	343	212	0.02%	0.002%
7	2.625	490	493	498	rBV2	208	186	0.02%	0.002%
8	2.812	547	551	556	rBV2	201	292	0.02%	0.003%
9	2.931	582	588	591	rVB2	241	262	0.02%	0.003%
10	3.011	610	613	619	rVB	198	201	0.02%	0.002%
11	3.063	624	629	633	rBV2	189	188	0.02%	0.002%
12	3.085	633	636	641	rBV2	197	195	0.02%	0.002%
13	3.297	698	702	708	rBV2	191	209	0.02%	0.002%
14	3.365	716	723	725	rBV2	273	297	0.03%	0.003%
15	3.391	725	731	739	rVB2	230	413	0.04%	0.005%
16	3.757	840	845	850	rVB	223	217	0.02%	0.003%
17	3.895	878	888	938	rBV	63163	222242	18.90%	2.609%
18	4.349	1013	1029	1062	rBV	185429	462149	39.30%	5.425%
19	4.612	1107	1111	1114	rBV2	255	248	0.02%	0.003%
20	4.892	1192	1198	1202	rBV	273	302	0.03%	0.004%
21	5.047	1230	1246	1286	rBV2	461146	1175955	100.00%	13.805%
22	5.182	1286	1288	1292	rVB2	414	295	0.03%	0.003%
23	5.317	1328	1330	1335	rVB2	286	188	0.02%	0.002%
24	5.455	1370	1373	1382	rVV2	294	272	0.02%	0.003%
25	5.497	1382	1386	1389	rVV	398	288	0.02%	0.003%
26	5.616	1411	1423	1447	rBV	313884	628415	53.44%	7.377%
27	5.915	1503	1516	1546	rVB5	57480	133013	11.31%	1.561%
28	6.069	1548	1564	1590	rBV	258384	524789	44.63%	6.161%
29	6.217	1605	1610	1618	rVB6	915	1178	0.10%	0.014%
30	6.262	1618	1624	1626	rBV2	249	194	0.02%	0.002%
31	6.628	1735	1738	1741	rVV	258	190	0.02%	0.002%
32	6.664	1744	1749	1753	rVV3	317	380	0.03%	0.004%
33	6.985	1837	1849	1873	rBV	130818	236227	20.09%	2.773%
34	7.317	1940	1952	1971	rBV	545837	945062	80.37%	11.094%
35	7.561	2026	2028	2032	rVB3	495	264	0.02%	0.003%
36	7.622	2037	2047	2069	rBV	86190	151106	12.85%	1.774%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024942.D
 Acq On : 11 Mar 2022 02:28
 Operator : SY/MD
 Sample : N1856-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	7.937	2137	2145	2148	rBV4	981	1068	0.09%	0.013%
38	8.088	2182	2192	2234	rBV	238673	472250	40.16%	5.544%
39	8.288	2247	2254	2256	rBV3	250	332	0.03%	0.004%
40	8.316	2262	2263	2268	rVB	270	215	0.02%	0.003%
41	8.435	2298	2300	2306	rVB2	358	238	0.02%	0.003%
42	8.513	2320	2324	2327	rBV2	384	302	0.03%	0.004%
43	8.619	2355	2357	2363	rVB3	378	315	0.03%	0.004%
44	8.677	2372	2375	2380	rBV	308	200	0.02%	0.002%
45	8.718	2385	2388	2391	rBV	221	176	0.01%	0.002%
46	8.850	2415	2429	2454	rBV	488127	784788	66.74%	9.213%
47	9.079	2497	2500	2505	rBV2	277	240	0.02%	0.003%
48	9.149	2516	2522	2524	rBV2	461	439	0.04%	0.005%
49	9.336	2577	2580	2584	rVB	255	175	0.01%	0.002%
50	9.419	2603	2606	2614	rVB2	203	256	0.02%	0.003%
51	9.471	2614	2622	2625	rBV2	198	250	0.02%	0.003%
52	9.590	2654	2659	2661	rBV	210	190	0.02%	0.002%
53	9.625	2666	2670	2674	rVB2	198	183	0.02%	0.002%
54	9.651	2674	2678	2681	rBV2	220	179	0.02%	0.002%
55	9.802	2720	2725	2728	rBV2	257	291	0.02%	0.003%
56	9.863	2740	2744	2750	rVB2	254	209	0.02%	0.002%
57	10.088	2809	2814	2816	rBV2	243	220	0.02%	0.003%
58	10.127	2819	2826	2835	rVB4	2280	3461	0.29%	0.041%
59	10.214	2841	2853	2870	rBV	315114	502255	42.71%	5.896%
60	10.310	2881	2883	2890	rVB4	517	471	0.04%	0.006%
61	10.374	2900	2903	2913	rVB4	731	1056	0.09%	0.012%
62	10.574	2961	2965	2977	rBV3	732	1369	0.12%	0.016%
63	10.795	3031	3034	3040	rVB2	254	227	0.02%	0.003%
64	10.918	3062	3072	3081	rVV5	1926	2925	0.25%	0.034%
65	11.030	3101	3107	3118	rVB2	641	840	0.07%	0.010%
66	11.107	3127	3131	3135	rBV2	260	242	0.02%	0.003%
67	11.143	3136	3142	3150	rVB5	990	1419	0.12%	0.017%
68	11.246	3158	3174	3204	rBV	474977	734923	62.50%	8.627%
69	11.387	3211	3218	3219	rBV3	811	708	0.06%	0.008%
70	11.429	3225	3231	3238	rVB5	1662	2336	0.20%	0.027%
71	11.622	3279	3291	3313	rBV	492052	768097	65.32%	9.017%
72	11.728	3322	3324	3329	rVB2	538	370	0.03%	0.004%
73	11.760	3329	3334	3336	rBV2	314	281	0.02%	0.003%
74	11.783	3339	3341	3343	rBV3	607	341	0.03%	0.004%
75	11.876	3366	3370	3376	rBV2	247	308	0.03%	0.004%
76	12.072	3427	3431	3434	rVB2	262	185	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024942.D
 Acq On : 11 Mar 2022 02:28
 Operator : SY/MD
 Sample : N1856-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	12.091	3434	3437	3438	rBV2	319	204	0.02%	0.002%
78	12.246	3481	3485	3487	rBV2	293	288	0.02%	0.003%
79	12.381	3524	3527	3529	rBV	259	175	0.01%	0.002%
80	12.500	3560	3564	3569	rVB2	359	365	0.03%	0.004%
81	12.529	3569	3573	3575	rBV	310	243	0.02%	0.003%
82	12.670	3614	3617	3624	rBV2	221	256	0.02%	0.003%
83	12.766	3643	3647	3650	rBV2	210	204	0.02%	0.002%
84	12.914	3689	3693	3697	rBV2	193	219	0.02%	0.003%
85	13.066	3737	3740	3745	rBV	301	222	0.02%	0.003%
86	13.207	3780	3784	3787	rBV	379	288	0.02%	0.003%
87	13.532	3882	3885	3888	rBV	292	192	0.02%	0.002%
88	13.574	3895	3898	3901	rBV2	275	227	0.02%	0.003%
89	13.908	4000	4002	4010	rBV2	253	266	0.02%	0.003%
90	14.030	4036	4040	4042	rBV	439	381	0.03%	0.004%
91	14.181	4085	4087	4091	rVB	357	207	0.02%	0.002%
92	14.204	4091	4094	4097	rBV2	331	235	0.02%	0.003%
93	14.258	4108	4111	4113	rBV2	319	178	0.02%	0.002%
94	14.336	4132	4135	4137	rBV2	276	176	0.01%	0.002%
95	14.548	4198	4201	4204	rBV3	219	175	0.01%	0.002%
96	14.728	4253	4257	4261	rBV2	314	274	0.02%	0.003%
97	15.564	4514	4517	4520	rBV2	387	236	0.02%	0.003%
98	16.059	4669	4671	4675	rBV2	424	302	0.03%	0.004%
99	16.258	4730	4733	4743	rVB5	892	982	0.08%	0.012%
100	16.329	4752	4755	4757	rBV2	590	398	0.03%	0.005%


Sum of corrected areas: 8518384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024942.D
Acq On : 11 Mar 2022 02:28
Operator : SY/MD
Sample : N1856-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

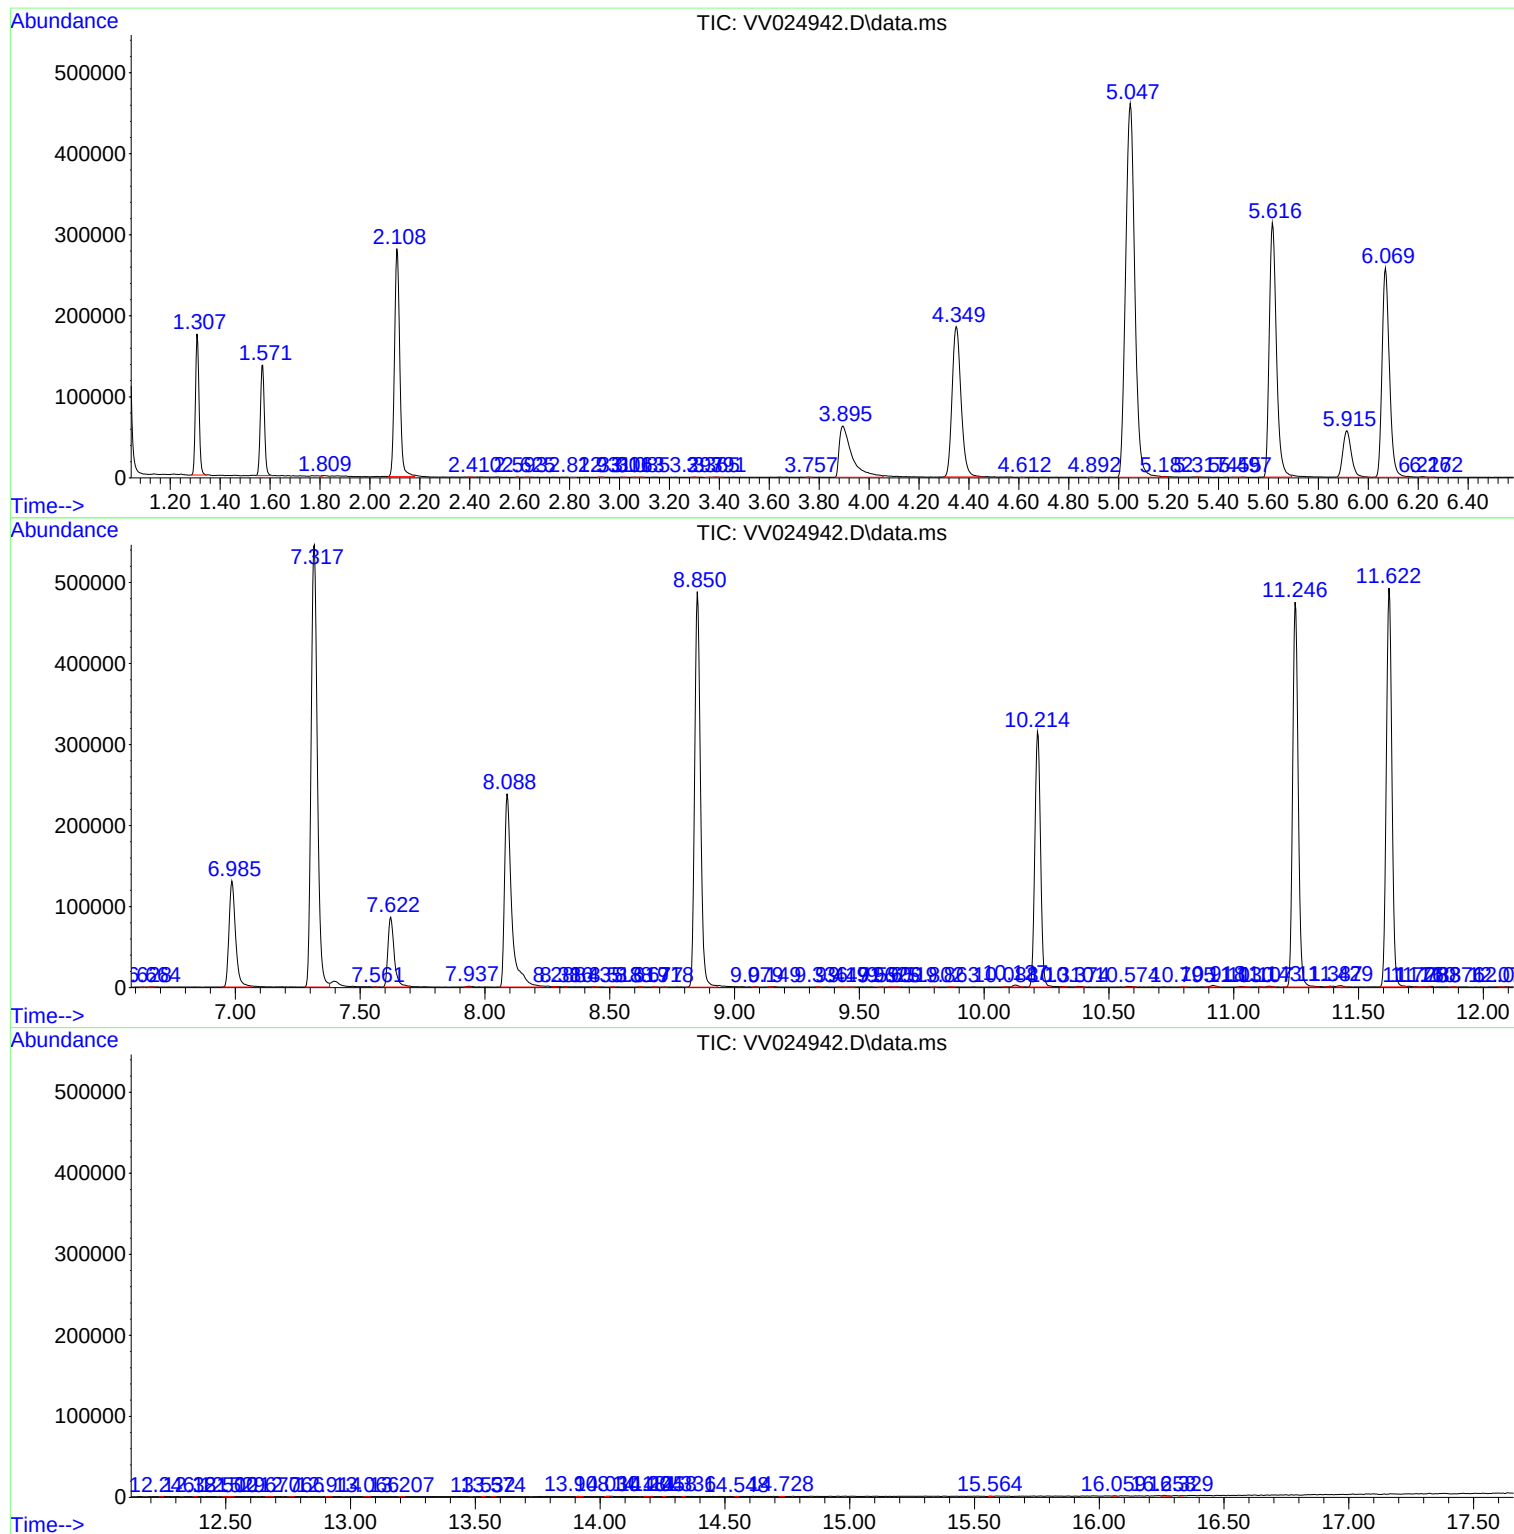

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024942.D
Acq On : 11 Mar 2022 02:28
Operator : SY/MD
Sample : N1856-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024942.D
Acq On : 11 Mar 2022 02:28
Operator : SY/MD
Sample : N1856-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------