

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024946.D
 Acq On : 11 Mar 2022 04:03
 Operator : SY/MD
 Sample : N1856-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	177139	177971	14.80%	1.889%
2	1.571	157	165	178	rVB	136865	156047	12.98%	1.657%
3	2.056	313	316	318	rBV2	761	494	0.04%	0.005%
4	2.108	322	332	372	rVB2	292610	452834	37.66%	4.808%
5	2.323	396	399	402	rBV2	362	277	0.02%	0.003%
6	2.712	517	520	522	rBV	273	142	0.01%	0.002%
7	2.966	595	599	600	rBV	173	116	0.01%	0.001%
8	3.031	610	619	623	rBV2	303	448	0.04%	0.005%
9	3.150	653	656	658	rBV2	222	153	0.01%	0.002%
10	3.297	700	702	706	rBV2	222	173	0.01%	0.002%
11	3.352	716	719	722	rBV	283	161	0.01%	0.002%
12	3.545	773	779	782	rBV2	294	279	0.02%	0.003%
13	3.719	831	833	834	rBV	127	55	0.00%	0.001%
14	3.728	834	836	839	rVV2	129	71	0.01%	0.001%
15	3.748	839	842	846	rBV2	222	179	0.01%	0.002%
16	3.902	878	890	935	rBV	82016	307932	25.61%	3.269%
17	4.349	1013	1029	1057	rBV	190776	474963	39.50%	5.043%
18	4.561	1091	1095	1096	rBV2	350	252	0.02%	0.003%
19	4.616	1101	1112	1130	rVB3	6557	16319	1.36%	0.173%
20	4.709	1138	1141	1142	rBV	97	57	0.00%	0.001%
21	4.722	1142	1145	1148	rVB	273	196	0.02%	0.002%
22	4.754	1153	1155	1156	rBV	173	77	0.01%	0.001%
23	4.796	1167	1168	1170	rVB	170	40	0.00%	0.000%
24	4.812	1170	1173	1176	rBV2	208	143	0.01%	0.002%
25	4.879	1189	1194	1196	rBV	265	250	0.02%	0.003%
26	4.944	1210	1214	1217	rBV	148	104	0.01%	0.001%
27	5.047	1228	1246	1276	rBV2	472141	1202488	100.00%	12.766%
28	5.413	1358	1360	1361	rBV2	307	129	0.01%	0.001%
29	5.513	1388	1391	1393	rBV	174	124	0.01%	0.001%
30	5.561	1404	1406	1408	rBV2	165	57	0.00%	0.001%
31	5.616	1411	1423	1453	rVV	317960	637991	53.06%	6.773%
32	5.912	1502	1515	1548	rBV2	354865	725795	60.36%	7.706%
33	6.069	1551	1564	1595	rVB	268501	537261	44.68%	5.704%
34	6.288	1629	1632	1633	rBV	128	81	0.01%	0.001%
35	6.346	1648	1650	1653	rVB2	271	115	0.01%	0.001%
36	6.387	1660	1663	1665	rBV	228	153	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024946.D
 Acq On : 11 Mar 2022 04:03
 Operator : SY/MD
 Sample : N1856-16
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.400	1665	1667	1674	rVB2	356	328	0.03%	0.003%
38	6.432	1674	1677	1680	rBV	106	90	0.01%	0.001%
39	6.474	1688	1690	1693	rVB2	129	74	0.01%	0.001%
40	6.500	1693	1698	1704	rBV2	184	214	0.02%	0.002%
41	6.551	1711	1714	1715	rBV	137	68	0.01%	0.001%
42	6.580	1720	1723	1725	rBV	196	113	0.01%	0.001%
43	6.625	1734	1737	1739	rBV	192	100	0.01%	0.001%
44	6.645	1739	1743	1747	rBV2	388	315	0.03%	0.003%
45	6.809	1792	1794	1800	rVB2	315	177	0.01%	0.002%
46	6.841	1801	1804	1805	rBV	118	72	0.01%	0.001%
47	6.985	1835	1849	1880	rBV	134171	245633	20.43%	2.608%
48	7.169	1904	1906	1908	rBV	156	76	0.01%	0.001%
49	7.198	1912	1915	1916	rBV2	358	173	0.01%	0.002%
50	7.313	1939	1951	1971	rBV	561131	966136	80.34%	10.257%
51	7.622	2037	2047	2068	rBV	88288	152532	12.68%	1.619%
52	7.796	2098	2101	2105	rVB2	377	311	0.03%	0.003%
53	7.821	2105	2109	2112	rBV2	220	211	0.02%	0.002%
54	7.854	2118	2119	2123	rBV2	163	116	0.01%	0.001%
55	7.931	2137	2143	2145	rBV3	692	637	0.05%	0.007%
56	8.088	2182	2192	2228	rBV	260081	516887	42.98%	5.488%
57	8.407	2289	2291	2294	rBV2	203	88	0.01%	0.001%
58	8.442	2300	2302	2305	rVB2	309	134	0.01%	0.001%
59	8.500	2317	2320	2322	rBV2	193	141	0.01%	0.001%
60	8.561	2336	2339	2341	rBV	188	121	0.01%	0.001%
61	8.657	2362	2369	2374	rBV2	284	409	0.03%	0.004%
62	8.735	2390	2393	2395	rBV2	129	71	0.01%	0.001%
63	8.850	2418	2429	2452	rBV	495124	790298	65.72%	8.390%
64	9.085	2498	2502	2504	rBV2	154	127	0.01%	0.001%
65	9.117	2509	2512	2515	rBV2	380	275	0.02%	0.003%
66	9.699	2690	2693	2700	rBV2	243	317	0.03%	0.003%
67	9.847	2736	2739	2741	rBV2	138	82	0.01%	0.001%
68	9.934	2763	2766	2769	rBV2	255	201	0.02%	0.002%
69	10.214	2839	2853	2872	rBV	330298	521039	43.33%	5.532%
70	10.358	2895	2898	2901	rBV2	310	145	0.01%	0.002%
71	10.538	2948	2954	2957	rBV2	219	248	0.02%	0.003%
72	10.741	3016	3017	3018	rVB	166	32	0.00%	0.000%
73	10.915	3063	3071	3079	rBV4	1673	2382	0.20%	0.025%
74	11.249	3163	3175	3195	rBV	478160	737168	61.30%	7.826%
75	11.622	3279	3291	3311	rBV	508577	786508	65.41%	8.350%
76	12.053	3422	3425	3430	rBV2	243	249	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024946.D
Acq On : 11 Mar 2022 04:03
Operator : SY/MD
Sample : N1856-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D73

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Title : VOC Analysis

77	14.027	4036	4039	4040	rBV	373	206	0.02%	0.002%
78	14.332	4130	4134	4139	rBV2	409	493	0.04%	0.005%
79	14.712	4249	4252	4254	rBV2	364	243	0.02%	0.003%


Sum of corrected areas: 9419167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024946.D
Acq On : 11 Mar 2022 04:03
Operator : SY/MD
Sample : N1856-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

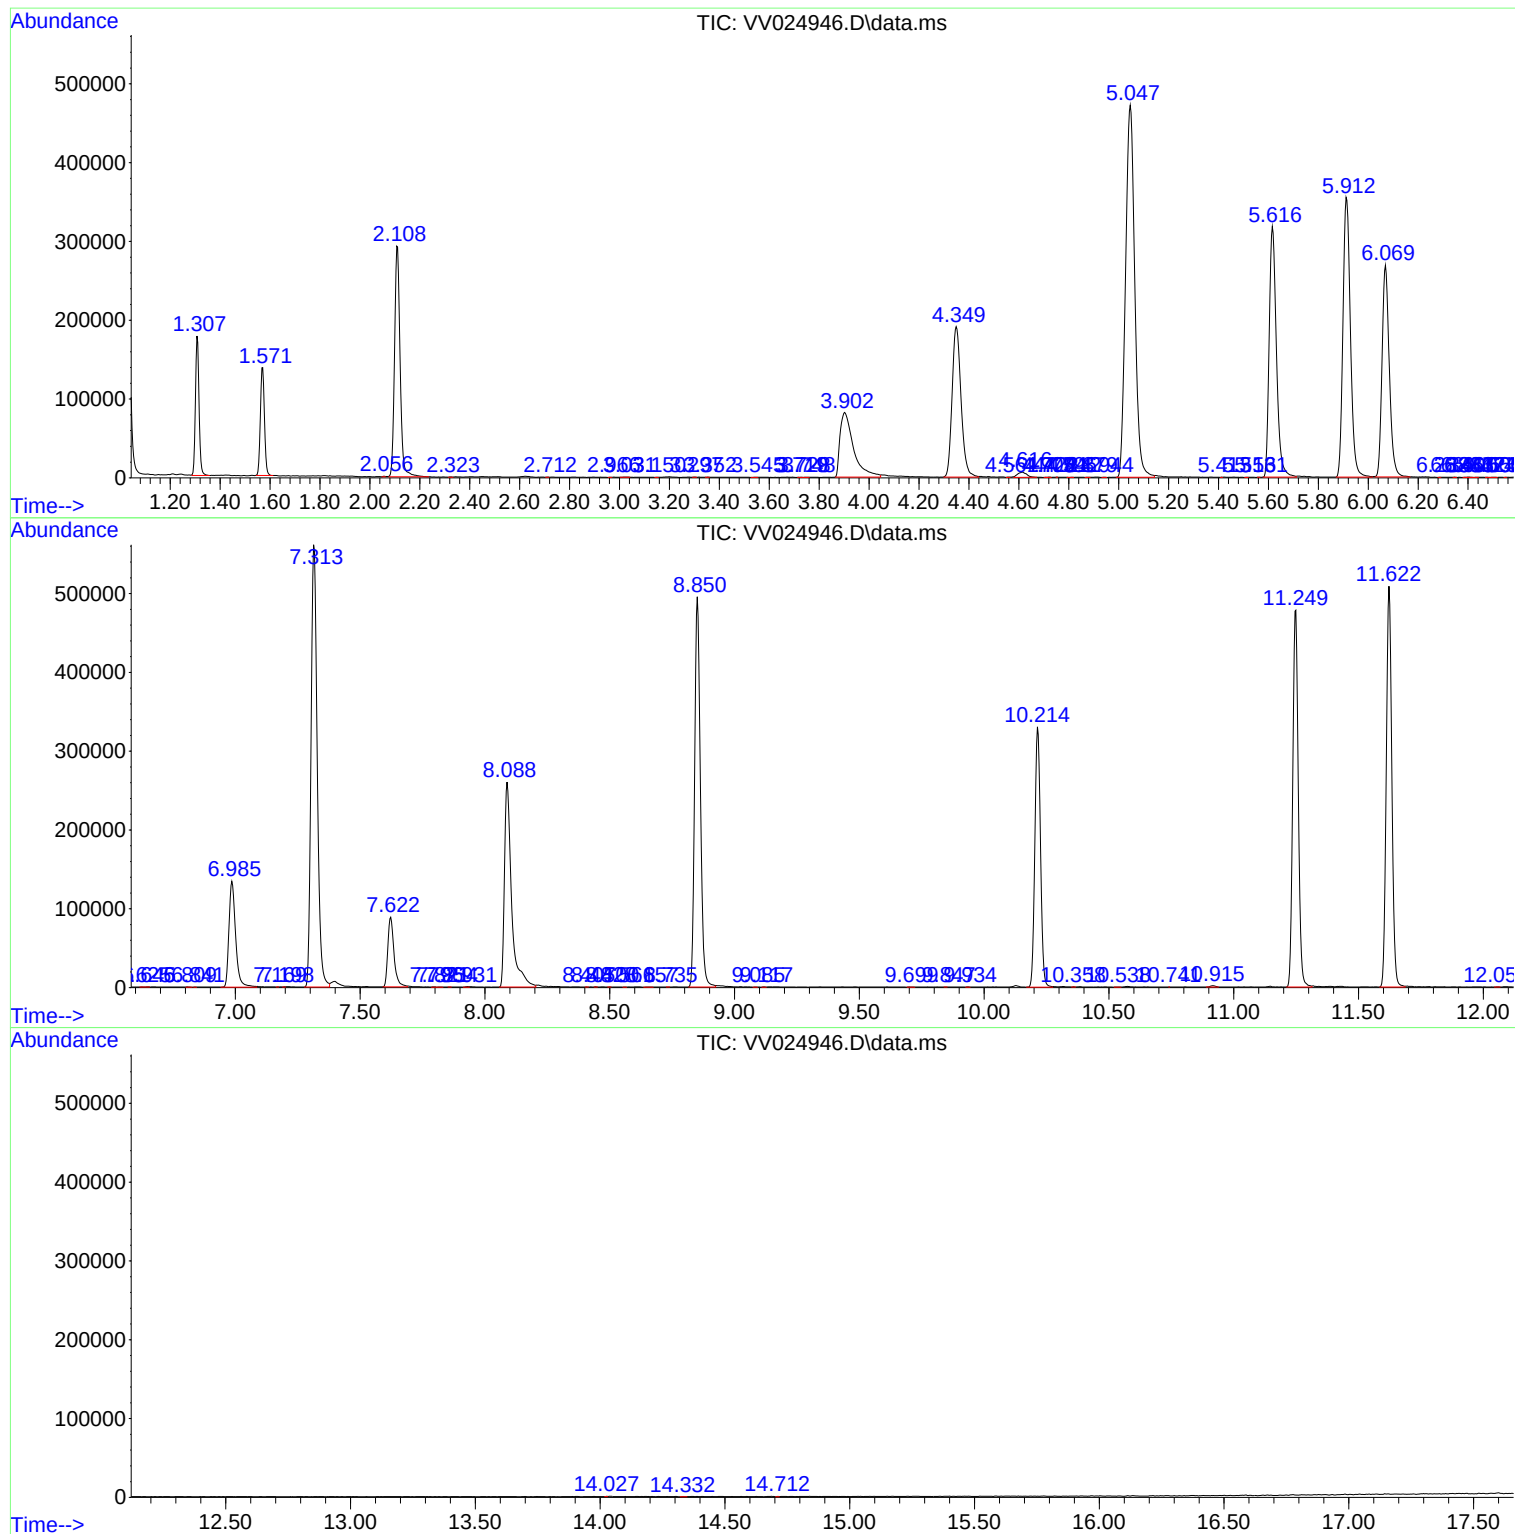

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024946.D
Acq On : 11 Mar 2022 04:03
Operator : SY/MD
Sample : N1856-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024946.D
Acq On : 11 Mar 2022 04:03
Operator : SY/MD
Sample : N1856-16
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------