

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024950.D
 Acq On : 11 Mar 2022 05:37
 Operator : SY/MD
 Sample : N1856-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	167892	171549	14.55%	2.001%
2	1.571	157	165	179	rVB	137026	155631	13.20%	1.816%
3	2.108	322	332	364	rBV	276441	409677	34.75%	4.779%
4	2.452	437	439	441	rBV2	390	257	0.02%	0.003%
5	2.510	454	457	461	rVB3	876	609	0.05%	0.007%
6	2.799	544	547	552	rVB2	160	138	0.01%	0.002%
7	2.921	581	585	589	rBV2	259	204	0.02%	0.002%
8	3.034	618	620	623	rBV	196	164	0.01%	0.002%
9	3.069	628	631	634	rBV2	177	139	0.01%	0.002%
10	3.336	709	714	718	rVB2	183	169	0.01%	0.002%
11	3.362	718	722	724	rBV	206	158	0.01%	0.002%
12	3.394	729	732	736	rBV	107	79	0.01%	0.001%
13	3.484	757	760	762	rBV	121	68	0.01%	0.001%
14	3.548	777	780	783	rBV	170	134	0.01%	0.002%
15	3.658	809	814	817	rBV	382	274	0.02%	0.003%
16	3.818	861	864	865	rBV	140	80	0.01%	0.001%
17	3.899	878	889	930	rBV	63885	229703	19.49%	2.680%
18	4.349	1013	1029	1055	rBV	187552	463196	39.29%	5.403%
19	4.680	1126	1132	1137	rBV2	317	352	0.03%	0.004%
20	4.857	1185	1187	1190	rBV	164	92	0.01%	0.001%
21	4.960	1215	1219	1220	rBV	120	90	0.01%	0.001%
22	5.047	1229	1246	1283	rBV2	457528	1178784	100.00%	13.751%
23	5.448	1368	1371	1372	rBV	84	42	0.00%	0.000%
24	5.461	1372	1375	1378	rVV2	123	75	0.01%	0.001%
25	5.493	1382	1385	1386	rBV	170	81	0.01%	0.001%
26	5.548	1399	1402	1405	rBV2	132	98	0.01%	0.001%
27	5.616	1410	1423	1454	rBV	318245	640761	54.36%	7.475%
28	5.911	1502	1515	1544	rVB7	45312	108096	9.17%	1.261%
29	6.069	1550	1564	1596	rBV	255096	525054	44.54%	6.125%
30	6.201	1602	1605	1609	rBV3	472	371	0.03%	0.004%
31	6.333	1643	1646	1649	rVB2	155	95	0.01%	0.001%
32	6.362	1650	1655	1659	rBV2	313	325	0.03%	0.004%
33	6.397	1663	1666	1668	rBV2	218	151	0.01%	0.002%
34	6.567	1714	1719	1720	rBV	180	141	0.01%	0.002%
35	6.735	1768	1771	1773	rBV	201	111	0.01%	0.001%
36	6.747	1773	1775	1777	rVV	144	67	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031022\
 Data File : VW024950.D
 Acq On : 11 Mar 2022 05:37
 Operator : SY/MD
 Sample : N1856-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.860	1807	1810	1814	rBV	158	114	0.01%	0.001%
38	6.985	1838	1849	1876	rBV	130496	235259	19.96%	2.744%
39	7.162	1901	1904	1905	rBV2	118	58	0.00%	0.001%
40	7.252	1930	1932	1935	rVB	94	50	0.00%	0.001%
41	7.313	1935	1951	1971	rBV	541298	941069	79.83%	10.978%
42	7.622	2037	2047	2077	rBV	85716	151422	12.85%	1.766%
43	7.783	2094	2097	2102	rVB2	255	268	0.02%	0.003%
44	7.809	2102	2105	2107	rBV2	124	79	0.01%	0.001%
45	7.921	2138	2140	2141	rBV	324	163	0.01%	0.002%
46	7.985	2157	2160	2163	rVB2	186	112	0.01%	0.001%
47	8.014	2164	2169	2173	rBV2	164	190	0.02%	0.002%
48	8.088	2182	2192	2232	rBV	248880	502086	42.59%	5.857%
49	8.304	2254	2259	2264	rBV5	503	611	0.05%	0.007%
50	8.371	2277	2280	2283	rBV2	363	246	0.02%	0.003%
51	8.471	2309	2311	2315	rVB2	298	203	0.02%	0.002%
52	8.493	2315	2318	2319	rBV2	170	95	0.01%	0.001%
53	8.503	2319	2321	2326	rVB2	226	151	0.01%	0.002%
54	8.529	2326	2329	2333	rVB	269	182	0.02%	0.002%
55	8.558	2333	2338	2340	rBV2	273	251	0.02%	0.003%
56	8.616	2352	2356	2359	rBV3	272	257	0.02%	0.003%
57	8.709	2382	2385	2392	rVB2	170	177	0.02%	0.002%
58	8.776	2404	2406	2409	rBV2	112	72	0.01%	0.001%
59	8.792	2409	2411	2412	rBV	143	69	0.01%	0.001%
60	8.850	2417	2429	2459	rBV	490118	801996	68.04%	9.356%
61	9.040	2486	2488	2492	rBV3	420	271	0.02%	0.003%
62	9.114	2508	2511	2514	rBV3	257	209	0.02%	0.002%
63	9.152	2518	2523	2527	rBV2	666	650	0.06%	0.008%
64	9.201	2536	2538	2540	rBV	101	66	0.01%	0.001%
65	9.445	2611	2614	2615	rBV2	147	86	0.01%	0.001%
66	9.574	2651	2654	2658	rBV	203	135	0.01%	0.002%
67	9.619	2666	2668	2670	rBV	101	69	0.01%	0.001%
68	9.754	2707	2710	2712	rBV	101	51	0.00%	0.001%
69	9.857	2739	2742	2745	rVB	251	137	0.01%	0.002%
70	9.876	2745	2748	2753	rBV2	135	109	0.01%	0.001%
71	10.098	2814	2817	2819	rBV	179	114	0.01%	0.001%
72	10.127	2819	2826	2836	rVB3	2243	3192	0.27%	0.037%
73	10.214	2841	2853	2875	rBV	323386	510142	43.28%	5.951%
74	10.542	2953	2955	2958	rVB	369	157	0.01%	0.002%
75	10.570	2959	2964	2967	rBV3	692	676	0.06%	0.008%
76	10.834	3042	3046	3047	rBV2	195	144	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024950.D
 Acq On : 11 Mar 2022 05:37
 Operator : SY/MD
 Sample : N1856-20
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	10.863	3051	3055	3058	rBV	311	230	0.02%	0.003%
78	11.030	3102	3107	3113	rBV	388	505	0.04%	0.006%
79	11.246	3163	3174	3201	rBV	490598	750538	63.67%	8.756%
80	11.381	3213	3216	3223	rVB4	914	962	0.08%	0.011%
81	11.471	3243	3244	3246	rVB	242	73	0.01%	0.001%
82	11.622	3279	3291	3312	rBV	502613	778820	66.07%	9.085%
83	11.776	3337	3339	3340	rBV2	279	153	0.01%	0.002%
84	11.844	3358	3360	3365	rVB3	317	183	0.02%	0.002%
85	12.056	3424	3426	3430	rBV	289	265	0.02%	0.003%
86	12.178	3461	3464	3466	rBV2	138	86	0.01%	0.001%
87	12.577	3585	3588	3590	rBV2	181	131	0.01%	0.002%
88	12.619	3599	3601	3604	rBV	181	141	0.01%	0.002%
89	12.660	3611	3614	3618	rVB2	314	226	0.02%	0.003%
90	13.992	4026	4028	4034	rBV2	337	269	0.02%	0.003%
91	14.091	4056	4059	4064	rBV3	376	384	0.03%	0.004%
92	14.339	4133	4136	4138	rBV2	328	245	0.02%	0.003%
93	14.647	4228	4232	4237	rBV	544	573	0.05%	0.007%




Sum of corrected areas: 8572187

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024950.D
Acq On : 11 Mar 2022 05:37
Operator : SY/MD
Sample : N1856-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

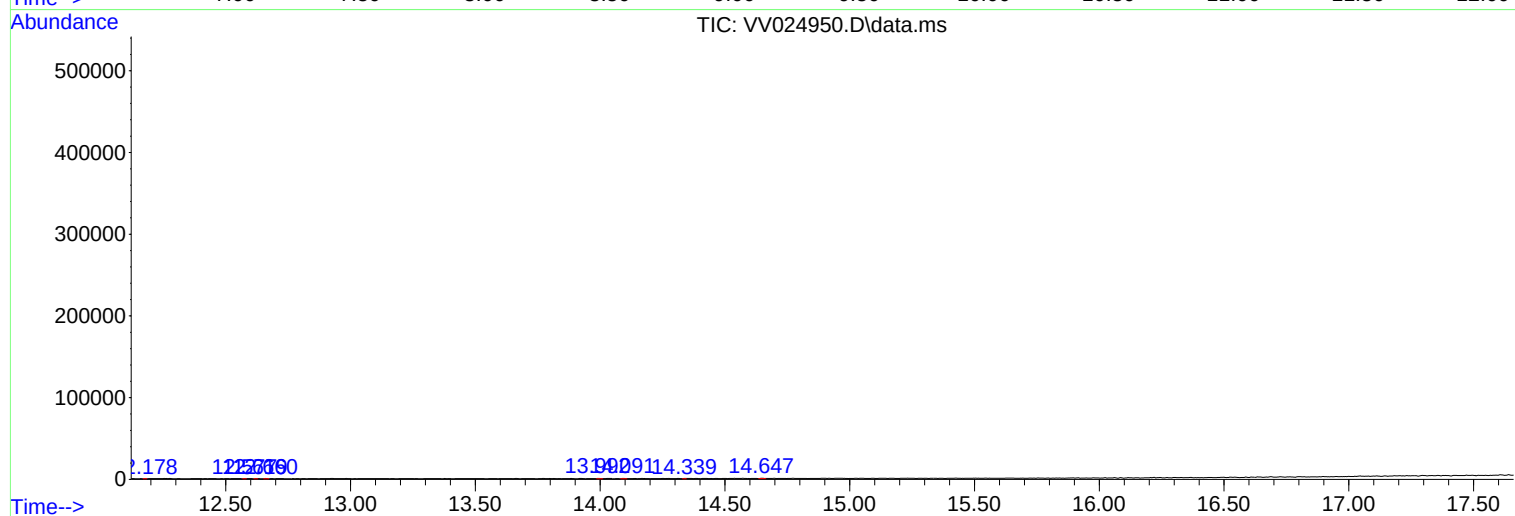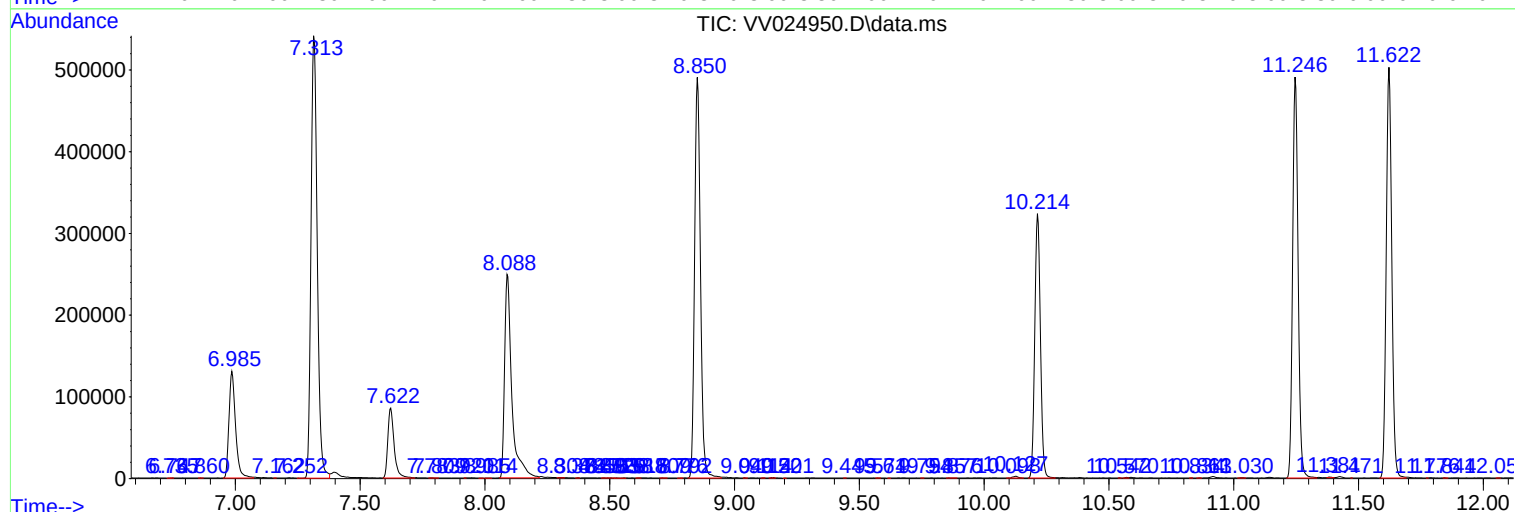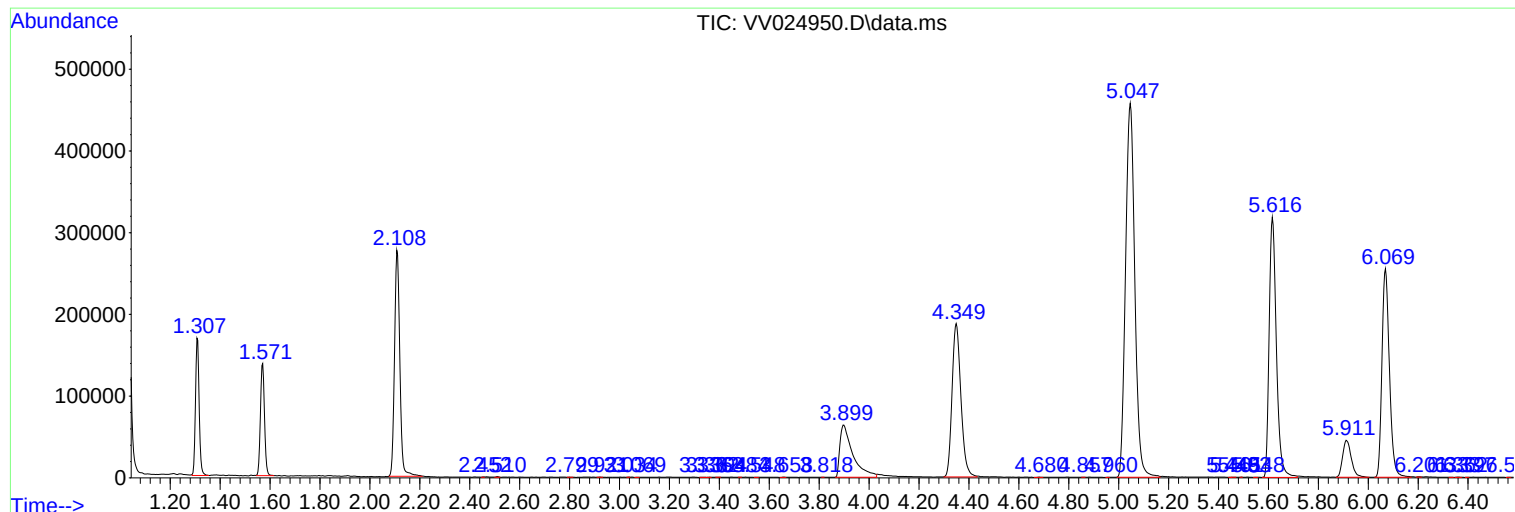

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024950.D
Acq On : 11 Mar 2022 05:37
Operator : SY/MD
Sample : N1856-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
Data File : VV024950.D
Acq On : 11 Mar 2022 05:37
Operator : SY/MD
Sample : N1856-20
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------