
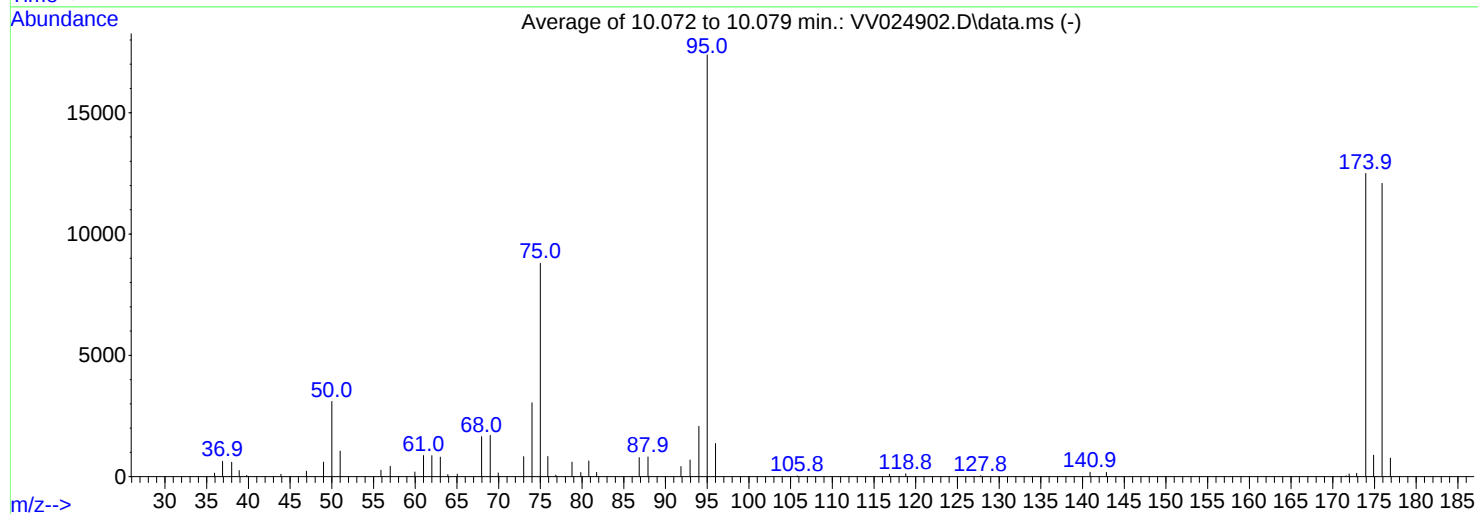


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031022\
 Data File : VV024902.D
 Acq On : 10 Mar 2022 08:55
 Operator : SY/MD
 Sample : BFB203
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB203

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis
 Last Update : Fri Mar 11 23:08:36 2022

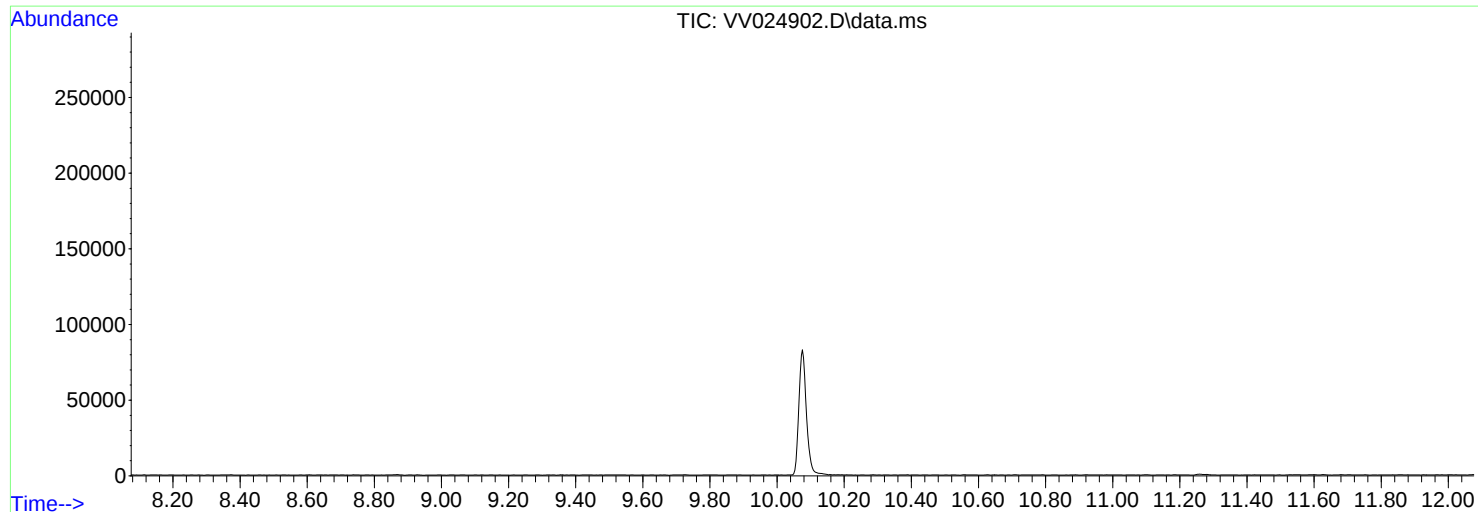

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	3099	PASS
75	95	30	80	50.6	8793	PASS
95	95	100	100	100.0	17387	PASS
96	95	5	9	7.8	1364	PASS
173	174	0.00	2	1.1	139	PASS
174	95	50	120	71.9	12498	PASS
175	174	5	9	7.0	881	PASS
176	174	95	105	96.7	12088	PASS
177	176	5	10	6.4	768	PASS

m/z	Abundance
39.80	346.0
43.90	295.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
35.90	155.0
36.90	619.0
38.00	610.0
38.90	257.0
39.80	411.0
43.90	369.0
47.00	228.0
49.00	584.0
50.00	3220.0
51.00	1088.0
55.90	231.0
57.00	400.0
59.90	213.0
61.00	916.0
62.00	945.0
63.00	870.0
65.10	110.0
68.00	1643.0
69.00	1719.0
69.90	130.0
73.00	774.0
74.00	3075.0
75.00	9013.0
75.90	804.0
76.80	102.0
78.80	678.0
79.90	158.0
80.80	639.0
81.80	168.0
86.80	746.0
87.90	750.0
91.90	444.0
93.00	623.0
94.00	2062.0
95.00	17216.0
96.00	1305.0
105.80	104.0
118.80	116.0
140.80	195.0
142.80	146.0
171.90	121.0
172.90	154.0
173.90	12502.0
174.90	846.0
175.90	11655.0
176.90	670.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
35.90	150.0
36.90	651.0
38.00	622.0
38.90	250.0
39.80	410.0
43.90	390.0
47.00	228.0
49.00	629.0
50.00	3219.0
51.00	1109.0
55.90	265.0
57.00	442.0
59.90	192.0
61.00	899.0
62.00	882.0
63.00	820.0
63.90	125.0
65.10	109.0
68.00	1694.0
69.00	1774.0
70.00	156.0
73.00	838.0
74.00	3161.0
75.00	9113.0
75.90	855.0
76.90	106.0
78.80	613.0
79.90	177.0
80.80	674.0
81.80	186.0
86.90	807.0
87.90	847.0
91.90	420.0
92.90	697.0
94.00	2145.0
95.00	18056.0
96.00	1433.0
116.90	136.0
118.80	118.0
127.80	111.0
140.90	185.0
142.90	178.0
171.90	117.0
172.90	133.0
174.00	12925.0
174.90	904.0
175.90	12561.0
176.90	813.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	133.0
36.90	635.0
38.00	557.0
38.90	237.0
39.90	367.0
43.90	419.0
46.90	219.0
49.00	593.0
50.00	2859.0
51.00	961.0
55.90	299.0
57.00	451.0
60.00	162.0
61.00	801.0
62.00	758.0
63.00	720.0
63.90	142.0
65.00	104.0
67.90	1617.0
69.00	1620.0
70.00	172.0
73.00	860.0
74.00	2899.0
75.00	8253.0
75.90	839.0
78.80	512.0
79.80	178.0
80.80	633.0
81.70	177.0
86.90	798.0
87.90	834.0
91.80	380.0
92.90	728.0
94.00	2020.0
95.00	16888.0
96.00	1354.0
116.80	169.0
118.80	120.0
141.00	163.0
142.90	219.0
171.60	102.0
172.00	107.0
172.80	129.0
174.00	12066.0
174.90	894.0
175.90	12048.0
176.90	822.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203