




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD9

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/14/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 11 23:10:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 23:08:36 2022
Response via : Initial Calibration

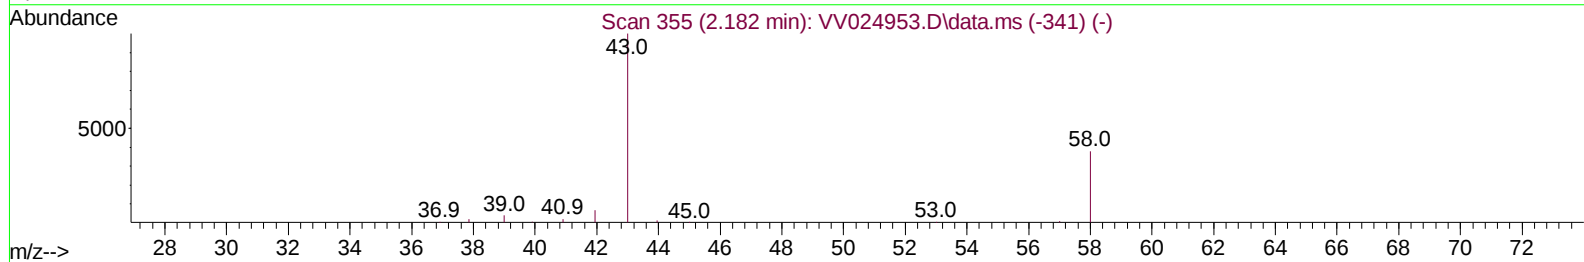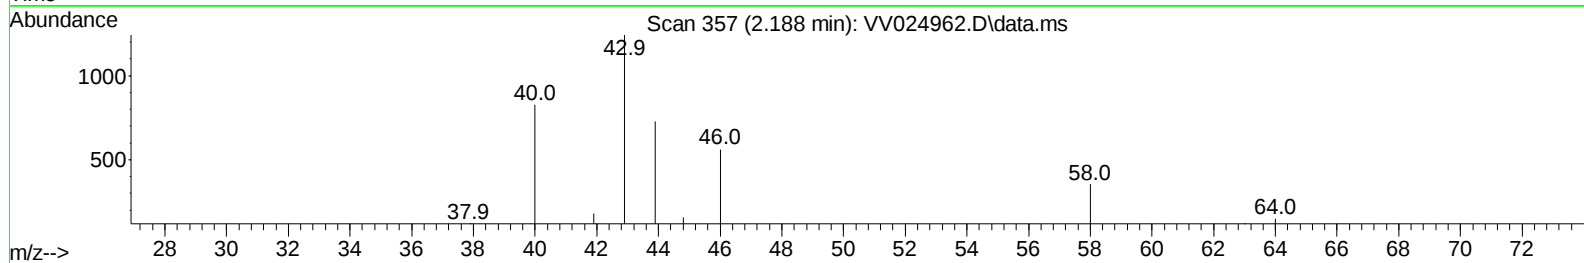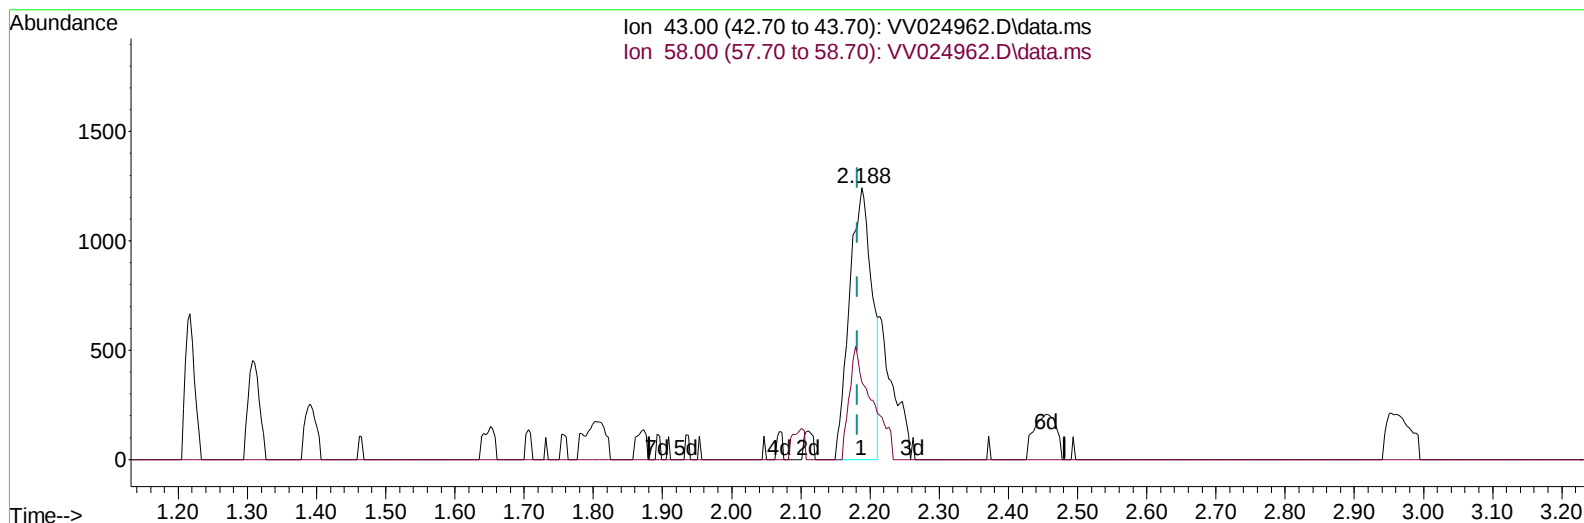

TIC: VV024962.D\data.ms

(13) Acetone (T)

2.188min (+ 0.006) 2.05 ug/L

response 2839

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.00	39.13
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD9

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/14/2022
Supervised By :Mahesh Dadoda 03/16/2022

Quant Time: Mar 11 23:10:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 23:08:36 2022
Response via : Initial Calibration

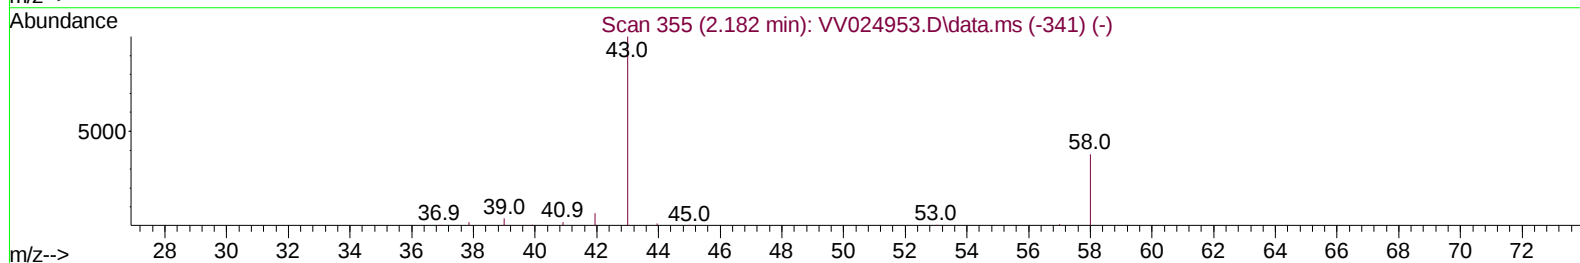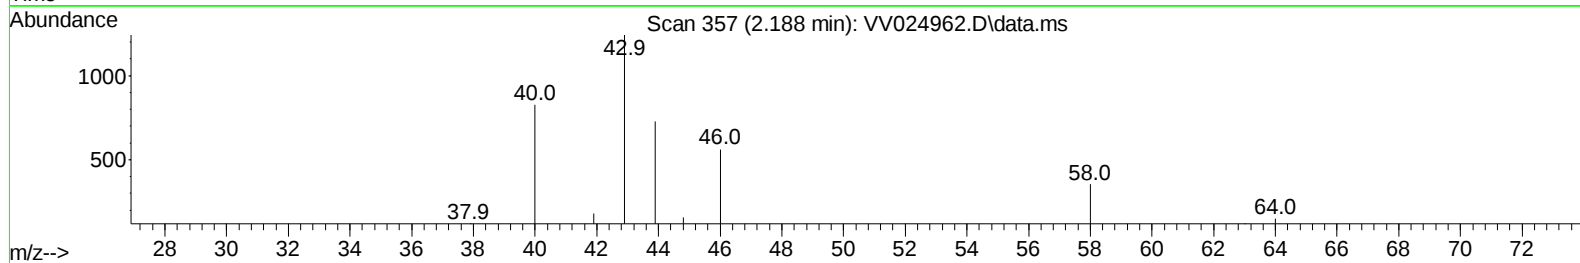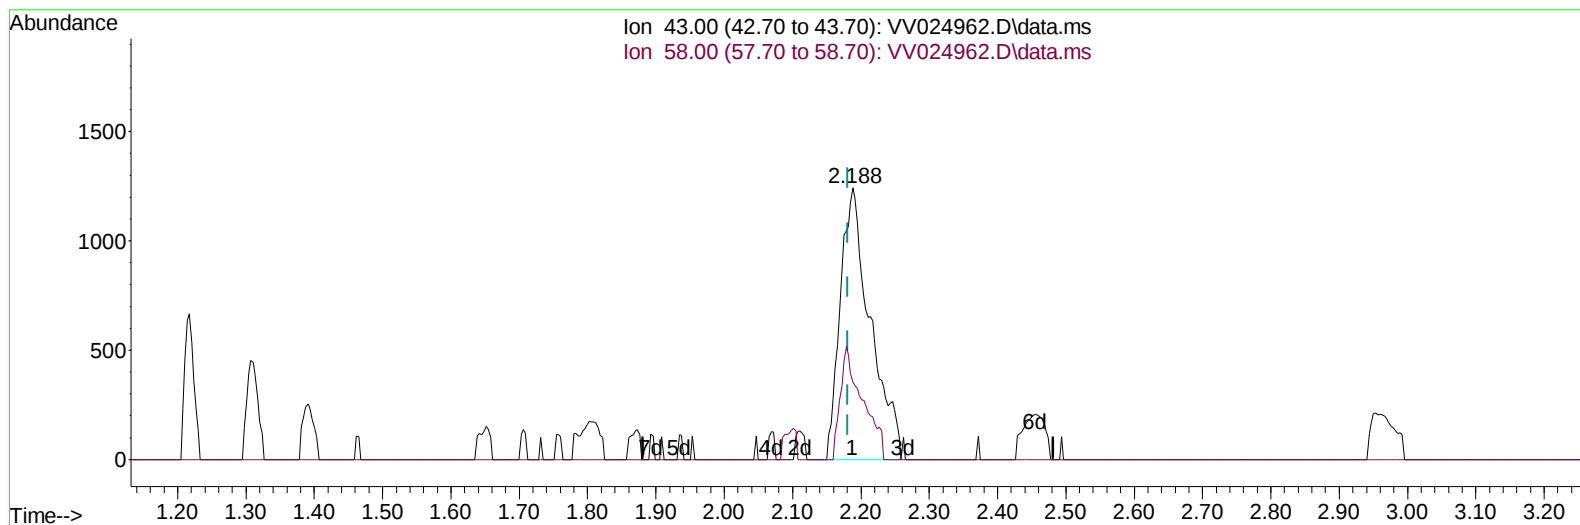

TIC: VV024962.D\data.ms

(13) Acetone (T)

2.188min (+ 0.006) 2.73 ug/L m

response 3774

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	35.00	29.44
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024962.D
 Acq On : 11 Mar 2022 14:11
 Operator : SY/MD
 Sample : N1880-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD9

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:10:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 23:08:36 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/14/2022
 Supervised By :Mahesh Dadoda 03/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	312978	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	305839	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	137950	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	148127	46.546	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	93.100%	
7) Chloroethane-d5	1.568	69	111074	44.486	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	88.980%	
11) 1,1-Dichloroethene-d2	2.108	63	184634	34.566	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	69.140%	
21) 2-Butanone-d5	3.892	46	164451	90.802	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	90.800%	
24) Chloroform-d	4.349	84	239509	43.113	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	86.220%	
26) 1,2-Dichloroethane-d4	5.031	65	144676	44.138	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	88.280%	
32) Benzene-d6	5.050	84	512741	45.231	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	90.460%	
36) 1,2-Dichloropropane-d6	6.069	67	159023	45.025	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	90.060%	
41) Toluene-d8	7.313	98	451000	44.908	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	89.820%	
43) trans-1,3-Dichloroprop...	7.619	79	65788	42.868	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.740%	
47) 2-Hexanone-d5	8.088	63	109905	81.981	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	81.980%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	183512	43.806	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	87.620%	
66) 1,2-Dichlorobenzene-d4	11.622	152	150357	47.316	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	94.640%	
Target Compounds						
13) Acetone	2.188	43	3774m	2.729	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD9

Manual IntegrationsAPPROVED

Quant Time: Mar 11 23:10:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 23:08:36 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/14/2022
Supervised By :Mahesh Dadoda 03/16/2022

