

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031122\
 Data File : VW024962.D
 Acq On : 11 Mar 2022 14:11
 Operator : SY/MD
 Sample : N1880-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD9

Manual Integrations
 APPROVED

Reviewed By : John Carlone 03/14/2022
 Supervised By : Mahesh Dadoda 03/16/2022

Quant Time: Mar 11 23:10:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 11 23:08:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	312978	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	305839	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	137950	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	148127	46.546	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.100%		
7) Chloroethane-d5	1.568	69	111074	44.486	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.980%		
11) 1,1-Dichloroethene-d2	2.108	63	184634	34.566	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.140%		
21) 2-Butanone-d5	3.892	46	164451	90.802	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.800%		
24) Chloroform-d	4.349	84	239509	43.113	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.220%		
26) 1,2-Dichloroethane-d4	5.031	65	144676	44.138	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.280%		
32) Benzene-d6	5.050	84	512741	45.231	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.460%		
36) 1,2-Dichloropropane-d6	6.069	67	159023	45.025	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.060%		
41) Toluene-d8	7.313	98	451000	44.908	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.820%		
43) trans-1,3-Dichloroprop...	7.619	79	65788	42.868	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.740%		
47) 2-Hexanone-d5	8.088	63	109905	81.981	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	81.980%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	183512	43.806	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.620%		
66) 1,2-Dichlorobenzene-d4	11.622	152	150357	47.316	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.640%		
Target Compounds					Qvalue	
13) Acetone	2.188	43	3774m	2.729	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0DD9

Manual Integrations
APPROVED

Reviewed By : John Carlone 03/14/2022
Supervised By : Mahesh Dadoda 03/16/2022


Quant Time: Mar 11 23:10:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 11 23:08:36 2022
Response via : Initial Calibration

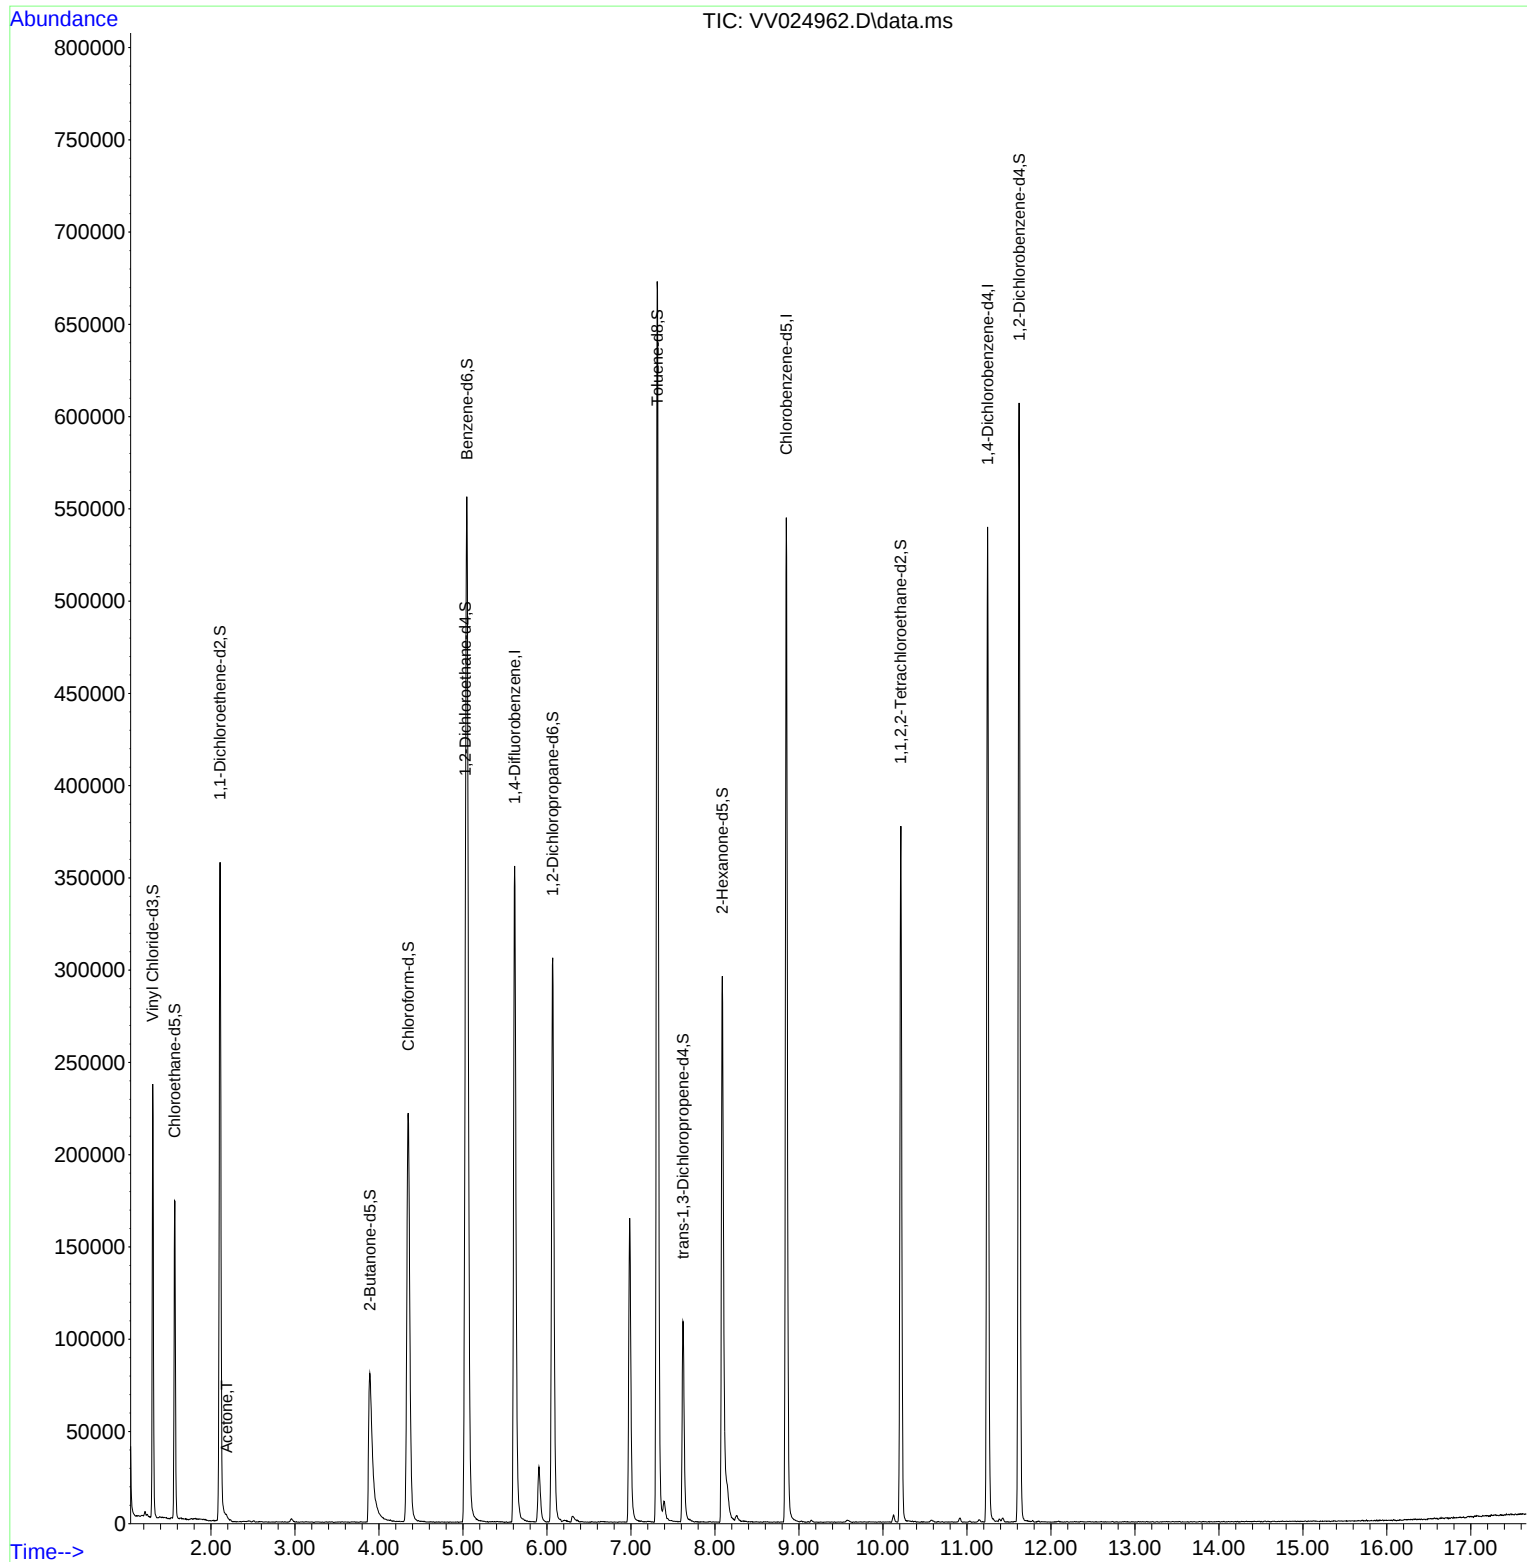

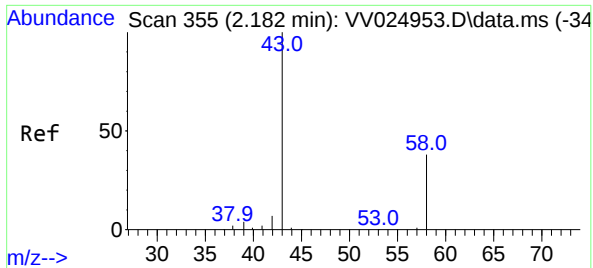

#13
Acetone
Concen: 2.729 ug/L m
RT: 2.188 min Scan# 31
Delta R.T. 0.006 min
Lab File: VV024962.D
Acq: 11 Mar 2022 14:11

Instrument :
MSVOA_V
ClientSampleId :
C0DD9

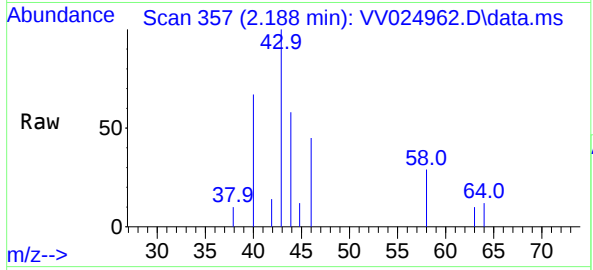

Tgt Ion: 43 Resp: 3774
Ion Ratio Lower Upper
43 100
58 29.4 0.0 70.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 03/14/2022
Supervised By :Mahesh Dadoda 03/16/2022

