

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024959.D
 Acq On : 11 Mar 2022 13:00
 Operator : SY/MD
 Sample : N1855-12DL 5X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024959.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	102	rVB	239537	243651	16.71%	2.161%
2	1.568	157	164	177	rBV	178209	199588	13.69%	1.770%
3	2.108	321	332	366	rBV2	379551	577950	39.63%	5.125%
4	2.371	408	414	415	rBV	196	189	0.01%	0.002%
5	2.912	580	582	585	rBV2	151	80	0.01%	0.001%
6	2.950	585	594	599	rVV	244	416	0.03%	0.004%
7	3.079	631	634	636	rBV	199	119	0.01%	0.001%
8	3.188	663	668	675	rBV3	648	1127	0.08%	0.010%
9	3.365	720	723	725	rBV	222	124	0.01%	0.001%
10	3.503	764	766	769	rBV	154	84	0.01%	0.001%
11	3.600	793	796	798	rBV2	155	106	0.01%	0.001%
12	3.638	804	808	812	rBV2	336	314	0.02%	0.003%
13	3.741	836	840	846	rBV2	279	354	0.02%	0.003%
14	3.851	871	874	876	rBV	244	153	0.01%	0.001%
15	3.902	877	890	935	rBV3	93611	349560	23.97%	3.100%
16	4.349	1013	1029	1064	rBV	227771	565049	38.75%	5.011%
17	4.613	1096	1111	1131	rVB2	18415	45035	3.09%	0.399%
18	4.683	1131	1133	1140	rVV2	397	339	0.02%	0.003%
19	4.719	1140	1144	1149	rVB	175	171	0.01%	0.002%
20	4.847	1182	1184	1195	rVB2	233	178	0.01%	0.002%
21	4.944	1212	1214	1219	rBV2	307	284	0.02%	0.003%
22	5.047	1228	1246	1285	rBV2	568473	1458203	100.00%	12.932%
23	5.339	1335	1337	1339	rBV3	288	158	0.01%	0.001%
24	5.416	1357	1361	1366	rBV2	268	299	0.02%	0.003%
25	5.494	1380	1385	1388	rBV3	339	318	0.02%	0.003%
26	5.616	1411	1423	1452	rBV	330685	670741	46.00%	5.948%
27	5.857	1494	1498	1501	rBV2	412	426	0.03%	0.004%
28	5.912	1501	1515	1544	rVV2	519584	1044571	71.63%	9.264%
29	6.069	1551	1564	1589	rBV	312718	635994	43.61%	5.640%
30	6.288	1629	1632	1635	rBV3	326	249	0.02%	0.002%
31	6.391	1662	1664	1665	rBV	133	61	0.00%	0.001%
32	6.448	1678	1682	1685	rBV	227	197	0.01%	0.002%
33	6.468	1685	1688	1690	rVV2	268	155	0.01%	0.001%
34	6.484	1690	1693	1696	rVV2	140	101	0.01%	0.001%
35	6.522	1702	1705	1707	rBV	126	87	0.01%	0.001%
36	6.567	1711	1719	1721	rBV2	355	423	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031122\
 Data File : VW024959.D
 Acq On : 11 Mar 2022 13:00
 Operator : SY/MD
 Sample : N1855-12DL 5X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.635	1736	1740	1742	rBV2	429	315	0.02%	0.003%
38	6.860	1806	1810	1813	rVV2	333	238	0.02%	0.002%
39	6.879	1813	1816	1820	rVB2	214	171	0.01%	0.002%
40	6.928	1828	1831	1838	rVB2	215	256	0.02%	0.002%
41	6.985	1838	1849	1875	rBV	169071	305729	20.97%	2.711%
42	7.191	1910	1913	1915	rBV	438	328	0.02%	0.003%
43	7.243	1927	1929	1932	rVB	334	174	0.01%	0.002%
44	7.259	1932	1934	1936	rBV	222	134	0.01%	0.001%
45	7.313	1939	1951	1970	rBV	691540	1192314	81.77%	10.574%
46	7.619	2036	2046	2074	rBV	110802	191929	13.16%	1.702%
47	7.744	2082	2085	2090	rVB4	544	435	0.03%	0.004%
48	7.825	2108	2110	2113	rBV	322	187	0.01%	0.002%
49	7.866	2121	2123	2124	rBV	335	120	0.01%	0.001%
50	8.030	2172	2174	2180	rBV2	259	242	0.02%	0.002%
51	8.088	2182	2192	2233	rBV	309852	606850	41.62%	5.382%
52	8.461	2304	2308	2311	rVB2	197	135	0.01%	0.001%
53	8.474	2311	2312	2313	rBV2	129	35	0.00%	0.000%
54	8.490	2314	2317	2324	rVB2	376	415	0.03%	0.004%
55	8.535	2328	2331	2335	rBV	371	274	0.02%	0.002%
56	8.609	2352	2354	2355	rBV	343	127	0.01%	0.001%
57	8.683	2373	2377	2389	rBV2	291	510	0.03%	0.005%
58	8.731	2389	2392	2393	rBV	193	116	0.01%	0.001%
59	8.767	2400	2403	2404	rBV2	204	119	0.01%	0.001%
60	8.799	2411	2413	2417	rBV	191	107	0.01%	0.001%
61	8.850	2418	2429	2466	rBV	514146	835852	57.32%	7.413%
62	9.111	2508	2510	2513	rVB	360	142	0.01%	0.001%
63	9.320	2572	2575	2577	rBV	181	117	0.01%	0.001%
64	9.529	2634	2640	2643	rBV2	294	323	0.02%	0.003%
65	9.577	2652	2655	2658	rBV2	202	112	0.01%	0.001%
66	9.792	2720	2722	2727	rVB2	229	156	0.01%	0.001%
67	9.818	2727	2730	2734	rBV	293	263	0.02%	0.002%
68	10.053	2800	2803	2805	rBV	137	82	0.01%	0.001%
69	10.091	2811	2815	2817	rBV	290	222	0.02%	0.002%
70	10.127	2819	2826	2835	rVB2	4388	6238	0.43%	0.055%
71	10.214	2841	2853	2873	rBV	384819	599101	41.08%	5.313%
72	10.654	2987	2990	2993	rBV	288	220	0.02%	0.002%
73	10.767	3023	3025	3029	rVB2	321	191	0.01%	0.002%
74	10.792	3030	3033	3036	rBV2	263	170	0.01%	0.002%
75	10.918	3063	3072	3080	rVB4	2802	4136	0.28%	0.037%
76	11.027	3102	3106	3114	rBV3	560	672	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024959.D
 Acq On : 11 Mar 2022 13:00
 Operator : SY/MD
 Sample : N1855-12DL 5X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0D38DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M

Title : VOC Analysis

77	11.095	3125	3127	3130	rBV2	146	82	0.01%	0.001%
78	11.146	3136	3143	3151	rVB6	1535	2374	0.16%	0.021%
79	11.246	3163	3174	3193	rBV	496060	775100	53.15%	6.874%
80	11.622	3279	3291	3310	rBV	603872	950363	65.17%	8.428%
81	11.783	3336	3341	3348	rVB6	1009	1249	0.09%	0.011%
82	12.210	3470	3474	3480	rBV2	245	303	0.02%	0.003%
83	12.480	3556	3558	3561	rBV2	202	118	0.01%	0.001%
84	13.731	3943	3947	3950	rBV2	326	308	0.02%	0.003%
85	14.197	4090	4092	4095	rBV	245	181	0.01%	0.002%




Sum of corrected areas: 11276189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024959.D
Acq On : 11 Mar 2022 13:00
Operator : SY/MD
Sample : N1855-12DL 5X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

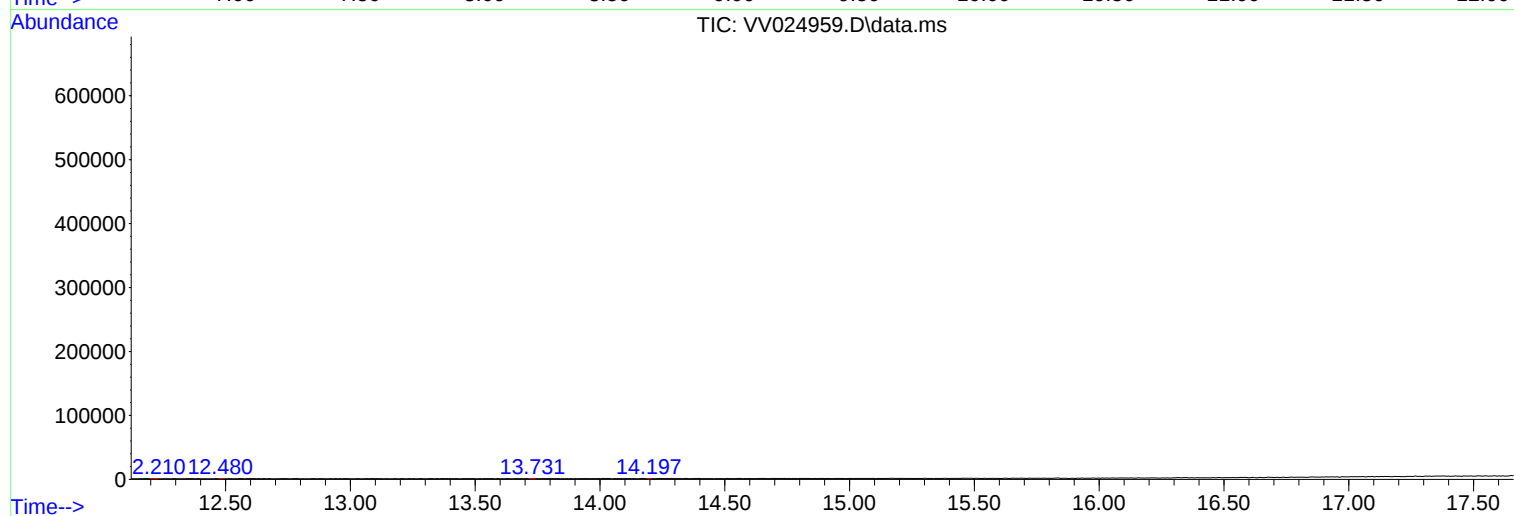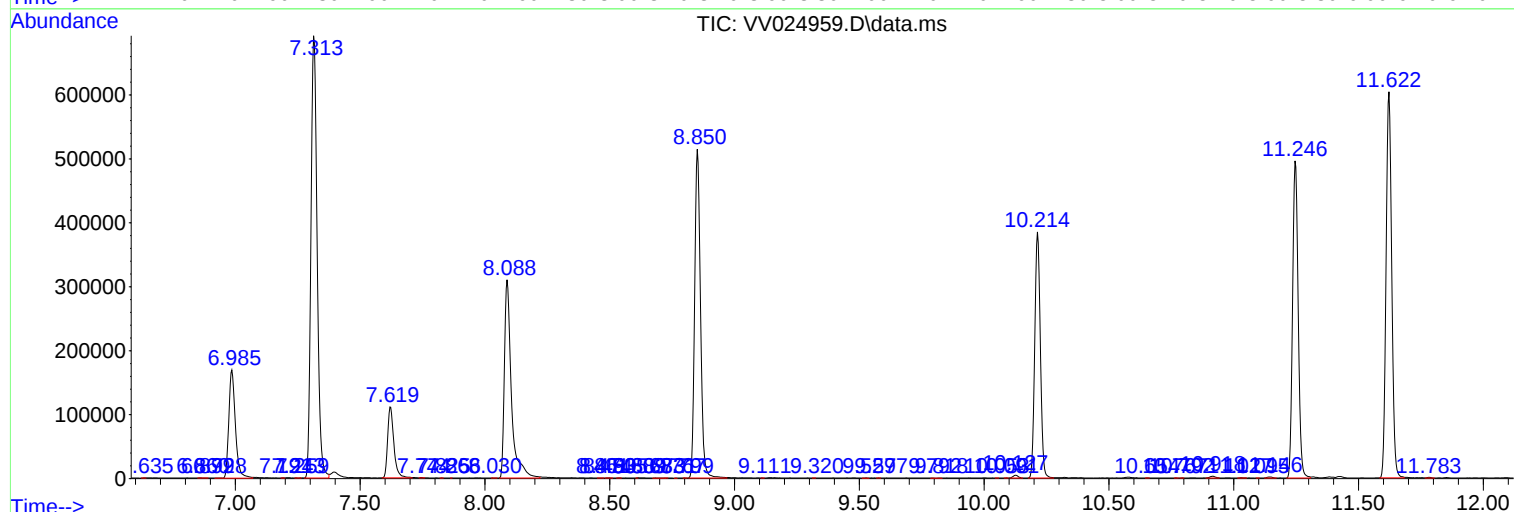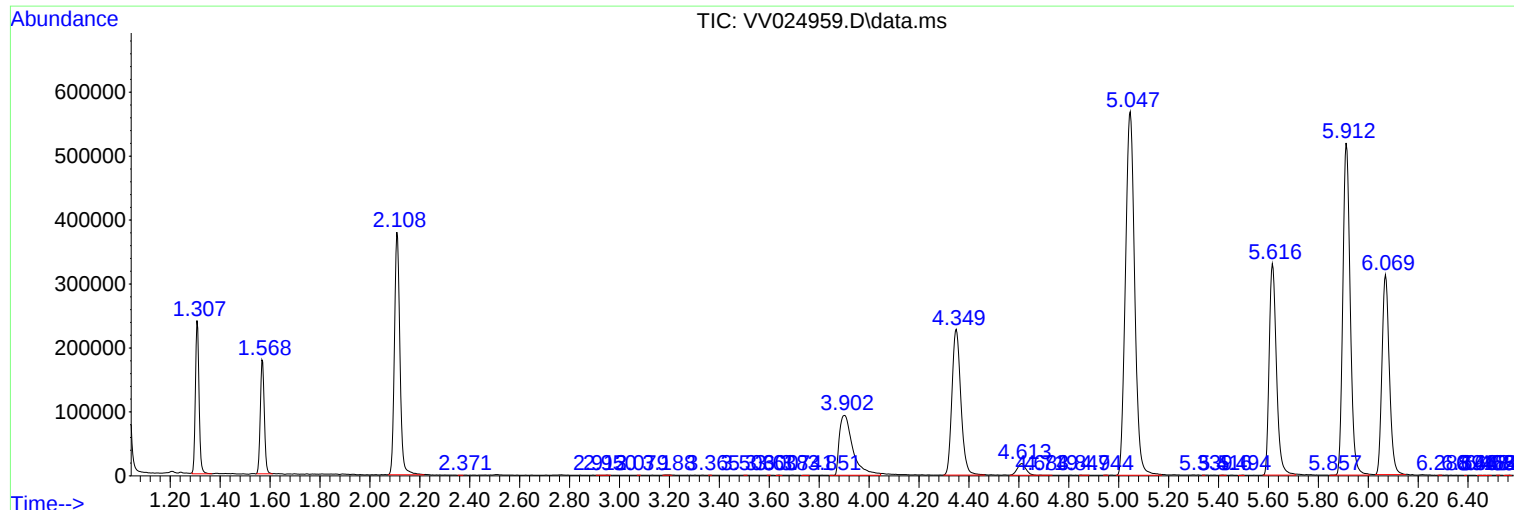

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024959.D
Acq On : 11 Mar 2022 13:00
Operator : SY/MD
Sample : N1855-12DL 5X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024959.D
Acq On : 11 Mar 2022 13:00
Operator : SY/MD
Sample : N1855-12DL 5X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0D38DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc