

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024962.D
 Acq On : 11 Mar 2022 14:11
 Operator : SY/MD
 Sample : N1880-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	98	rVB	235046	236654	16.69%	2.346%
2	1.568	156	164	179	rVB	172271	195437	13.79%	1.937%
3	2.108	321	332	353	rBV	356630	518504	36.57%	5.140%
4	2.378	410	416	417	rBV2	285	260	0.02%	0.003%
5	2.507	449	456	464	rVB4	707	1103	0.08%	0.011%
6	2.777	536	540	544	rBV2	377	356	0.03%	0.004%
7	2.880	569	572	581	rVB2	280	323	0.02%	0.003%
8	2.957	586	596	606	rBV5	1790	3274	0.23%	0.032%
9	3.066	625	630	634	rBV	242	278	0.02%	0.003%
10	3.243	681	685	688	rBV2	303	311	0.02%	0.003%
11	3.375	718	726	731	rBV2	252	397	0.03%	0.004%
12	3.407	731	736	741	rBV2	251	327	0.02%	0.003%
13	3.564	778	785	790	rBV	249	347	0.02%	0.003%
14	3.783	847	853	863	rBV2	326	532	0.04%	0.005%
15	3.892	876	887	935	rBV	80657	272133	19.20%	2.698%
16	4.349	1011	1029	1063	rBV	221472	551113	38.87%	5.463%
17	4.539	1086	1088	1093	rVB4	353	273	0.02%	0.003%
18	4.677	1128	1131	1134	rBV	267	220	0.02%	0.002%
19	4.844	1179	1183	1189	rBV	243	283	0.02%	0.003%
20	4.976	1215	1224	1226	rBV	247	316	0.02%	0.003%
21	5.047	1229	1246	1281	rBV2	555717	1417670	100.00%	14.053%
22	5.320	1326	1331	1334	rBV2	331	347	0.02%	0.003%
23	5.410	1355	1359	1364	rVB2	268	273	0.02%	0.003%
24	5.519	1386	1393	1396	rVB3	370	367	0.03%	0.004%
25	5.548	1396	1402	1404	rBV	324	222	0.02%	0.002%
26	5.616	1411	1423	1460	rBV	355602	707777	49.93%	7.016%
27	5.905	1501	1513	1537	rBV	29861	63037	4.45%	0.625%
28	6.069	1549	1564	1591	rBV	305817	621093	43.81%	6.157%
29	6.207	1598	1607	1609	rBV4	844	1110	0.08%	0.011%
30	6.307	1631	1638	1649	rBV6	3178	7409	0.52%	0.073%
31	6.532	1704	1708	1714	rVV3	325	355	0.03%	0.004%
32	6.612	1728	1733	1738	rBV2	248	264	0.02%	0.003%
33	6.638	1738	1741	1743	rBV	343	213	0.02%	0.002%
34	6.860	1805	1810	1815	rBV2	276	382	0.03%	0.004%
35	6.985	1838	1849	1876	rBV	164756	296729	20.93%	2.941%
36	7.194	1911	1914	1916	rBV2	417	296	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024962.D
 Acq On : 11 Mar 2022 14:11
 Operator : SY/MD
 Sample : N1880-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	7.252	1929	1932	1938	rVB3	291	243	0.02%	0.002%
38	7.313	1939	1951	1970	rBV	672412	1156269	81.56%	11.462%
39	7.548	2021	2024	2027	rVB4	366	276	0.02%	0.003%
40	7.619	2037	2046	2067	rBV	108671	186827	13.18%	1.852%
41	7.773	2088	2094	2097	rBV3	360	299	0.02%	0.003%
42	8.088	2181	2192	2237	rBV	295984	583184	41.14%	5.781%
43	8.259	2237	2245	2255	rVV8	3213	6934	0.49%	0.069%
44	8.580	2341	2345	2347	rBV2	354	280	0.02%	0.003%
45	8.706	2377	2384	2389	rBV2	202	282	0.02%	0.003%
46	8.850	2418	2429	2459	rBV	544448	878709	61.98%	8.710%
47	9.018	2477	2481	2483	rBV	410	300	0.02%	0.003%
48	9.030	2483	2485	2489	rVB3	486	358	0.03%	0.004%
49	9.111	2507	2510	2515	rVV2	350	271	0.02%	0.003%
50	9.149	2515	2522	2531	rVV3	1138	1759	0.12%	0.017%
51	9.387	2590	2596	2599	rBV2	195	241	0.02%	0.002%
52	9.571	2647	2653	2654	rBV3	880	799	0.06%	0.008%
53	9.648	2673	2677	2682	rBV2	278	284	0.02%	0.003%
54	9.680	2682	2687	2693	rBV3	308	353	0.02%	0.003%
55	9.834	2732	2735	2740	rBV2	351	325	0.02%	0.003%
56	9.966	2773	2776	2780	rVB2	332	251	0.02%	0.002%
57	10.008	2780	2789	2793	rBV2	205	362	0.03%	0.004%
58	10.085	2810	2813	2817	rVB2	333	241	0.02%	0.002%
59	10.127	2817	2826	2840	rBV5	4032	6443	0.45%	0.064%
60	10.214	2841	2853	2872	rBV	377189	576719	40.68%	5.717%
61	10.461	2928	2930	2935	rBV	329	239	0.02%	0.002%
62	10.580	2958	2967	2972	rBV4	1001	1826	0.13%	0.018%
63	10.657	2986	2991	2994	rBV2	434	360	0.03%	0.004%
64	10.709	3000	3007	3012	rVB2	307	431	0.03%	0.004%
65	10.915	3063	3071	3082	rVB5	2275	3759	0.27%	0.037%
66	11.037	3100	3109	3114	rVB3	640	968	0.07%	0.010%
67	11.143	3136	3142	3152	rVB5	1246	1977	0.14%	0.020%
68	11.246	3163	3174	3194	rBV	539362	829600	58.52%	8.223%
69	11.387	3213	3218	3224	rBV4	1333	1740	0.12%	0.017%
70	11.426	3224	3230	3240	rVB3	2218	3632	0.26%	0.036%
71	11.570	3269	3275	3278	rBV3	255	313	0.02%	0.003%
72	11.622	3279	3291	3313	rBV	606288	932309	65.76%	9.242%
73	11.783	3339	3341	3346	rVB3	825	632	0.04%	0.006%
74	11.844	3356	3360	3361	rBV2	361	226	0.02%	0.002%
75	11.886	3370	3373	3378	rBV2	268	295	0.02%	0.003%
76	12.046	3420	3423	3428	rBV2	278	246	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024962.D
 Acq On : 11 Mar 2022 14:11
 Operator : SY/MD
 Sample : N1880-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	12.072	3428	3431	3433	rVV2	285	211	0.01%	0.002%
78	12.091	3435	3437	3442	rVB4	525	412	0.03%	0.004%
79	12.236	3478	3482	3486	rBV2	211	209	0.01%	0.002%
80	12.352	3514	3518	3521	rBV2	388	343	0.02%	0.003%
81	12.599	3592	3595	3600	rVB3	265	244	0.02%	0.002%
82	13.043	3729	3733	3737	rBV	266	245	0.02%	0.002%
83	13.143	3759	3764	3768	rVB2	338	319	0.02%	0.003%
84	13.262	3795	3801	3811	rBV2	329	509	0.04%	0.005%
85	13.304	3811	3814	3819	rBV2	199	216	0.02%	0.002%
86	13.403	3841	3845	3853	rVB2	220	270	0.02%	0.003%
87	13.451	3857	3860	3867	rVB2	214	234	0.02%	0.002%
88	13.660	3921	3925	3927	rBV2	263	208	0.01%	0.002%
89	13.770	3954	3959	3966	rVB2	318	417	0.03%	0.004%
90	13.882	3990	3994	3997	rVB2	342	267	0.02%	0.003%
91	13.898	3997	3999	4001	rBV2	387	231	0.02%	0.002%
92	14.033	4035	4041	4044	rBV2	249	290	0.02%	0.003%
93	14.114	4062	4066	4069	rBV	273	244	0.02%	0.002%
94	14.223	4097	4100	4104	rVB2	430	318	0.02%	0.003%
95	14.548	4194	4201	4208	rBV3	492	766	0.05%	0.008%
96	14.586	4208	4213	4216	rBV2	378	364	0.03%	0.004%
97	15.210	4404	4407	4409	rBV	319	219	0.02%	0.002%
98	15.757	4575	4577	4581	rVB	609	360	0.03%	0.004%
99	15.879	4613	4615	4620	rVB2	673	456	0.03%	0.005%
100	15.902	4620	4622	4625	rBV2	499	346	0.02%	0.003%




Sum of corrected areas: 10088245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

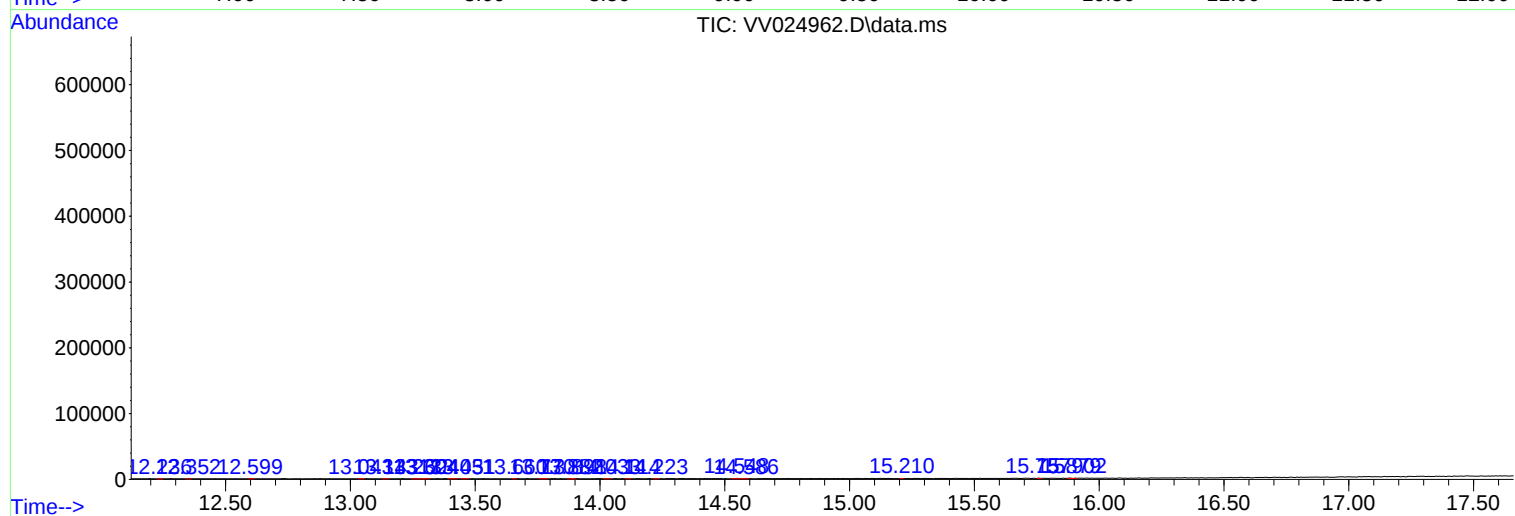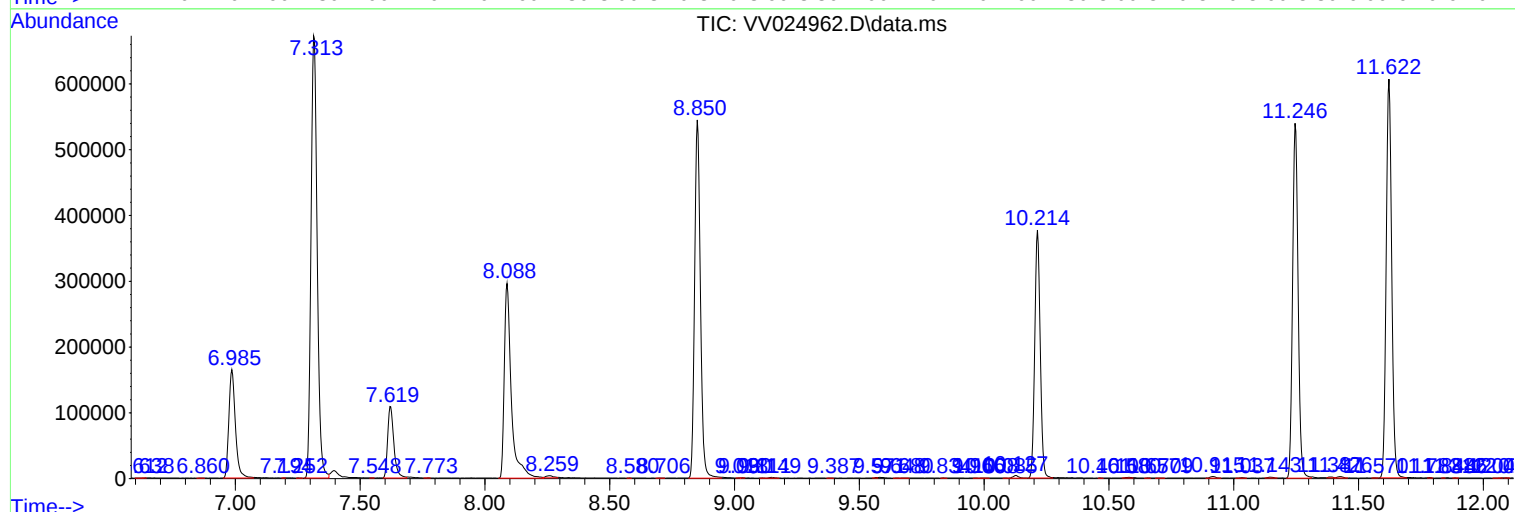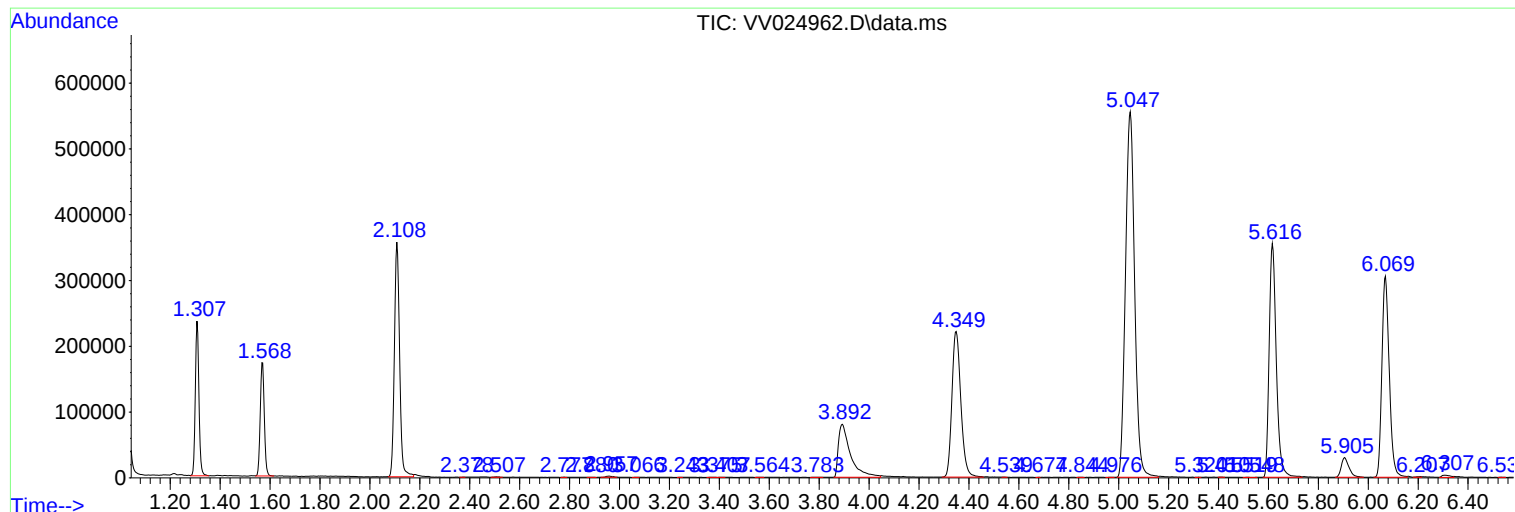

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.905	4.45 ug/L	63037	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethylene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	38
2			Propanoic acid, 2,2,3-trichloro-...	190	C4H5Cl3O2	004749-35-3	37
3			4-Chloro-3-fluoropyridine	131	C5H3ClFN	002546-56-7	32
4			Ethane, 1,1,1,2-tetrachloro-	166	C2H2Cl4	000630-20-6	25
5			Dihydro-4,5-dichloro-2(3H)furanone	154	C4H4Cl2O2	114434-99-0	25

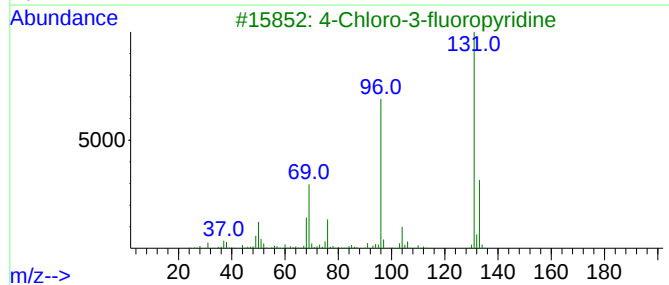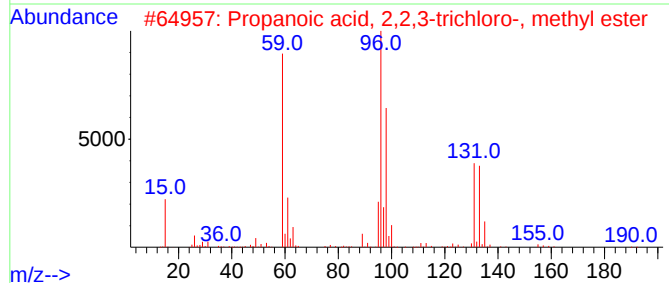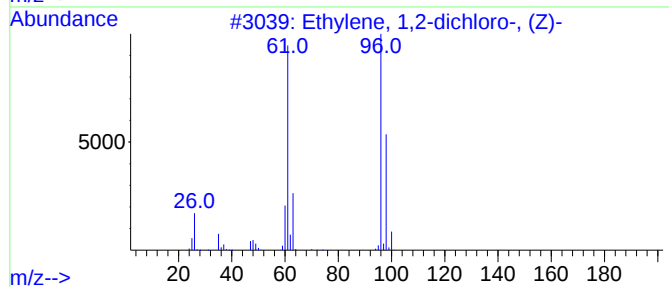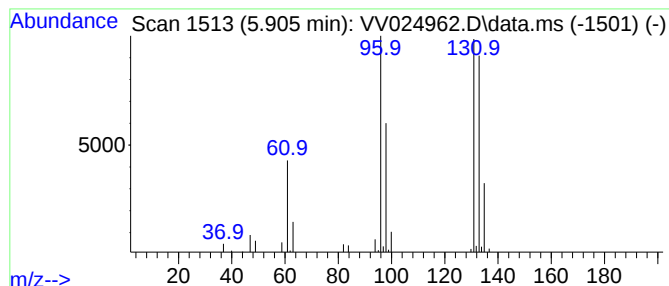

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024962.D
Acq On : 11 Mar 2022 14:11
Operator : SY/MD
Sample : N1880-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	5.905	4.5	ug/L	63037	1	5.616	707777	50.0