

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024970.D
 Acq On : 11 Mar 2022 17:44
 Operator : SY/MD
 Sample : N1880-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	224126	227284	15.99%	2.088%
2	1.568	157	164	178	rVB	169736	189706	13.35%	1.743%
3	2.108	321	332	371	rVB2	366944	554843	39.04%	5.098%
4	2.670	504	507	512	rBV2	192	205	0.01%	0.002%
5	2.918	580	584	586	rBV	178	151	0.01%	0.001%
6	3.072	626	632	633	rBV2	168	160	0.01%	0.001%
7	3.105	640	642	645	rBV2	136	101	0.01%	0.001%
8	3.143	651	654	656	rBV	197	135	0.01%	0.001%
9	3.548	777	780	783	rBV2	220	145	0.01%	0.001%
10	3.680	818	821	829	rBV2	218	250	0.02%	0.002%
11	3.857	870	876	877	rBV	202	203	0.01%	0.002%
12	3.899	877	889	934	rBV	85650	314254	22.11%	2.887%
13	4.349	1011	1029	1057	rBV	224338	554555	39.02%	5.095%
14	4.616	1098	1112	1130	rVB3	4739	11684	0.82%	0.107%
15	4.831	1177	1179	1182	rBV2	260	142	0.01%	0.001%
16	4.950	1214	1216	1218	rBV	269	151	0.01%	0.001%
17	5.047	1226	1246	1289	rBV2	557292	1421241	100.00%	13.058%
18	5.410	1352	1359	1363	rBV3	368	517	0.04%	0.005%
19	5.484	1380	1382	1386	rBV2	197	121	0.01%	0.001%
20	5.506	1386	1389	1392	rVB2	311	174	0.01%	0.002%
21	5.555	1402	1404	1408	rBV2	230	153	0.01%	0.001%
22	5.616	1408	1423	1453	rBV	343786	683440	48.09%	6.280%
23	5.911	1502	1515	1541	rBV2	441503	887684	62.46%	8.156%
24	6.069	1551	1564	1600	rVB	311920	629529	44.29%	5.784%
25	6.281	1627	1630	1632	rBV2	187	141	0.01%	0.001%
26	6.365	1655	1656	1658	rBV	104	24	0.00%	0.000%
27	6.407	1666	1669	1672	rBV	181	113	0.01%	0.001%
28	6.471	1686	1689	1693	rBV2	168	124	0.01%	0.001%
29	6.510	1698	1701	1704	rBV	177	122	0.01%	0.001%
30	6.542	1709	1711	1714	rVB2	177	84	0.01%	0.001%
31	6.558	1714	1716	1717	rBV	261	96	0.01%	0.001%
32	6.567	1717	1719	1721	rVB2	177	75	0.01%	0.001%
33	6.648	1737	1744	1748	rBV4	622	719	0.05%	0.007%
34	6.751	1772	1776	1779	rBV	331	267	0.02%	0.002%
35	6.767	1779	1781	1784	rVV2	148	107	0.01%	0.001%
36	6.882	1813	1817	1819	rBV2	136	96	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW031122\
 Data File : VW024970.D
 Acq On : 11 Mar 2022 17:44
 Operator : SY/MD
 Sample : N1880-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.985	1837	1849	1874	rBV	162683	295883	20.82%	2.719%
38	7.313	1939	1951	1970	rBV	666413	1148804	80.83%	10.555%
39	7.622	2037	2047	2070	rBV	108639	185286	13.04%	1.702%
40	7.876	2123	2126	2128	rBV	203	131	0.01%	0.001%
41	8.014	2165	2169	2172	rBV	304	231	0.02%	0.002%
42	8.088	2179	2192	2229	rBV	308432	591875	41.64%	5.438%
43	8.320	2261	2264	2265	rBV2	298	147	0.01%	0.001%
44	8.464	2307	2309	2313	rVB2	192	76	0.01%	0.001%
45	8.487	2313	2316	2317	rBV2	175	102	0.01%	0.001%
46	8.619	2352	2357	2362	rBV4	602	546	0.04%	0.005%
47	8.661	2368	2370	2375	rBV2	209	144	0.01%	0.001%
48	8.796	2405	2412	2415	rBV	229	190	0.01%	0.002%
49	8.812	2415	2417	2418	rBV	110	51	0.00%	0.000%
50	8.850	2418	2429	2454	rBV	529802	845863	59.52%	7.772%
51	9.024	2482	2483	2488	rBV3	282	196	0.01%	0.002%
52	9.226	2543	2546	2547	rBV	93	56	0.00%	0.001%
53	9.278	2557	2562	2563	rBV	172	152	0.01%	0.001%
54	9.487	2624	2627	2630	rBV2	212	161	0.01%	0.001%
55	9.577	2652	2655	2657	rBV2	192	116	0.01%	0.001%
56	9.596	2657	2661	2664	rVV	408	302	0.02%	0.003%
57	9.747	2702	2708	2711	rBV2	140	158	0.01%	0.001%
58	10.127	2818	2826	2841	rVB3	3460	4762	0.34%	0.044%
59	10.214	2841	2853	2873	rBV	388284	602298	42.38%	5.534%
60	10.381	2901	2905	2911	rVB3	704	745	0.05%	0.007%
61	10.570	2959	2964	2965	rBV	802	699	0.05%	0.006%
62	10.657	2989	2991	2996	rVB2	433	301	0.02%	0.003%
63	10.889	3061	3063	3064	rBV	275	121	0.01%	0.001%
64	10.914	3064	3071	3081	rVB6	2089	3203	0.23%	0.029%
65	11.120	3130	3135	3136	rBV2	320	256	0.02%	0.002%
66	11.146	3137	3143	3149	rVB3	1364	1898	0.13%	0.017%
67	11.246	3163	3174	3205	rBV	512024	793126	55.81%	7.287%
68	11.426	3225	3230	3239	rVB3	2162	2924	0.21%	0.027%
69	11.622	3279	3291	3314	rBV	584476	921261	64.82%	8.465%
70	11.786	3338	3342	3347	rVB4	684	491	0.03%	0.005%
71	11.840	3357	3359	3362	rBV3	462	300	0.02%	0.003%
72	12.046	3420	3423	3426	rBV2	142	105	0.01%	0.001%
73	12.082	3426	3434	3436	rBV2	401	457	0.03%	0.004%
74	12.249	3483	3486	3490	rBV	371	347	0.02%	0.003%
75	12.593	3589	3593	3595	rBV2	365	318	0.02%	0.003%
76	12.664	3611	3615	3619	rBV2	318	326	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024970.D
Acq On : 11 Mar 2022 17:44
Operator : SY/MD
Sample : N1880-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Title : VOC Analysis

77	13.210	3782	3785	3788	rBV	217	142	0.01%	0.001%
78	13.619	3910	3912	3914	rBV2	273	153	0.01%	0.001%
79	14.040	4040	4043	4047	rBV2	253	149	0.01%	0.001%




Sum of corrected areas: 10883648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024970.D
Acq On : 11 Mar 2022 17:44
Operator : SY/MD
Sample : N1880-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

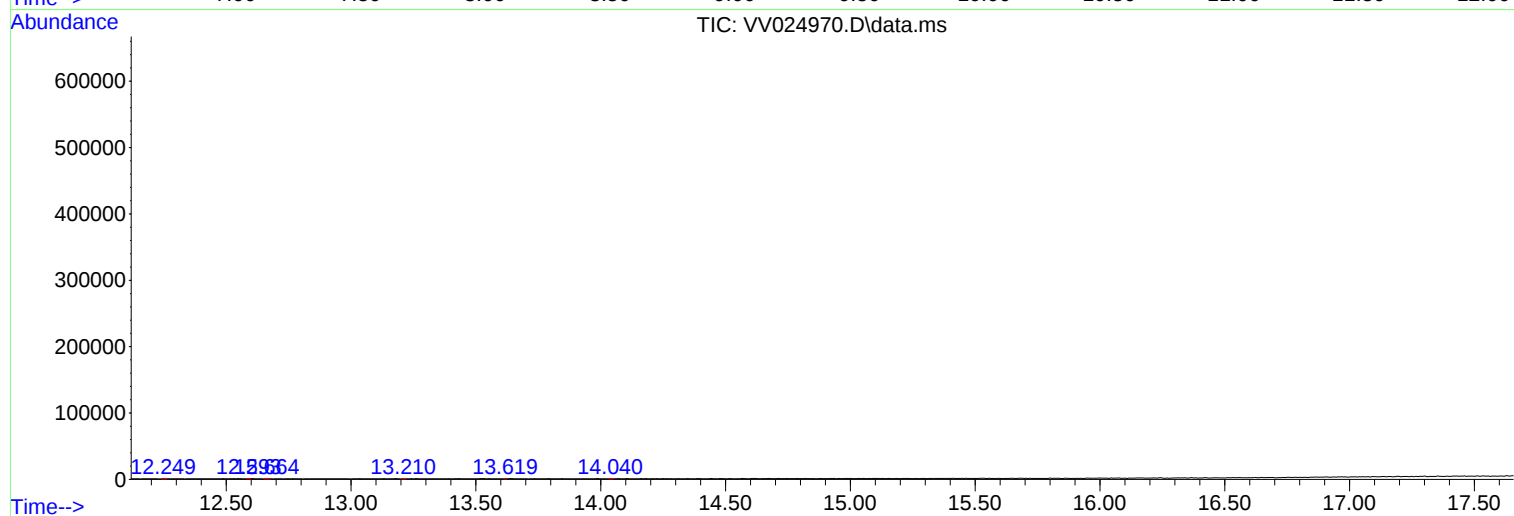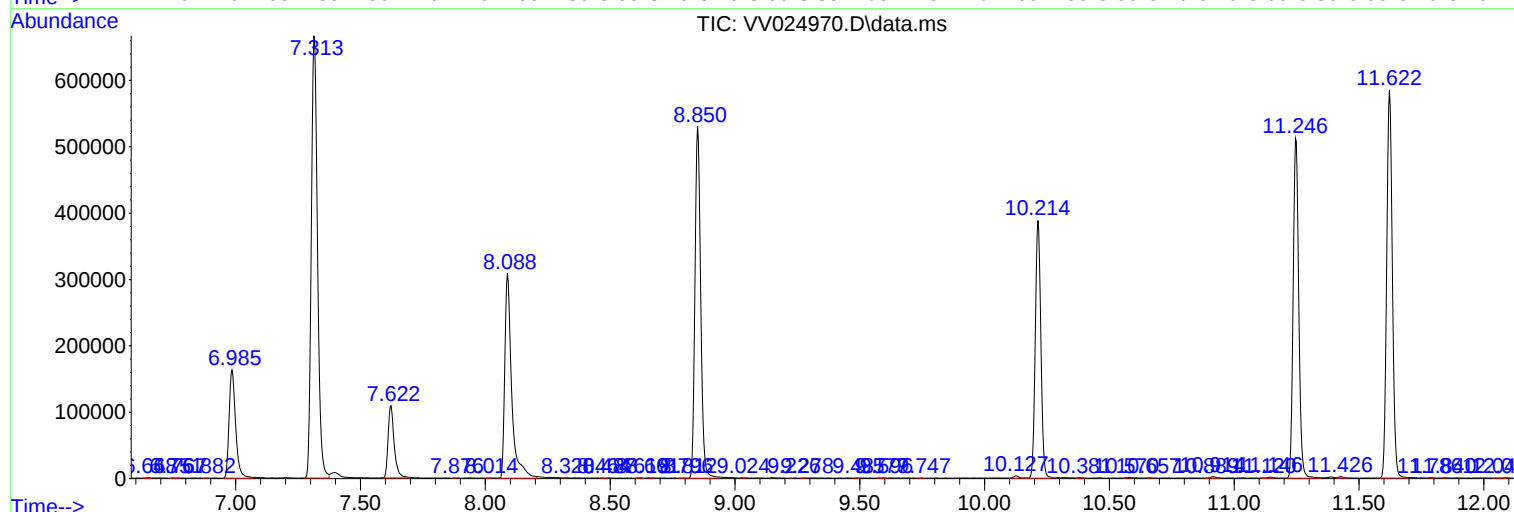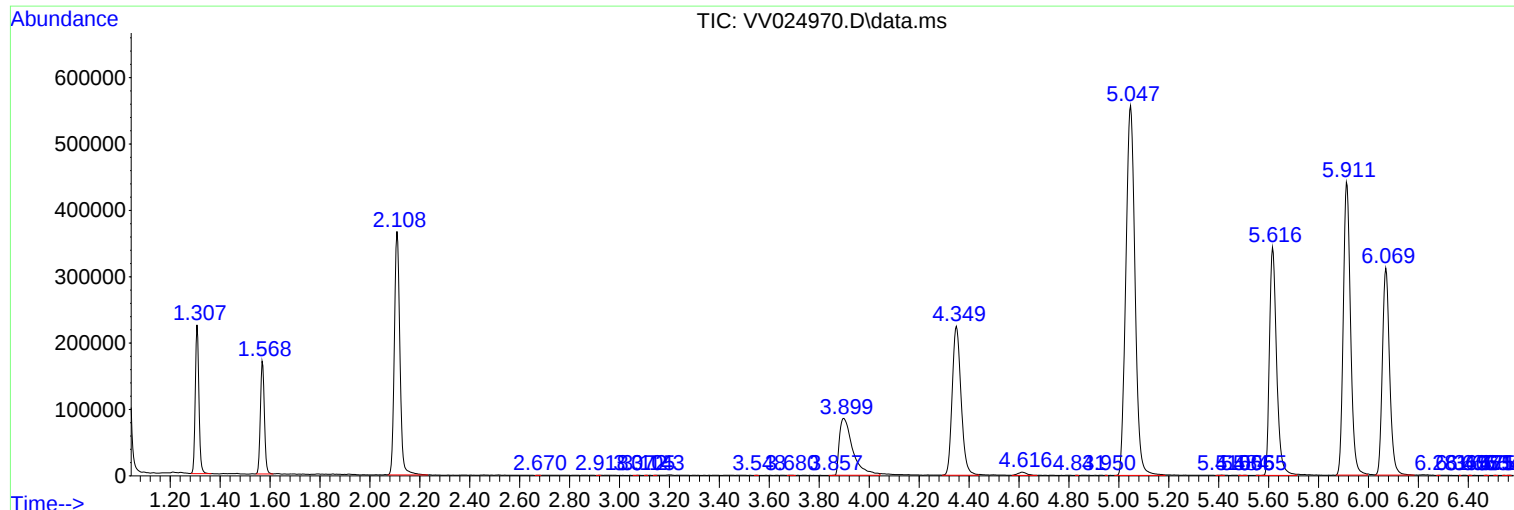

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024970.D
Acq On : 11 Mar 2022 17:44
Operator : SY/MD
Sample : N1880-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024970.D
Acq On : 11 Mar 2022 17:44
Operator : SY/MD
Sample : N1880-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------