

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024972.D
 Acq On : 11 Mar 2022 18:32
 Operator : SY/MD
 Sample : N1880-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

Signal : TIC: VV024972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	212898	212931	16.14%	2.115%
2	1.568	156	164	179	rVB	160291	182474	13.83%	1.812%
3	2.108	321	332	349	rBV2	335761	499783	37.88%	4.963%
4	2.349	402	407	413	rVB2	246	260	0.02%	0.003%
5	2.397	418	422	429	rVB3	341	464	0.04%	0.005%
6	2.439	432	435	436	rBV	392	236	0.02%	0.002%
7	2.500	450	454	456	rBV2	547	420	0.03%	0.004%
8	2.716	514	521	523	rBV2	204	221	0.02%	0.002%
9	2.870	566	569	576	rVB2	211	224	0.02%	0.002%
10	2.947	590	593	598	rVB2	253	213	0.02%	0.002%
11	3.037	615	621	626	rBV2	201	234	0.02%	0.002%
12	3.185	662	667	669	rBV3	295	300	0.02%	0.003%
13	3.201	669	672	679	rVB3	462	483	0.04%	0.005%
14	3.310	700	706	711	rVB2	307	432	0.03%	0.004%
15	3.339	711	715	718	rBV2	275	234	0.02%	0.002%
16	3.542	771	778	782	rBV2	196	272	0.02%	0.003%
17	3.732	832	837	841	rBV2	282	359	0.03%	0.004%
18	3.896	877	888	932	rBV2	78429	288448	21.86%	2.864%
19	4.191	977	980	984	rVB	333	240	0.02%	0.002%
20	4.349	1012	1029	1064	rBV	210088	516979	39.18%	5.134%
21	4.529	1081	1085	1087	rVB2	302	207	0.02%	0.002%
22	4.613	1097	1111	1127	rVB4	7510	18121	1.37%	0.180%
23	4.712	1139	1142	1145	rBV2	369	225	0.02%	0.002%
24	4.825	1174	1177	1182	rVB	257	209	0.02%	0.002%
25	4.944	1209	1214	1216	rBV2	272	234	0.02%	0.002%
26	5.047	1229	1246	1275	rBV2	520332	1319403	100.00%	13.102%
27	5.275	1314	1317	1322	rVB3	342	302	0.02%	0.003%
28	5.423	1360	1363	1366	rBV3	405	258	0.02%	0.003%
29	5.500	1382	1387	1394	rVB2	156	215	0.02%	0.002%
30	5.561	1402	1406	1410	rVB2	418	373	0.03%	0.004%
31	5.616	1410	1423	1446	rBV	343122	689717	52.27%	6.849%
32	5.912	1502	1515	1546	rBV2	300240	616890	46.76%	6.126%
33	6.069	1551	1564	1594	rVV	285021	579452	43.92%	5.754%
34	6.217	1608	1610	1612	rVB2	564	222	0.02%	0.002%
35	6.240	1612	1617	1619	rVB3	410	323	0.02%	0.003%
36	6.294	1630	1634	1637	rVB2	262	222	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024972.D
 Acq On : 11 Mar 2022 18:32
 Operator : SY/MD
 Sample : N1880-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

37	6.513	1696	1702	1706	rBV2	266	341	0.03%	0.003%
38	6.564	1712	1718	1723	rVV2	238	285	0.02%	0.003%
39	6.641	1738	1742	1746	rBV2	188	241	0.02%	0.002%
40	6.805	1784	1793	1798	rBV	344	474	0.04%	0.005%
41	6.857	1805	1809	1815	rVB2	340	316	0.02%	0.003%
42	6.986	1838	1849	1881	rVV	152769	275765	20.90%	2.739%
43	7.198	1909	1915	1919	rBV5	570	625	0.05%	0.006%
44	7.313	1938	1951	1971	rBV	615709	1061946	80.49%	10.546%
45	7.622	2037	2047	2073	rVV	98389	173539	13.15%	1.723%
46	7.757	2087	2089	2093	rVB2	463	257	0.02%	0.003%
47	7.931	2136	2143	2144	rBV2	304	290	0.02%	0.003%
48	7.947	2144	2148	2155	rVB3	478	523	0.04%	0.005%
49	8.040	2172	2177	2182	rVB2	223	221	0.02%	0.002%
50	8.088	2182	2192	2232	rBV	275447	537538	40.74%	5.338%
51	8.436	2297	2300	2304	rVB3	229	204	0.02%	0.002%
52	8.477	2311	2313	2322	rVV2	274	276	0.02%	0.003%
53	8.555	2331	2337	2342	rVB3	306	366	0.03%	0.004%
54	8.764	2398	2402	2404	rBV	226	199	0.02%	0.002%
55	8.850	2417	2429	2457	rBV	540294	863252	65.43%	8.573%
56	9.018	2477	2481	2490	rVB2	427	493	0.04%	0.005%
57	9.159	2520	2525	2535	rVB3	509	802	0.06%	0.008%
58	9.252	2547	2554	2557	rBV2	338	309	0.02%	0.003%
59	9.365	2583	2589	2592	rBV2	352	369	0.03%	0.004%
60	9.551	2643	2647	2652	rBV2	275	250	0.02%	0.002%
61	9.940	2762	2768	2773	rBV2	242	226	0.02%	0.002%
62	10.127	2817	2826	2834	rVB2	3026	4130	0.31%	0.041%
63	10.214	2841	2853	2875	rBV	356423	553468	41.95%	5.496%
64	10.381	2900	2905	2908	rBV2	564	635	0.05%	0.006%
65	10.580	2960	2967	2973	rBV4	1010	1366	0.10%	0.014%
66	10.741	3009	3017	3020	rBV2	266	252	0.02%	0.003%
67	10.857	3050	3053	3058	rBV2	222	251	0.02%	0.002%
68	10.918	3064	3072	3084	rVB5	2208	3241	0.25%	0.032%
69	11.034	3102	3108	3117	rBV3	574	724	0.05%	0.007%
70	11.072	3117	3120	3124	rVB	375	265	0.02%	0.003%
71	11.101	3124	3129	3131	rBV	337	273	0.02%	0.003%
72	11.143	3136	3142	3154	rBV4	837	1485	0.11%	0.015%
73	11.246	3163	3174	3198	rBV	530100	803302	60.88%	7.977%
74	11.426	3225	3230	3238	rVB5	1660	2242	0.17%	0.022%
75	11.622	3279	3291	3310	rBV	545980	840116	63.67%	8.343%
76	11.898	3372	3377	3383	rVB2	207	264	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024972.D
 Acq On : 11 Mar 2022 18:32
 Operator : SY/MD
 Sample : N1880-10
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0DC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis

77	11.937	3383	3389	3393	rVB2	213	233	0.02%	0.002%
78	11.992	3398	3406	3412	rBV2	285	575	0.04%	0.006%
79	12.043	3415	3422	3425	rBV2	241	294	0.02%	0.003%
80	12.088	3433	3436	3442	rVB3	321	306	0.02%	0.003%
81	12.349	3515	3517	3525	rVB2	290	298	0.02%	0.003%
82	12.577	3585	3588	3593	rBV2	266	267	0.02%	0.003%
83	12.603	3593	3596	3606	rVB2	214	302	0.02%	0.003%
84	12.670	3613	3617	3621	rBV	296	221	0.02%	0.002%
85	12.812	3655	3661	3665	rBV2	203	294	0.02%	0.003%
86	13.014	3721	3724	3730	rVB	310	255	0.02%	0.003%
87	13.098	3742	3750	3755	rBV2	254	322	0.02%	0.003%
88	13.378	3835	3837	3844	rVB2	323	273	0.02%	0.003%
89	13.763	3954	3957	3963	rBV2	192	247	0.02%	0.002%
90	14.082	4053	4056	4058	rBV2	282	220	0.02%	0.002%
91	14.345	4136	4138	4145	rVB2	319	281	0.02%	0.003%
92	14.381	4145	4149	4152	rBV	300	292	0.02%	0.003%
93	14.419	4157	4161	4163	rBV3	297	214	0.02%	0.002%
94	14.439	4163	4167	4170	rVB2	430	316	0.02%	0.003%
95	14.484	4176	4181	4189	rVV2	398	568	0.04%	0.006%
96	14.677	4238	4241	4245	rBV	261	235	0.02%	0.002%
97	14.959	4326	4329	4331	rBV2	461	326	0.02%	0.003%
98	15.516	4498	4502	4504	rBV2	360	285	0.02%	0.003%
99	15.924	4626	4629	4631	rBV3	473	230	0.02%	0.002%
100	16.024	4657	4660	4664	rVB3	578	338	0.03%	0.003%




Sum of corrected areas: 10069893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024972.D
Acq On : 11 Mar 2022 18:32
Operator : SY/MD
Sample : N1880-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

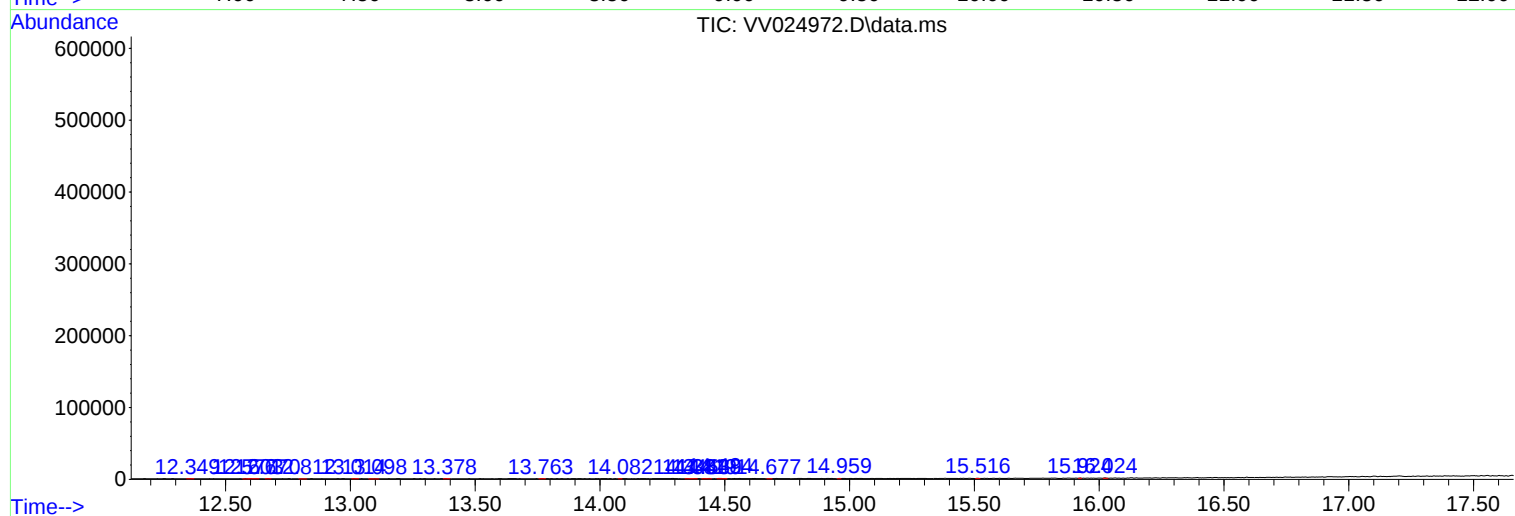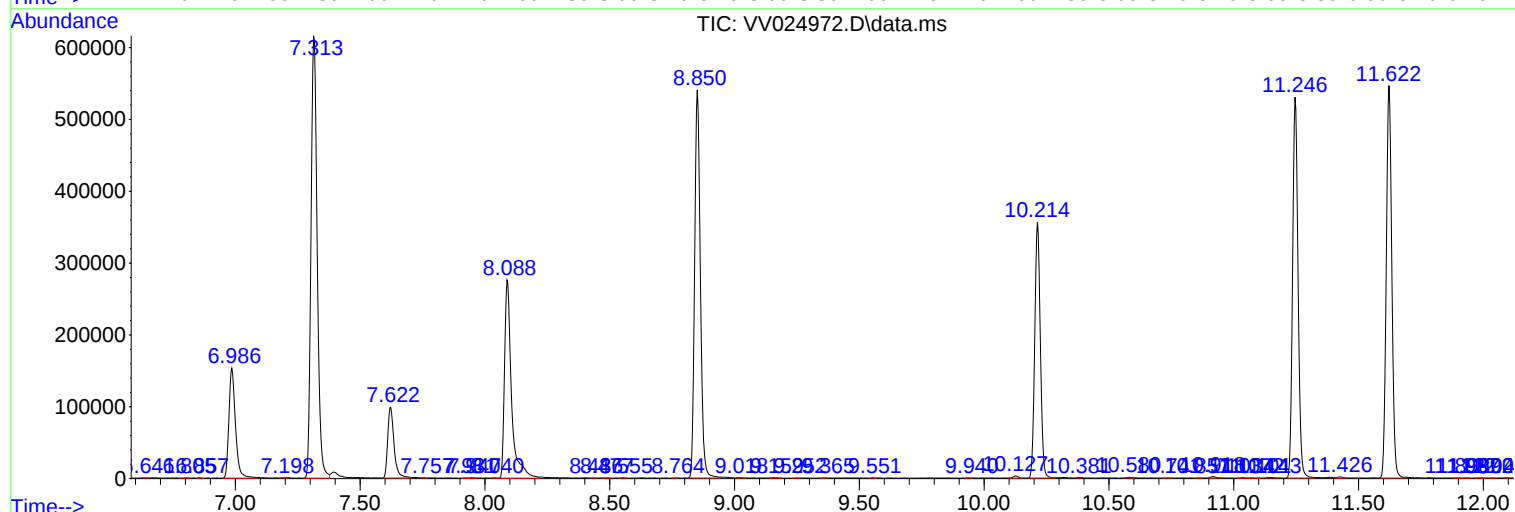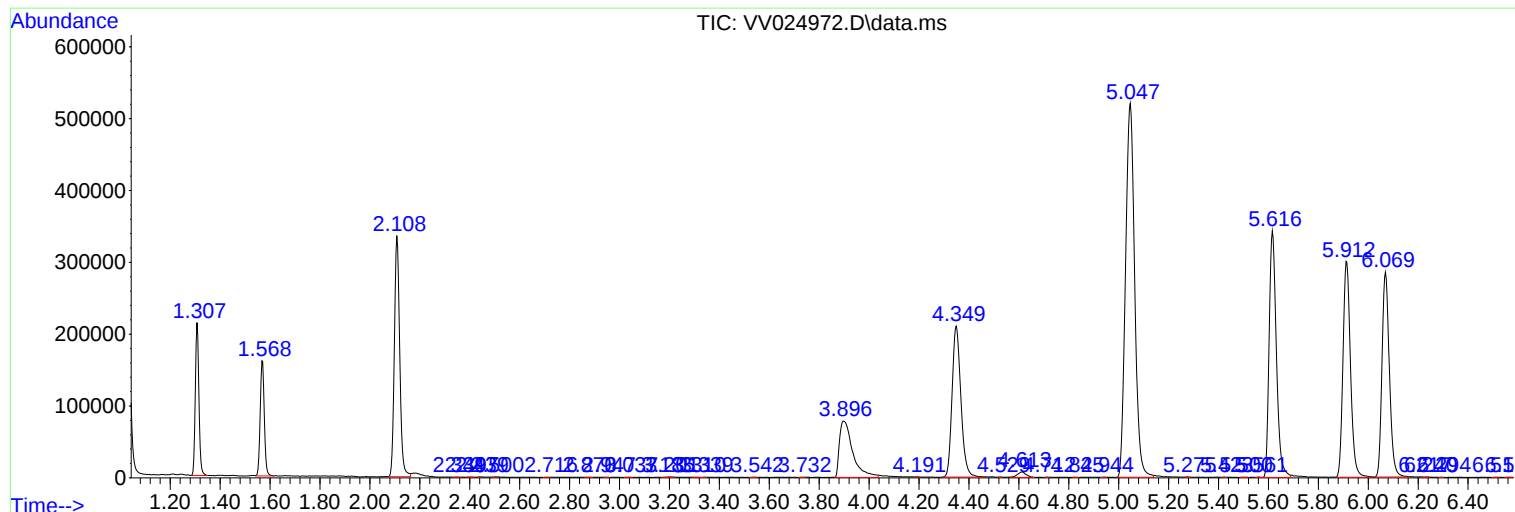

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024972.D
Acq On : 11 Mar 2022 18:32
Operator : SY/MD
Sample : N1880-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
Data File : VV024972.D
Acq On : 11 Mar 2022 18:32
Operator : SY/MD
Sample : N1880-10
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0DC2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc