


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031122\
 Data File : VV024952.D
 Acq On : 11 Mar 2022 08:40
 Operator : SY/MD
 Sample : BFB204
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB204

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022822WMA.M
 Title : VOC Analysis
 Last Update : Tue Mar 15 02:18:50 2022

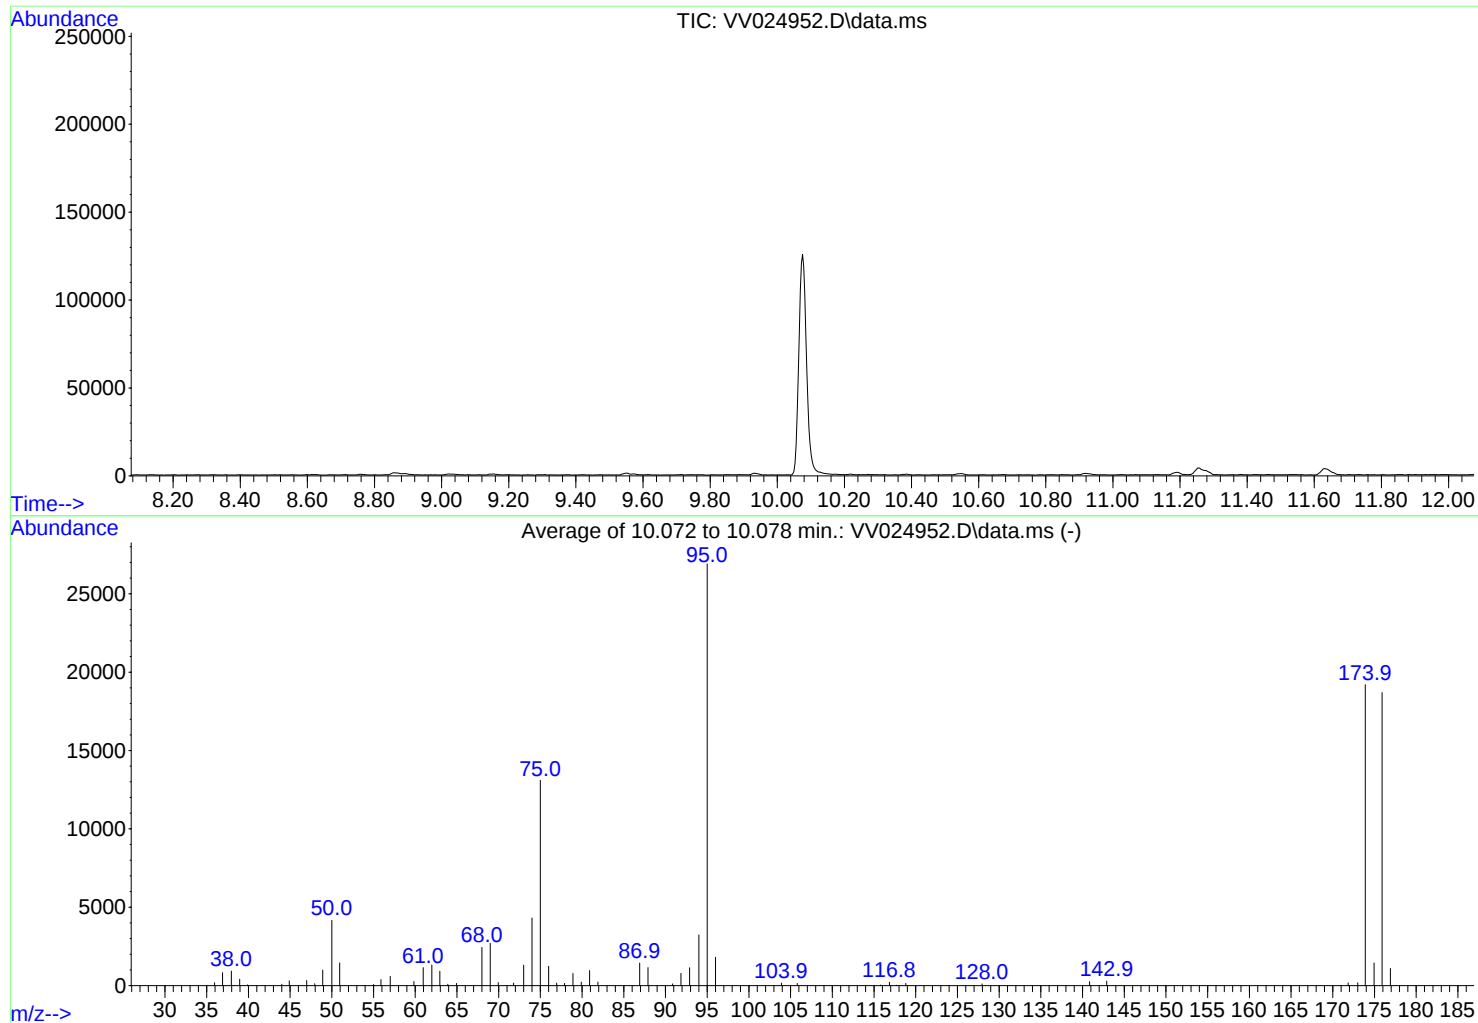

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	4165	PASS
75	95	30	80	48.7	13095	PASS
95	95	100	100	100.0	26909	PASS
96	95	5	9	6.7	1805	PASS
173	174	0.00	2	1.0	184	PASS
174	95	50	120	71.4	19205	PASS
175	174	5	9	7.6	1451	PASS
176	174	95	105	97.4	18701	PASS
177	176	5	10	5.8	1088	PASS

m/z	Abundance
39.90	347.0
44.00	236.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
36.00	174.0
36.90	849.0
37.90	940.0
38.90	397.0
39.90	425.0
44.00	358.0
44.90	333.0
47.00	336.0
47.90	133.0
48.90	1028.0
50.00	4047.0
51.00	1431.0
55.90	382.0
57.00	601.0
59.80	257.0
60.90	1184.0
62.00	1212.0
63.00	992.0
64.90	121.0
68.00	2424.0
69.00	2637.0
69.90	196.0
71.80	207.0
73.00	1334.0
74.00	4444.0
75.00	13265.0
76.00	1263.0
77.00	184.0
77.90	122.0
78.90	756.0
79.90	250.0
80.90	1007.0
81.90	252.0
86.90	1437.0
87.90	1266.0
90.80	114.0
91.80	807.0
92.90	1176.0
94.00	3155.0
95.00	27024.0
96.00	1911.0
103.90	151.0
105.80	150.0
116.80	210.0
118.90	132.0
128.00	109.0
140.80	256.0
142.90	307.0
172.00	180.0
173.00	188.0
173.90	18456.0
175.00	1466.0
175.90	18000.0
176.90	1010.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
36.00	188.0
36.90	832.0
38.00	947.0
39.00	419.0
39.90	407.0
44.00	325.0
44.90	326.0
47.00	344.0
47.90	130.0
48.90	1025.0
50.00	4355.0
51.00	1520.0
55.00	100.0
55.90	403.0
57.00	617.0
59.80	271.0
61.00	1210.0
62.00	1370.0
63.00	929.0
63.90	123.0
64.90	140.0
68.00	2529.0
69.00	2744.0
70.00	205.0
71.80	181.0
73.00	1335.0
74.00	4417.0
75.00	13465.0
76.00	1283.0
77.00	178.0
77.90	154.0
78.90	807.0
79.90	227.0
80.90	1010.0
81.90	242.0
86.90	1504.0
87.90	1186.0
90.90	107.0
91.90	839.0
92.90	1196.0
94.00	3328.0
95.00	27760.0
96.00	1861.0
103.90	167.0
105.80	143.0
116.90	218.0
117.70	105.0
118.80	138.0
127.90	116.0
140.90	261.0
142.90	289.0
171.80	176.0
173.00	180.0
173.90	19744.0
174.90	1515.0
175.90	19304.0
176.90	1095.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204

m/z	Abundance
35.90	205.0
36.90	811.0
38.00	898.0
39.00	409.0
39.90	369.0
44.00	299.0
44.90	253.0
47.00	316.0
48.00	112.0
48.90	909.0
50.00	4093.0
50.90	1383.0
55.00	111.0
55.90	384.0
57.00	566.0
59.90	279.0
60.90	1064.0
62.00	1359.0
62.90	825.0
63.90	157.0
65.00	162.0
68.00	2378.0
69.00	2697.0
69.90	187.0
71.90	113.0
73.00	1243.0
74.00	4089.0
75.00	12555.0
76.00	1153.0
76.90	141.0
77.90	160.0
78.90	776.0
79.90	189.0
80.90	867.0
81.90	195.0
86.90	1384.0
87.90	996.0
90.90	103.0
91.90	717.0
92.90	1060.0
94.00	3225.0
95.00	25944.0
96.00	1643.0
103.90	165.0
105.80	135.0
115.80	124.0
116.90	212.0
118.70	166.0
127.90	122.0
140.90	244.0
142.90	270.0
171.80	163.0
173.00	184.0
173.90	19416.0
174.90	1372.0
175.90	18800.0
176.90	1160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB204