

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034565.D
 Acq On : 13 Mar 2024 11:17
 Operator : SY/MD
 Sample : VV0313WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 14 02:22:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 14 02:21:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	319901	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	302121	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	146205	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	92595	33.389	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	66.780%
7) Chloroethane-d5	1.526	69	87632	40.561	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.120%
11) 1,1-Dichloroethene-d2	2.056	65	44152	35.204	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.400%
21) 2-Butanone-d5	3.777	46	202495	109.188	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	109.190%
24) Chloroform-d	4.246	84	221468	45.167	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.340%
26) 1,2-Dichloroethane-d4	4.937	65	154881	48.337	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.680%
32) Benzene-d6	4.957	84	396811	43.519	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.040%
36) 1,2-Dichloropropane-d6	5.986	67	135128	48.561	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.120%
41) Toluene-d8	7.240	98	337819	40.941	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.880%
43) trans-1,3-Dichloroprop...	7.551	79	59292	42.431	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.860%
47) 2-Hexanone-d5	8.018	63	148729	107.035	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	107.030%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	190057	51.901	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.800%
66) 1,2-Dichlorobenzene-d4	11.558	152	142170	47.573	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.140%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.185	75	17402	6.235	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034565.D
Acq On : 13 Mar 2024 11:17
Operator : SY/MD
Sample : VV0313WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Mar 14 02:22:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 14 02:21:30 2024
Response via : Initial Calibration

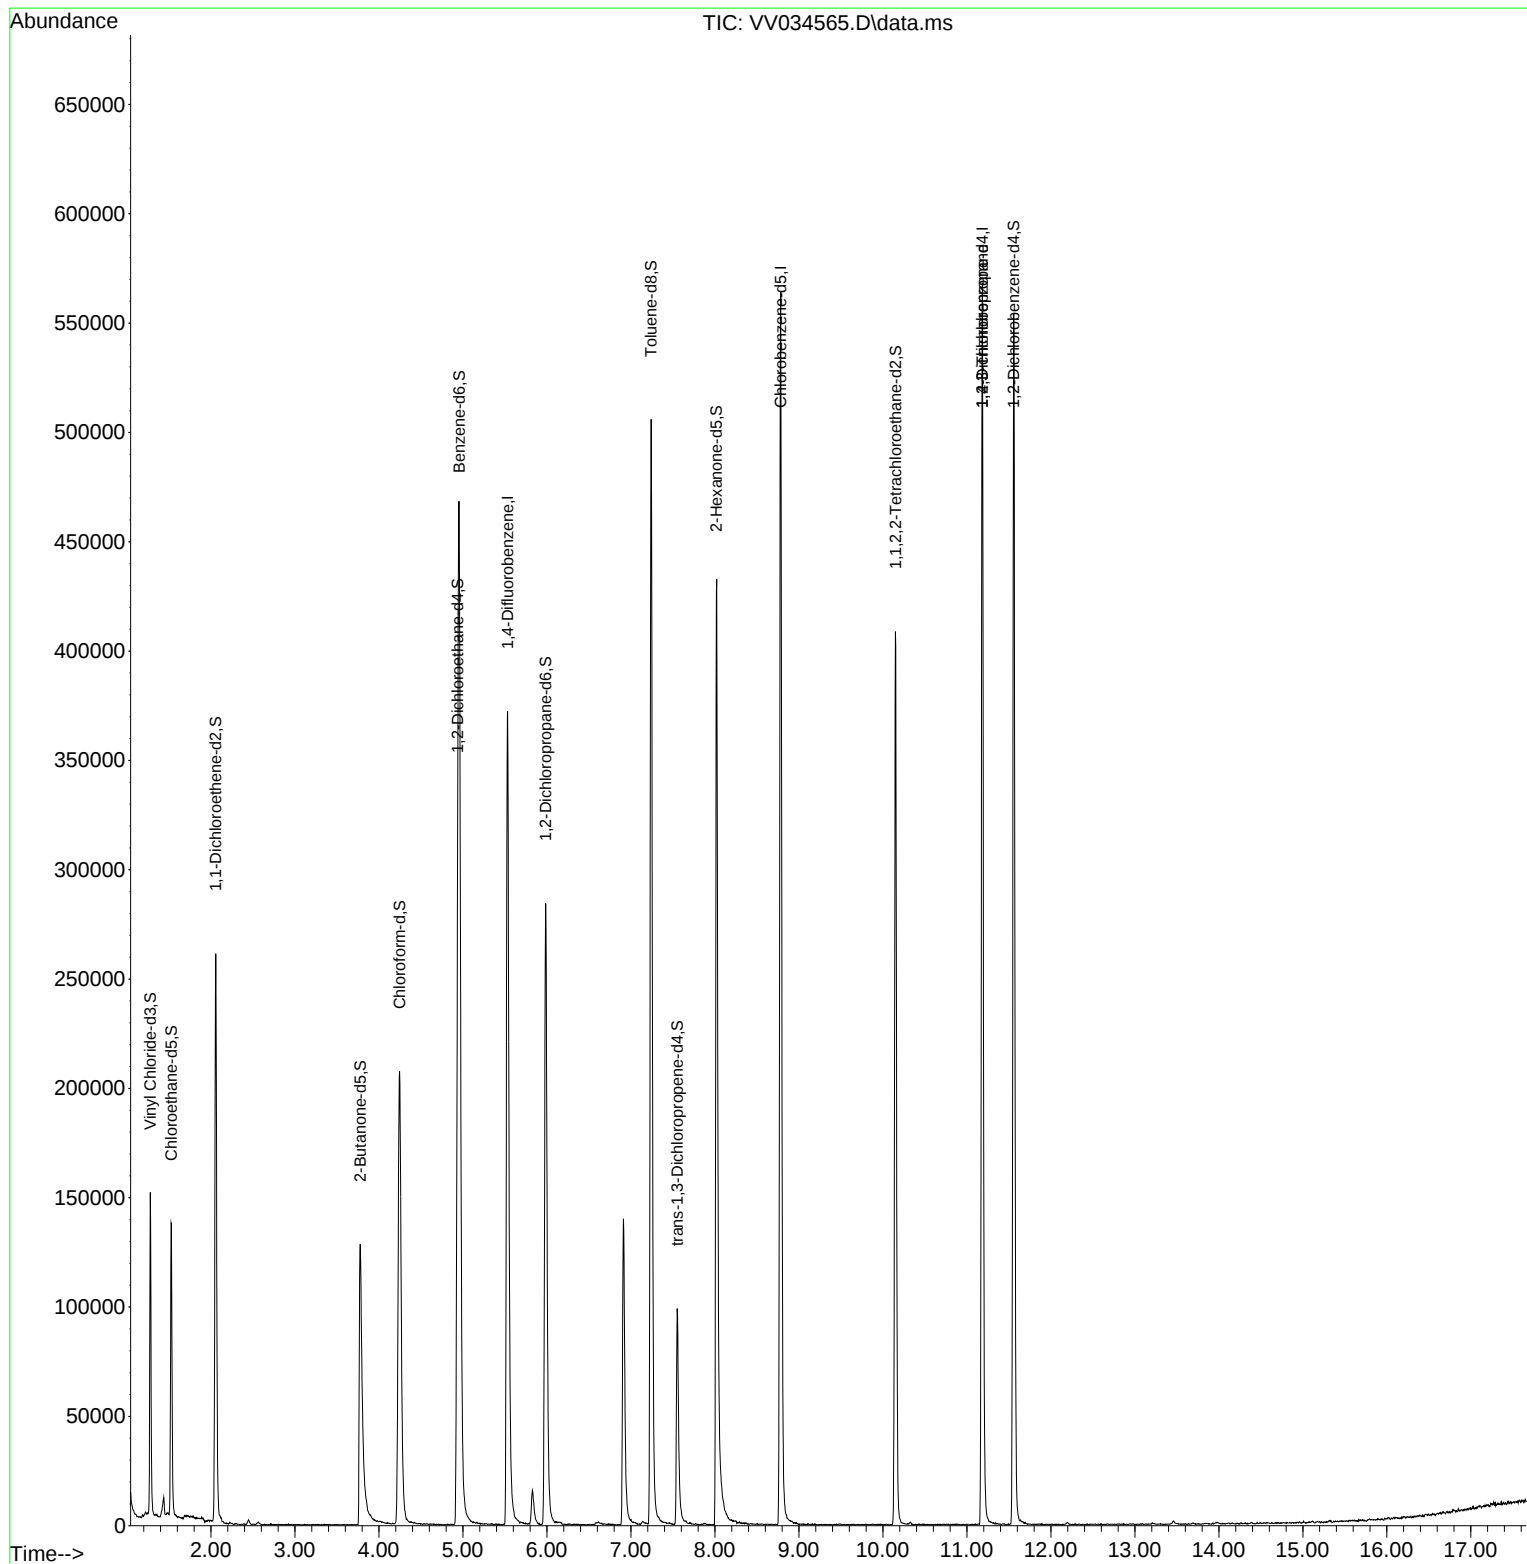

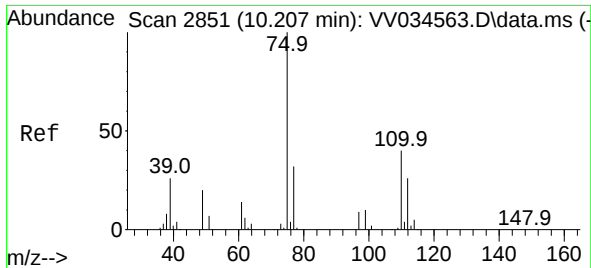

#61
 1,2,3-Trichloropropane
 Concen: 6.235 ug/L
 RT: 11.185 min Scan# 3155
 Delta R.T. 0.978 min
 Lab File: VV034565.D
 Acq: 13 Mar 2024 11:17

Instrument :
 MSVOA_V
 ClientSampleId :

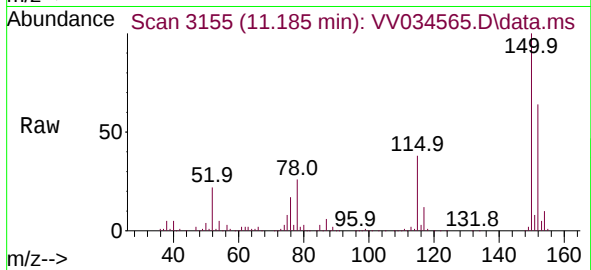

Tgt Ion: 75 Resp: 17402
 Ion Ratio Lower Upper
 75 100
 77 35.4 25.9 38.9
 110 3.0 33.1 49.7#

