

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034581.D
 Acq On : 13 Mar 2024 17:40
 Operator : SY/MD
 Sample : P1739-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Mar 14 02:26:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 14 02:21:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	310009	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	281996	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	134240	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	72772	27.078	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	54.160%#
7) Chloroethane-d5	1.532	69	72621	34.685	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	69.380%#
11) 1,1-Dichloroethene-d2	2.059	65	36695	30.192	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.380%
21) 2-Butanone-d5	3.793	46	205448	114.315	ug/L	0.01
Spiked Amount	100.000	Range	40 - 130	Recovery	=	114.320%
24) Chloroform-d	4.246	84	197394	41.542	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.080%
26) 1,2-Dichloroethane-d4	4.940	65	138329	44.549	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.100%
32) Benzene-d6	4.960	84	342877	40.288	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.580%
36) 1,2-Dichloropropane-d6	5.989	67	118141	45.486	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.980%
41) Toluene-d8	7.243	98	278914	36.214	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	72.420%#
43) trans-1,3-Dichloroprop...	7.554	79	49868	38.234	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.460%
47) 2-Hexanone-d5	8.024	63	141859	109.376	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.380%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	176034	51.502	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.000%
66) 1,2-Dichlorobenzene-d4	11.561	152	123043	44.842	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.680%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.185	75	16671	6.506	ug/L #	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034581.D
Acq On : 13 Mar 2024 17:40
Operator : SY/MD
Sample : P1739-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Mar 14 02:26:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 14 02:21:30 2024
Response via : Initial Calibration

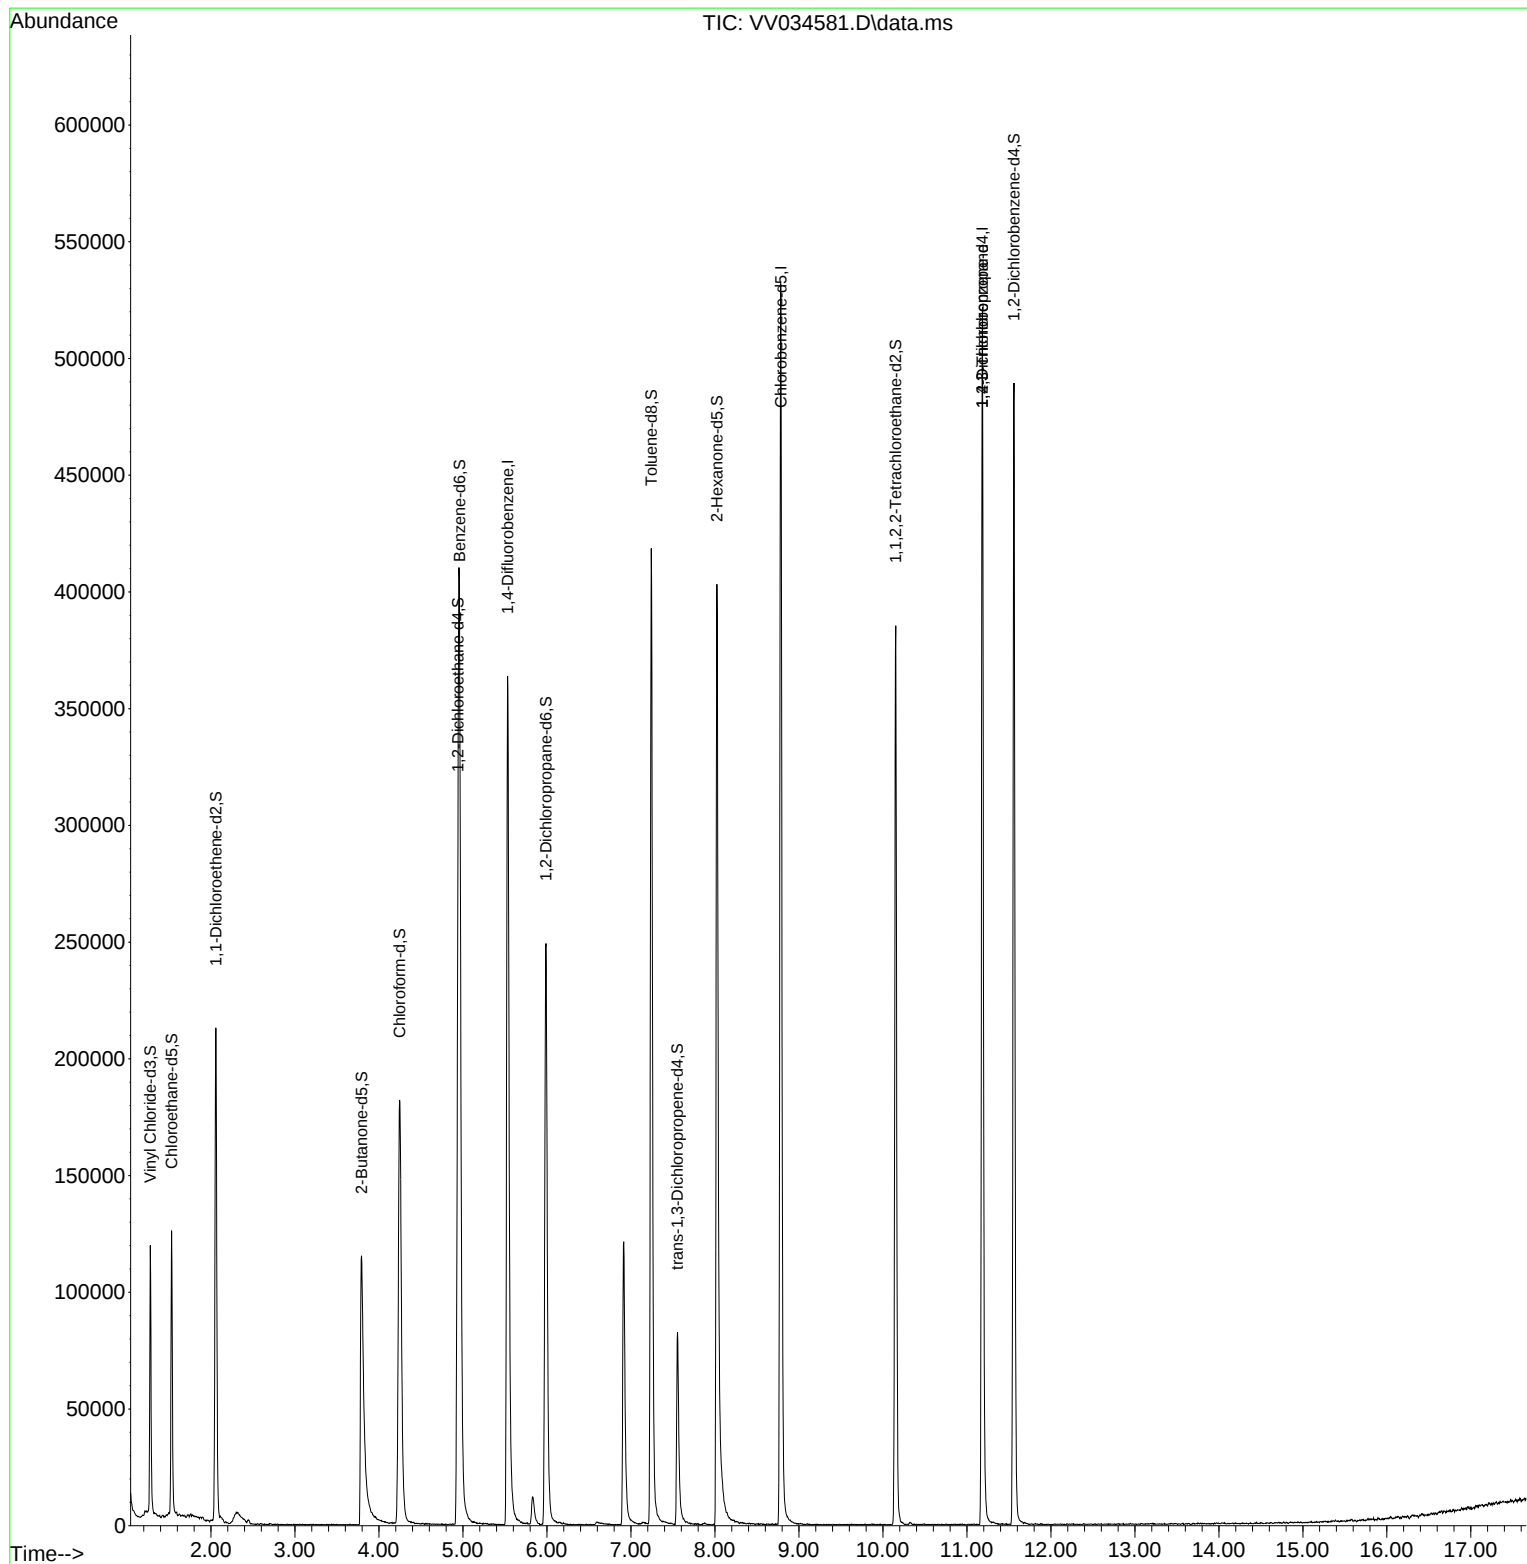

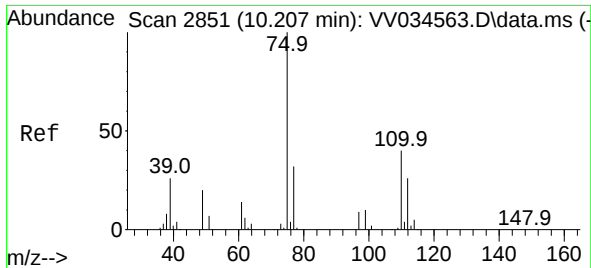

#61

1,2,3-Trichloropropane

Concen: 6.506 ug/L

RT: 11.185 min Scan# 31

Delta R.T. 0.977 min


Lab File: VV034581.D

Acq: 13 Mar 2024 17:40

Instrument :

MSVOA_V

ClientSampleId :

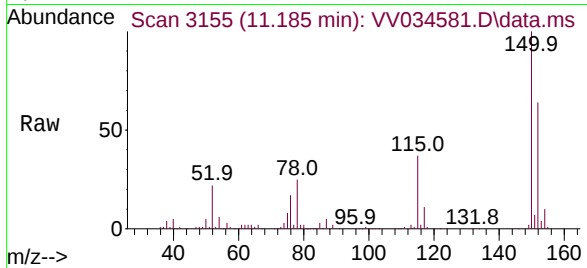

Tgt Ion: 75 Resp: 16671

Ion Ratio Lower Upper

75 100

77 32.9 25.9 38.9

110 2.1 33.1 49.7#

