

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034570.D
 Acq On : 13 Mar 2024 13:17
 Operator : SY/MD
 Sample : P1739-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	134133	141926	12.31%	1.479%
2	1.529	145	152	168	rVB	130201	156701	13.60%	1.632%
3	2.060	307	317	331	rBV2	251656	377539	32.76%	3.933%
4	2.224	361	368	382	rVB2	11100	20347	1.77%	0.212%
5	2.352	406	408	409	rBV2	286	95	0.01%	0.001%
6	2.442	432	436	437	rBV2	977	681	0.06%	0.007%
7	2.558	460	472	485	rBV2	5070	10990	0.95%	0.114%
8	2.806	547	549	555	rVB2	368	236	0.02%	0.002%
9	2.915	580	583	586	rBV2	257	219	0.02%	0.002%
10	3.082	631	635	638	rBV2	196	192	0.02%	0.002%
11	3.240	682	684	686	rVB2	181	70	0.01%	0.001%
12	3.362	720	722	725	rVB	112	51	0.00%	0.001%
13	3.465	751	754	756	rVB2	134	60	0.01%	0.001%
14	3.490	756	762	765	rBV	192	180	0.02%	0.002%
15	3.561	781	784	787	rBV	82	50	0.00%	0.001%
16	3.577	787	789	791	rVB	168	52	0.00%	0.001%
17	3.593	791	794	795	rBV	172	96	0.01%	0.001%
18	3.600	795	796	800	rVV	256	98	0.01%	0.001%
19	3.648	809	811	814	rVB2	108	55	0.00%	0.001%
20	3.667	814	817	818	rBV2	270	190	0.02%	0.002%
21	3.741	834	840	841	rBV2	226	159	0.01%	0.002%
22	3.780	841	852	895	rBV	116905	344340	29.88%	3.587%
23	4.246	982	997	1031	rBV	190865	492080	42.70%	5.126%
24	4.519	1069	1082	1095	rVB6	2837	6556	0.57%	0.068%
25	4.609	1108	1110	1113	rVB2	315	121	0.01%	0.001%
26	4.629	1114	1116	1120	rVB3	304	146	0.01%	0.002%
27	4.706	1135	1140	1143	rBV	519	459	0.04%	0.005%
28	4.844	1178	1183	1186	rBV2	242	288	0.02%	0.003%
29	4.953	1201	1217	1252	rBV2	428565	1152535	100.00%	12.007%
30	5.400	1353	1356	1360	rBV3	166	140	0.01%	0.001%
31	5.420	1360	1362	1363	rBV3	155	57	0.00%	0.001%
32	5.532	1386	1397	1434	rBV	353604	733958	63.68%	7.646%
33	5.834	1478	1491	1524	rBV2	208508	443206	38.45%	4.617%
34	5.986	1526	1538	1566	rBV2	257297	536229	46.53%	5.586%
35	6.281	1628	1630	1635	rBV2	623	515	0.04%	0.005%
36	6.320	1640	1642	1647	rVB2	256	192	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034570.D
 Acq On : 13 Mar 2024 13:17
 Operator : SY/MD
 Sample : P1739-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	6.368	1655	1657	1659	rBV	132	83	0.01%	0.001%
38	6.407	1665	1669	1674	rVB2	201	154	0.01%	0.002%
39	6.439	1675	1679	1682	rBV2	197	195	0.02%	0.002%
40	6.487	1692	1694	1695	rBV	251	80	0.01%	0.001%
41	6.548	1710	1713	1715	rBV2	156	99	0.01%	0.001%
42	6.596	1720	1728	1729	rBV3	865	1123	0.10%	0.012%
43	6.822	1797	1798	1799	rVB3	246	47	0.00%	0.000%
44	6.912	1814	1826	1850	rBV2	129858	247446	21.47%	2.578%
45	7.111	1887	1888	1891	rBV	219	90	0.01%	0.001%
46	7.243	1918	1929	1956	rBV	474673	829296	71.95%	8.639%
47	7.555	2017	2026	2047	rBV	87231	160922	13.96%	1.676%
48	7.748	2084	2086	2090	rVB	315	117	0.01%	0.001%
49	7.776	2093	2095	2097	rBV	443	244	0.02%	0.003%
50	7.818	2106	2108	2114	rVB3	386	353	0.03%	0.004%
51	7.879	2114	2127	2134	rBV2	1109	1992	0.17%	0.021%
52	7.915	2135	2138	2141	rBV2	319	258	0.02%	0.003%
53	8.021	2162	2171	2211	rBV	392680	718514	62.34%	7.485%
54	8.542	2331	2333	2336	rVB3	384	231	0.02%	0.002%
55	8.558	2336	2338	2340	rBV	233	116	0.01%	0.001%
56	8.667	2368	2372	2375	rBV3	225	150	0.01%	0.002%
57	8.696	2378	2381	2387	rVB2	463	406	0.04%	0.004%
58	8.725	2387	2390	2391	rBV	171	106	0.01%	0.001%
59	8.741	2391	2395	2397	rBV3	361	229	0.02%	0.002%
60	8.783	2397	2408	2431	rBV	529236	873539	75.79%	9.100%
61	9.030	2483	2485	2486	rBV	163	60	0.01%	0.001%
62	9.082	2499	2501	2502	rBV	185	64	0.01%	0.001%
63	9.239	2548	2550	2551	rBV	141	47	0.00%	0.000%
64	9.268	2558	2559	2560	rBV	223	49	0.00%	0.001%
65	9.323	2575	2576	2580	rBV2	192	73	0.01%	0.001%
66	9.349	2581	2584	2586	rBV	186	122	0.01%	0.001%
67	9.465	2618	2620	2622	rBV2	130	58	0.01%	0.001%
68	9.484	2622	2626	2630	rBV2	396	254	0.02%	0.003%
69	9.513	2630	2635	2638	rBV2	297	209	0.02%	0.002%
70	9.529	2638	2640	2642	rBV2	158	100	0.01%	0.001%
71	9.657	2677	2680	2682	rBV	299	186	0.02%	0.002%
72	9.815	2727	2729	2730	rBV	211	84	0.01%	0.001%
73	9.976	2775	2779	2782	rBV	171	183	0.02%	0.002%
74	10.030	2791	2796	2797	rBV	136	131	0.01%	0.001%
75	10.037	2797	2798	2799	rVV	194	43	0.00%	0.000%
76	10.153	2822	2834	2858	rBV	387543	612515	53.15%	6.381%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034570.D
 Acq On : 13 Mar 2024 13:17
 Operator : SY/MD
 Sample : P1739-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	10.323	2882	2887	2894	rVB3	1171	1578	0.14%	0.016%
78	10.381	2902	2905	2908	rVB	412	199	0.02%	0.002%
79	10.429	2917	2920	2922	rBV2	173	77	0.01%	0.001%
80	10.497	2937	2941	2945	rBV	410	362	0.03%	0.004%
81	10.516	2945	2947	2953	rVV2	269	268	0.02%	0.003%
82	10.580	2963	2967	2969	rBV	305	207	0.02%	0.002%
83	10.603	2972	2974	2984	rVB2	247	294	0.03%	0.003%
84	10.654	2984	2990	2993	rBV3	265	266	0.02%	0.003%
85	10.683	2997	2999	3001	rBV	202	144	0.01%	0.002%
86	10.715	3006	3009	3011	rBV	189	129	0.01%	0.001%
87	10.808	3036	3038	3042	rVB2	258	107	0.01%	0.001%
88	10.828	3042	3044	3047	rVB2	215	104	0.01%	0.001%
89	10.963	3083	3086	3089	rBV2	230	176	0.02%	0.002%
90	11.130	3133	3138	3143	rVB2	629	780	0.07%	0.008%
91	11.185	3143	3155	3182	rBV	534679	859869	74.61%	8.958%
92	11.480	3244	3247	3250	rBV2	289	159	0.01%	0.002%
93	11.558	3250	3271	3302	rBV	525670	849984	73.75%	8.855%
94	12.120	3444	3446	3449	rVB	349	155	0.01%	0.002%
95	12.696	3623	3625	3627	rBV	342	212	0.02%	0.002%
96	13.017	3723	3725	3727	rBV2	306	144	0.01%	0.002%
97	13.207	3775	3784	3795	rBV7	3639	6173	0.54%	0.064%
98	13.516	3877	3880	3881	rBV2	314	178	0.02%	0.002%
99	13.686	3926	3933	3943	rBV5	3989	6164	0.53%	0.064%
100	13.805	3968	3970	3975	rBV3	633	399	0.03%	0.004%




Sum of corrected areas: 9598905

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034570.D
Acq On : 13 Mar 2024 13:17
Operator : SY/MD
Sample : P1739-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

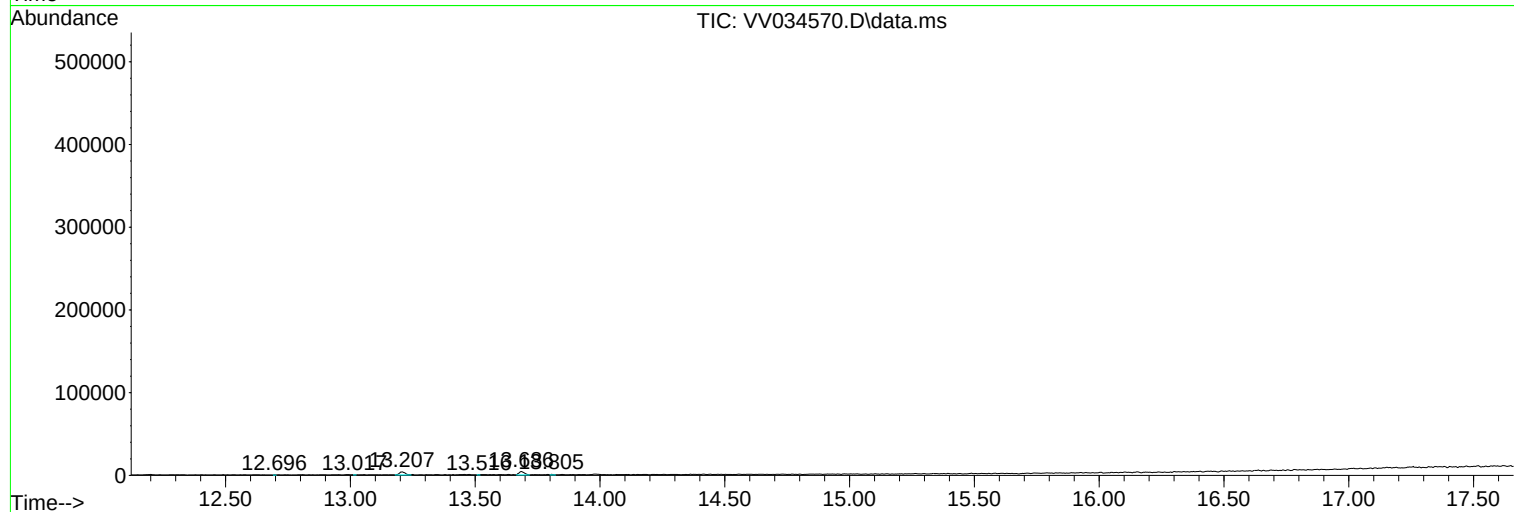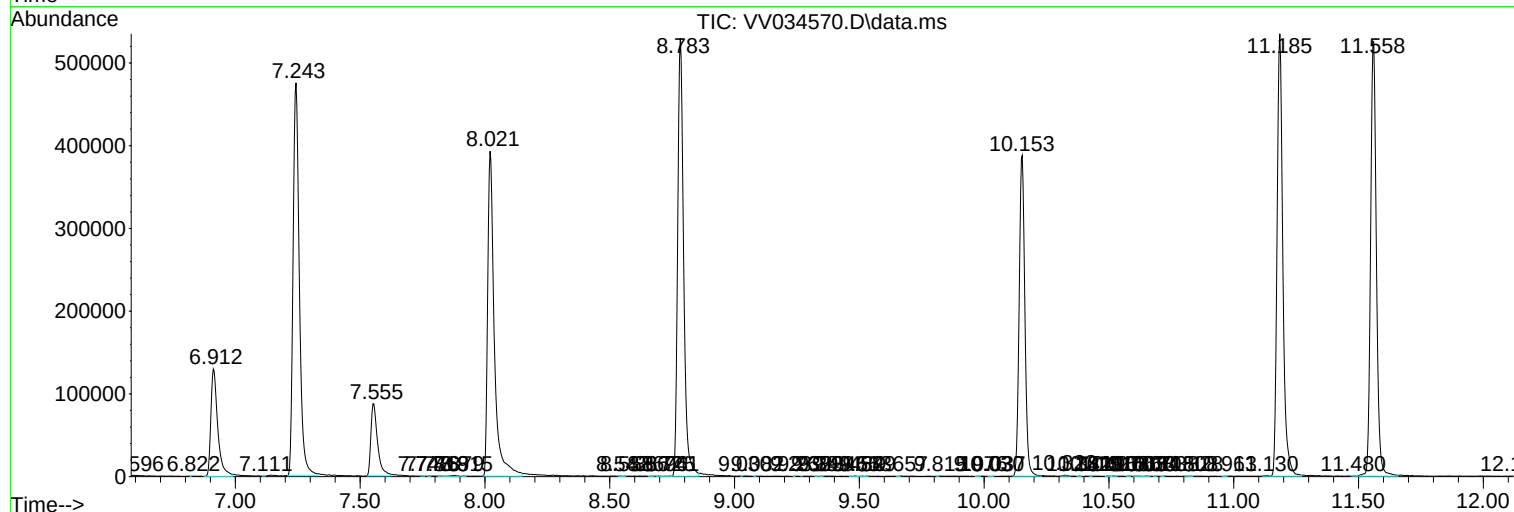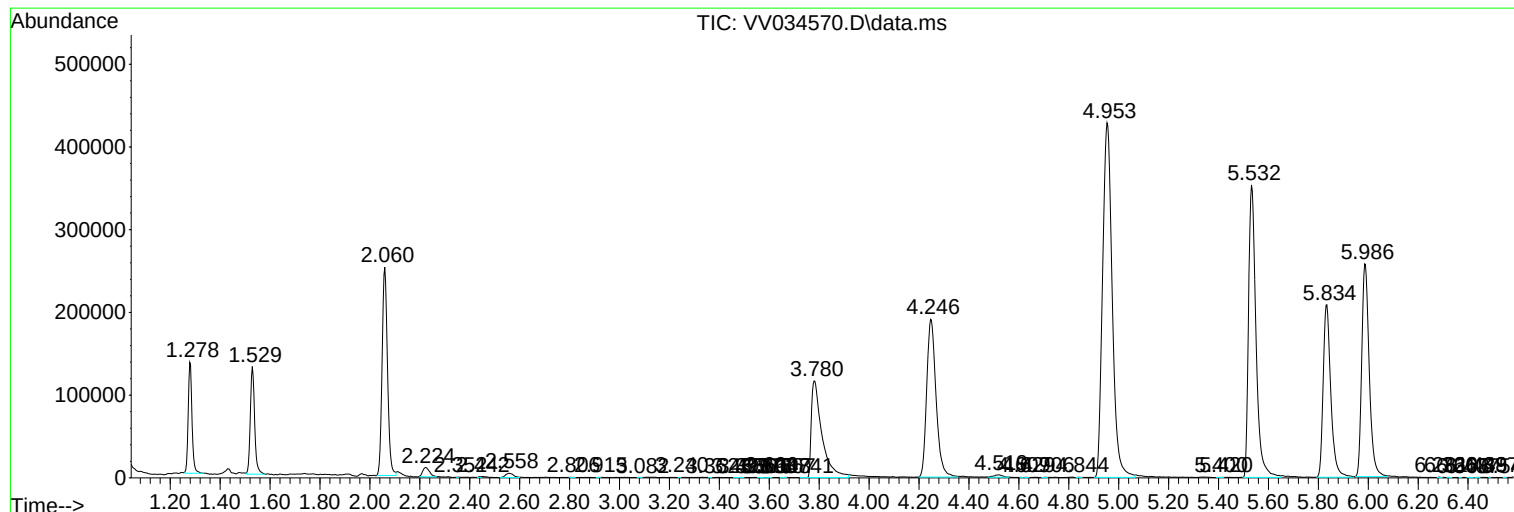

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034570.D
Acq On : 13 Mar 2024 13:17
Operator : SY/MD
Sample : P1739-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034570.D
Acq On : 13 Mar 2024 13:17
Operator : SY/MD
Sample : P1739-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc