

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034573.D
 Acq On : 13 Mar 2024 14:29
 Operator : SY/MD
 Sample : P1739-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

Signal : TIC: VV034573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	86	rBV	129357	132495	11.74%	1.474%
2	1.529	144	152	167	rVB	129307	150138	13.31%	1.671%
3	2.056	306	316	329	rBV	229135	332137	29.44%	3.696%
4	2.233	360	371	388	rBV	10871	22624	2.01%	0.252%
5	2.391	417	420	423	rBV2	403	277	0.02%	0.003%
6	2.429	426	432	434	rVV4	625	587	0.05%	0.007%
7	2.449	434	438	444	rVB3	1530	1676	0.15%	0.019%
8	2.516	456	459	461	rBV2	316	190	0.02%	0.002%
9	2.564	465	474	487	rVV5	1603	3367	0.30%	0.037%
10	2.744	527	530	538	rBV3	243	272	0.02%	0.003%
11	2.828	553	556	561	rVV2	262	225	0.02%	0.003%
12	2.902	572	579	583	rVB2	194	245	0.02%	0.003%
13	2.998	606	609	612	rVB2	299	179	0.02%	0.002%
14	3.249	682	687	690	rBV2	283	261	0.02%	0.003%
15	3.590	788	793	796	rBV2	275	295	0.03%	0.003%
16	3.783	844	853	895	rBV	122784	343177	30.42%	3.819%
17	4.246	981	997	1030	rBV2	186376	483052	42.81%	5.375%
18	4.468	1063	1066	1069	rBV3	338	200	0.02%	0.002%
19	4.686	1127	1134	1135	rBV2	188	215	0.02%	0.002%
20	4.757	1154	1156	1161	rVB2	325	180	0.02%	0.002%
21	4.786	1161	1165	1168	rBB3	209	178	0.02%	0.002%
22	4.953	1202	1217	1251	rBV2	419709	1128268	100.00%	12.555%
23	5.297	1321	1324	1328	rBV	429	247	0.02%	0.003%
24	5.394	1352	1354	1356	rBV2	327	180	0.02%	0.002%
25	5.490	1380	1384	1386	rBV3	275	259	0.02%	0.003%
26	5.532	1386	1397	1430	rBV	352426	731942	64.87%	8.145%
27	5.783	1474	1475	1480	rBV	355	247	0.02%	0.003%
28	5.834	1480	1491	1512	rVV7	15419	38425	3.41%	0.428%
29	5.989	1525	1539	1574	rBV2	253644	534411	47.37%	5.947%
30	6.136	1582	1585	1589	rBV4	847	719	0.06%	0.008%
31	6.153	1589	1590	1594	rVB3	579	295	0.03%	0.003%
32	6.461	1681	1686	1691	rVB2	177	178	0.02%	0.002%
33	6.497	1691	1697	1701	rBV2	163	229	0.02%	0.003%
34	6.577	1718	1722	1723	rBV2	573	384	0.03%	0.004%
35	6.596	1724	1728	1732	rVV4	543	687	0.06%	0.008%
36	6.911	1816	1826	1862	rBV	125906	249261	22.09%	2.774%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034573.D
 Acq On : 13 Mar 2024 14:29
 Operator : SY/MD
 Sample : P1739-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

37	7.136	1891	1896	1898	rBV	890	757	0.07%	0.008%
38	7.243	1918	1929	1957	rBV	457256	806065	71.44%	8.970%
39	7.464	1996	1998	2000	rBV2	369	172	0.02%	0.002%
40	7.554	2016	2026	2050	rBV	90167	164095	14.54%	1.826%
41	7.686	2064	2067	2070	rBB3	393	234	0.02%	0.003%
42	7.834	2109	2113	2117	rVB2	360	275	0.02%	0.003%
43	7.857	2117	2120	2122	rBV	712	471	0.04%	0.005%
44	7.879	2123	2127	2131	rVB2	712	684	0.06%	0.008%
45	8.021	2162	2171	2214	rBV	417430	758179	67.20%	8.437%
46	8.304	2256	2259	2261	rBV2	484	348	0.03%	0.004%
47	8.525	2325	2328	2330	rBV2	286	191	0.02%	0.002%
48	8.583	2343	2346	2348	rBV	284	207	0.02%	0.002%
49	8.651	2363	2367	2370	rBV2	245	173	0.02%	0.002%
50	8.734	2388	2393	2394	rBV2	240	195	0.02%	0.002%
51	8.783	2397	2408	2437	rBV	530903	874424	77.50%	9.730%
52	9.033	2484	2486	2490	rVB	425	212	0.02%	0.002%
53	9.069	2495	2497	2500	rVB2	360	204	0.02%	0.002%
54	9.136	2515	2518	2523	rVB2	256	185	0.02%	0.002%
55	9.233	2540	2548	2553	rBV2	168	306	0.03%	0.003%
56	9.329	2576	2578	2584	rVB3	393	243	0.02%	0.003%
57	9.795	2718	2723	2725	rBV2	304	216	0.02%	0.002%
58	9.963	2769	2775	2778	rBV	181	187	0.02%	0.002%
59	10.043	2797	2800	2806	rVB2	249	293	0.03%	0.003%
60	10.088	2808	2814	2820	rBV2	320	388	0.03%	0.004%
61	10.152	2822	2834	2852	rBV	380524	597554	52.96%	6.650%
62	10.326	2882	2888	2893	rVV2	1291	1479	0.13%	0.016%
63	10.519	2944	2948	2954	rVB2	380	253	0.02%	0.003%
64	10.599	2971	2973	2980	rVB2	223	197	0.02%	0.002%
65	10.750	3015	3020	3023	rBV	212	196	0.02%	0.002%
66	10.795	3030	3034	3038	rBV	232	210	0.02%	0.002%
67	11.107	3127	3131	3133	rBV2	237	215	0.02%	0.002%
68	11.185	3144	3155	3182	rBV	514712	817926	72.49%	9.102%
69	11.358	3207	3209	3211	rBV2	380	217	0.02%	0.002%
70	11.403	3220	3223	3229	rVB4	586	458	0.04%	0.005%
71	11.487	3246	3249	3252	rVV	352	236	0.02%	0.003%
72	11.557	3258	3271	3300	rBV	493395	791362	70.14%	8.806%
73	11.757	3329	3333	3336	rBV2	323	294	0.03%	0.003%
74	11.847	3357	3361	3364	rBV2	288	219	0.02%	0.002%
75	11.905	3375	3379	3383	rBV2	263	272	0.02%	0.003%
76	12.046	3420	3423	3428	rBV	202	178	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
 Data File : VV034573.D
 Acq On : 13 Mar 2024 14:29
 Operator : SY/MD
 Sample : P1739-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
 Title : VOC Analysis

77	12.094	3436	3438	3441	rVB	354	183	0.02%	0.002%
78	12.188	3464	3467	3470	rBV	337	272	0.02%	0.003%
79	12.252	3485	3487	3492	rBV2	248	180	0.02%	0.002%
80	12.831	3662	3667	3671	rBV2	340	323	0.03%	0.004%
81	12.905	3687	3690	3693	rVB	338	178	0.02%	0.002%
82	13.004	3718	3721	3723	rBV	258	181	0.02%	0.002%
83	13.210	3778	3785	3792	rVB4	1283	1745	0.15%	0.019%
84	13.242	3792	3795	3798	rBV4	507	384	0.03%	0.004%
85	13.410	3844	3847	3849	rBV	506	318	0.03%	0.004%
86	13.464	3859	3864	3868	rVV3	560	551	0.05%	0.006%
87	13.487	3868	3871	3875	rVB3	509	393	0.03%	0.004%
88	13.525	3880	3883	3886	rVB2	502	313	0.03%	0.003%
89	13.631	3910	3916	3917	rBV	288	297	0.03%	0.003%
90	13.664	3922	3926	3927	rBV2	237	178	0.02%	0.002%
91	13.680	3929	3931	3935	rBV2	515	391	0.03%	0.004%
92	13.850	3981	3984	3987	rBV3	315	207	0.02%	0.002%
93	13.966	4015	4020	4021	rBV2	685	453	0.04%	0.005%
94	14.159	4078	4080	4081	rBV	372	170	0.02%	0.002%
95	14.274	4113	4116	4120	rBV3	501	417	0.04%	0.005%
96	14.297	4120	4123	4125	rBV2	307	213	0.02%	0.002%
97	14.509	4186	4189	4190	rBV	388	225	0.02%	0.003%
98	14.879	4301	4304	4309	rBV2	582	439	0.04%	0.005%
99	15.294	4431	4433	4436	rBV4	714	489	0.04%	0.005%
100	15.477	4488	4490	4492	rBV4	668	256	0.02%	0.003%




Sum of corrected areas: 8986428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034573.D
Acq On : 13 Mar 2024 14:29
Operator : SY/MD
Sample : P1739-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

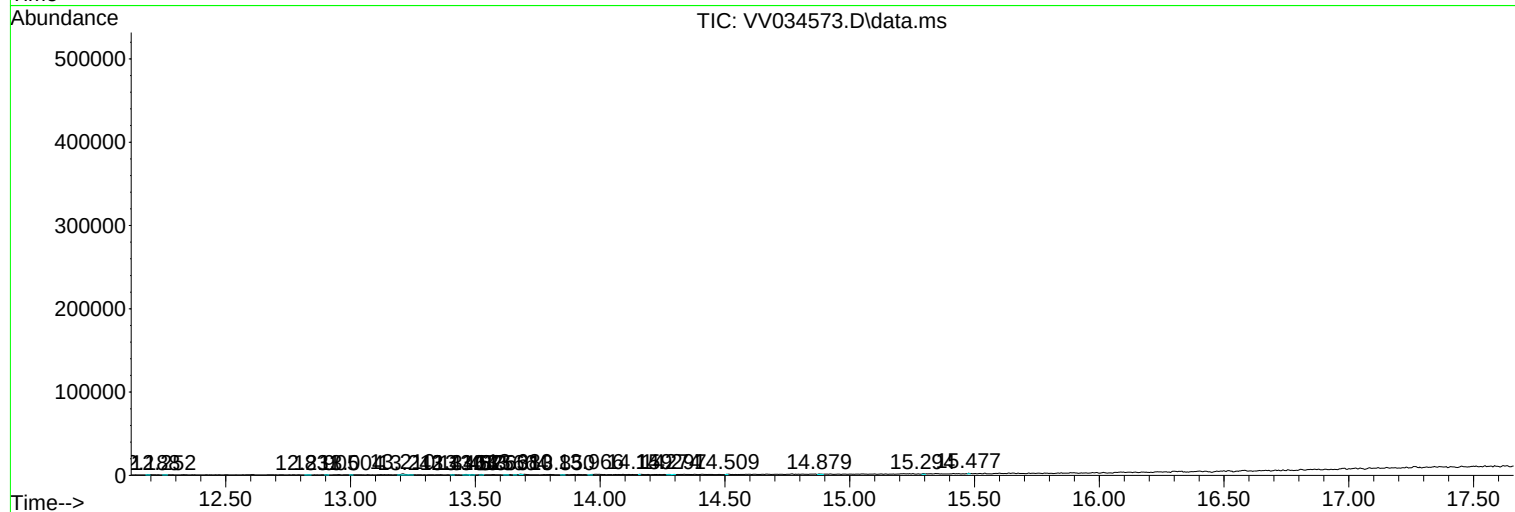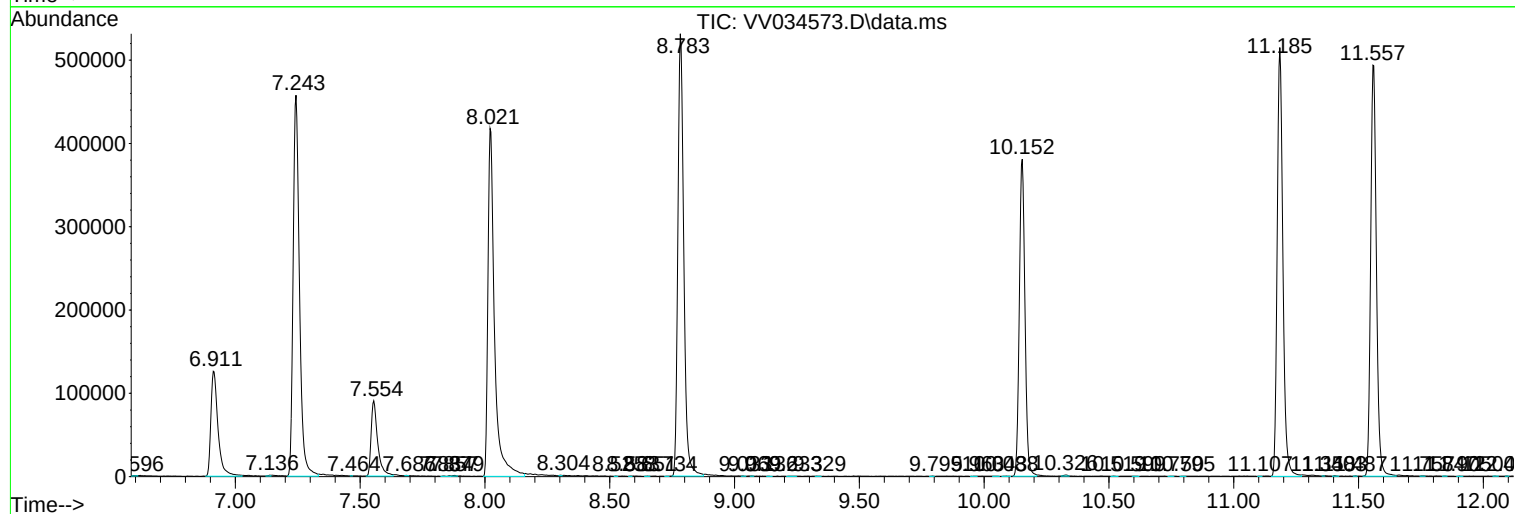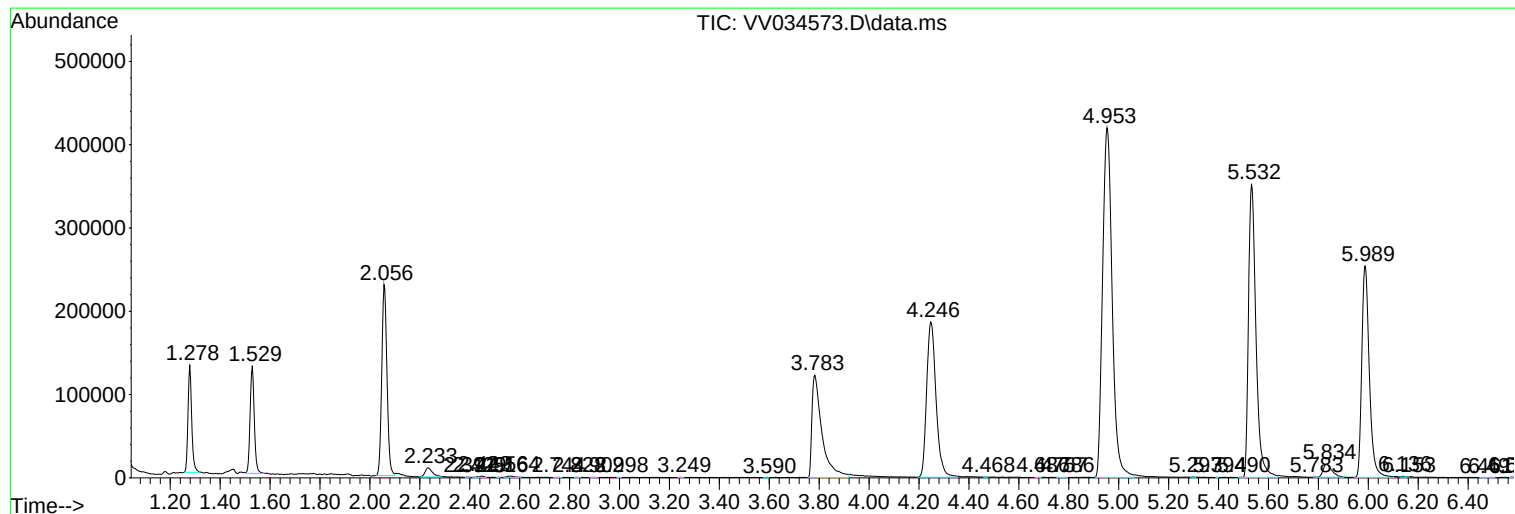

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034573.D
Acq On : 13 Mar 2024 14:29
Operator : SY/MD
Sample : P1739-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV031324\
Data File : VV034573.D
Acq On : 13 Mar 2024 14:29
Operator : SY/MD
Sample : P1739-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM022924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
